

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110122\
 Data File : VV028815.D
 Acq On : 01 Nov 2022 14:50
 Operator : SY/MD
 Sample : N5353-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBWU7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis

Signal : TIC: VV028815.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	76	84	116	rBV2	1307752	1514186	100.00%	12.197%
2	1.564	157	163	177	rVB	168730	200460	13.24%	1.615%
3	2.105	323	331	344	rVB	313201	449073	29.66%	3.617%
4	2.642	496	498	500	rBV3	1704	1069	0.07%	0.009%
5	2.757	524	534	551	rVV	210737	361326	23.86%	2.910%
6	2.960	595	597	600	rBV3	1407	1106	0.07%	0.009%
7	3.015	610	614	618	rBV7	1362	1274	0.08%	0.010%
8	3.063	627	629	630	rBV3	1138	495	0.03%	0.004%
9	3.159	657	659	661	rBV3	1814	1005	0.07%	0.008%
10	3.246	684	686	691	rVB5	1917	1171	0.08%	0.009%
11	3.336	711	714	716	rBV3	1183	975	0.06%	0.008%
12	3.381	725	728	729	rBV3	1420	791	0.05%	0.006%
13	3.490	758	762	763	rBV4	2003	1049	0.07%	0.008%
14	3.529	772	774	777	rBV3	1062	580	0.04%	0.005%
15	3.593	792	794	800	rBV7	1041	891	0.06%	0.007%
16	3.754	842	844	845	rBV2	1197	679	0.04%	0.005%
17	3.815	860	863	867	rVB5	1971	1323	0.09%	0.011%
18	3.841	867	871	872	rBV4	2347	1255	0.08%	0.010%
19	3.902	873	890	918	rBV2	182218	678149	44.79%	5.462%
20	4.227	989	991	992	rBV2	1758	737	0.05%	0.006%
21	4.342	1014	1027	1053	rVB	211558	517065	34.15%	4.165%
22	4.822	1174	1176	1179	rBV4	1115	784	0.05%	0.006%
23	4.838	1179	1181	1185	rVB4	1385	784	0.05%	0.006%
24	4.867	1185	1190	1193	rBV6	1456	1194	0.08%	0.010%
25	5.040	1227	1244	1274	rBV2	517710	1375412	90.84%	11.079%
26	5.516	1390	1392	1395	rBV3	1308	600	0.04%	0.005%
27	5.613	1411	1422	1453	rBV	437319	885334	58.47%	7.131%
28	6.066	1551	1563	1589	rBV	321519	662304	43.74%	5.335%
29	6.738	1770	1772	1773	rBV2	1780	790	0.05%	0.006%
30	6.982	1836	1848	1868	rBV	145909	279494	18.46%	2.251%
31	7.310	1940	1950	1972	rBV	566006	995159	65.72%	8.016%
32	7.619	2036	2046	2068	rBV	93085	176938	11.69%	1.425%
33	8.050	2177	2180	2182	rBV4	2204	1451	0.10%	0.012%
34	8.085	2182	2191	2225	rVV	371462	748415	49.43%	6.028%
35	8.619	2354	2357	2360	rBV4	1686	1229	0.08%	0.010%
36	8.847	2417	2428	2448	rBV	633714	1053048	69.55%	8.482%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110122\
 Data File : VV028815.D
 Acq On : 01 Nov 2022 14:50
 Operator : SY/MD
 Sample : N5353-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBWU7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis

37	9.246	2550	2552	2553	rBV2	1357	567	0.04%	0.005%
38	9.268	2558	2559	2561	rBV2	1564	640	0.04%	0.005%
39	9.394	2595	2598	2601	rVB5	898	671	0.04%	0.005%
40	9.519	2634	2637	2640	rBV4	1890	1560	0.10%	0.013%
41	9.661	2678	2681	2683	rBV4	1831	1225	0.08%	0.010%
42	9.715	2694	2698	2699	rBV5	2163	1275	0.08%	0.010%
43	9.870	2744	2746	2747	rBV2	1280	654	0.04%	0.005%
44	10.059	2803	2805	2808	rVB5	2122	968	0.06%	0.008%
45	10.072	2808	2809	2812	rBV3	910	615	0.04%	0.005%
46	10.095	2814	2816	2818	rBV3	1379	572	0.04%	0.005%
47	10.114	2818	2822	2823	rBV3	1416	976	0.06%	0.008%
48	10.165	2834	2838	2839	rBV3	1189	1039	0.07%	0.008%
49	10.207	2839	2851	2868	rVV	412673	666534	44.02%	5.369%
50	10.683	2997	2999	3003	rBV6	1847	1010	0.07%	0.008%
51	10.735	3013	3015	3017	rBV3	1427	719	0.05%	0.006%
52	10.805	3035	3037	3040	rBV3	1295	566	0.04%	0.005%
53	10.863	3052	3055	3059	rBV6	1307	1162	0.08%	0.009%
54	10.979	3089	3091	3096	rVB5	1310	903	0.06%	0.007%
55	11.017	3098	3103	3105	rBV6	1916	1752	0.12%	0.014%
56	11.117	3129	3134	3137	rVB6	2100	1866	0.12%	0.015%
57	11.149	3140	3144	3147	rBV6	1512	1024	0.07%	0.008%
58	11.175	3147	3152	3156	rVV6	2220	1786	0.12%	0.014%
59	11.243	3162	3173	3194	rBV	570483	913656	60.34%	7.359%
60	11.400	3220	3222	3227	rBV6	1354	1199	0.08%	0.010%
61	11.435	3231	3233	3235	rBV3	1808	794	0.05%	0.006%
62	11.484	3246	3248	3250	rVB2	1824	713	0.05%	0.006%
63	11.616	3278	3289	3309	rBV	527037	854025	56.40%	6.879%
64	11.786	3340	3342	3346	rBV4	1875	1467	0.10%	0.012%
65	12.162	3457	3459	3463	rBV5	1177	607	0.04%	0.005%
66	12.226	3475	3479	3481	rBV4	2111	1626	0.11%	0.013%
67	12.271	3489	3493	3494	rBV4	1398	784	0.05%	0.006%
68	12.288	3494	3498	3504	rVB7	1629	1819	0.12%	0.015%
69	12.387	3527	3529	3530	rBV2	1629	594	0.04%	0.005%
70	12.426	3535	3541	3545	rBV9	1495	1945	0.13%	0.016%
71	12.464	3551	3553	3555	rVB3	1842	597	0.04%	0.005%
72	12.477	3555	3557	3558	rBV2	1283	548	0.04%	0.004%
73	12.593	3589	3593	3594	rBV4	1365	912	0.06%	0.007%
74	12.677	3615	3619	3620	rBV4	1386	963	0.06%	0.008%
75	12.844	3669	3671	3674	rBV4	1280	781	0.05%	0.006%
76	12.886	3677	3684	3685	rBV7	1618	1508	0.10%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110122\
 Data File : VV028815.D
 Acq On : 01 Nov 2022 14:50
 Operator : SY/MD
 Sample : N5353-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBWU7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis

77	13.014	3721	3724	3726	rBV3	1997	1117	0.07%	0.009%
78	13.175	3768	3774	3777	rBV8	1937	2071	0.14%	0.017%
79	13.249	3795	3797	3798	rBV2	1237	492	0.03%	0.004%
80	13.300	3810	3813	3815	rVB3	1181	554	0.04%	0.004%
81	13.316	3815	3818	3819	rBV3	1507	889	0.06%	0.007%
82	13.397	3840	3843	3846	rVB3	1869	1145	0.08%	0.009%
83	13.413	3846	3848	3850	rBV2	1103	712	0.05%	0.006%
84	13.519	3878	3881	3882	rBV2	1068	550	0.04%	0.004%
85	13.699	3934	3937	3938	rBV3	1735	764	0.05%	0.006%
86	13.763	3952	3957	3960	rBV6	1837	1671	0.11%	0.013%
87	13.834	3975	3979	3981	rBV5	1210	927	0.06%	0.007%
88	13.886	3992	3995	3997	rBV4	1846	1016	0.07%	0.008%
89	13.963	4016	4019	4023	rBV5	1426	998	0.07%	0.008%
90	14.017	4034	4036	4040	rBV5	1602	1251	0.08%	0.010%
91	14.223	4097	4100	4105	rBV7	1385	1399	0.09%	0.011%
92	14.291	4119	4121	4124	rVB4	1879	748	0.05%	0.006%
93	14.371	4143	4146	4147	rBV3	1443	758	0.05%	0.006%
94	14.384	4148	4150	4153	rVB4	1977	892	0.06%	0.007%
95	14.458	4168	4173	4174	rBV5	1386	1089	0.07%	0.009%
96	14.606	4217	4219	4221	rBV3	1660	891	0.06%	0.007%
97	14.930	4318	4320	4322	rBV3	1939	939	0.06%	0.008%
98	15.001	4340	4342	4345	rBV4	2146	1508	0.10%	0.012%
99	15.184	4396	4399	4402	rBV5	1916	1294	0.09%	0.010%
100	15.210	4405	4407	4408	rBV2	1876	910	0.06%	0.007%




Sum of corrected areas: 12414802

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110122\
Data File : VV028815.D
Acq On : 01 Nov 2022 14:50
Operator : SY/MD
Sample : N5353-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBWU7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

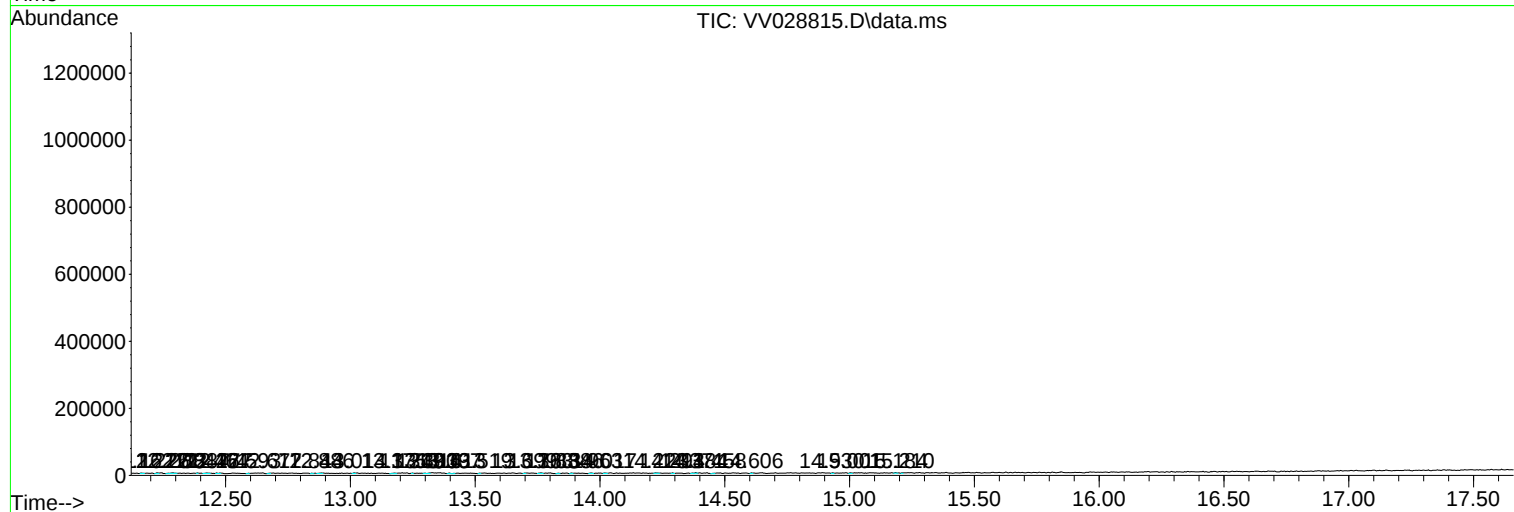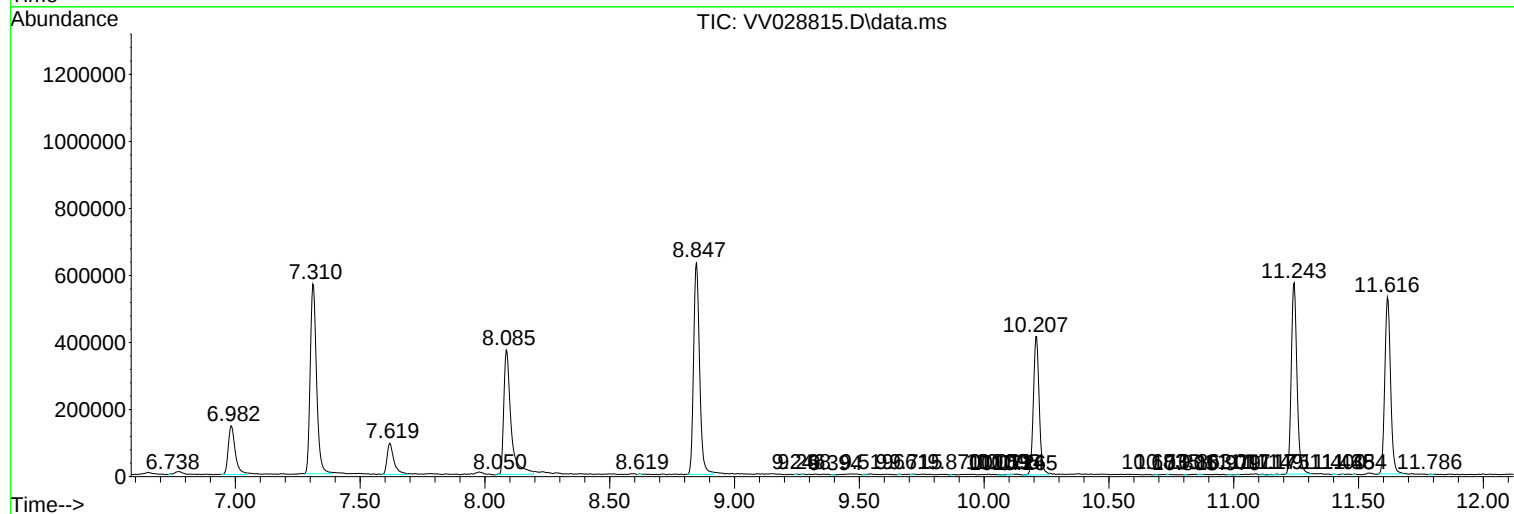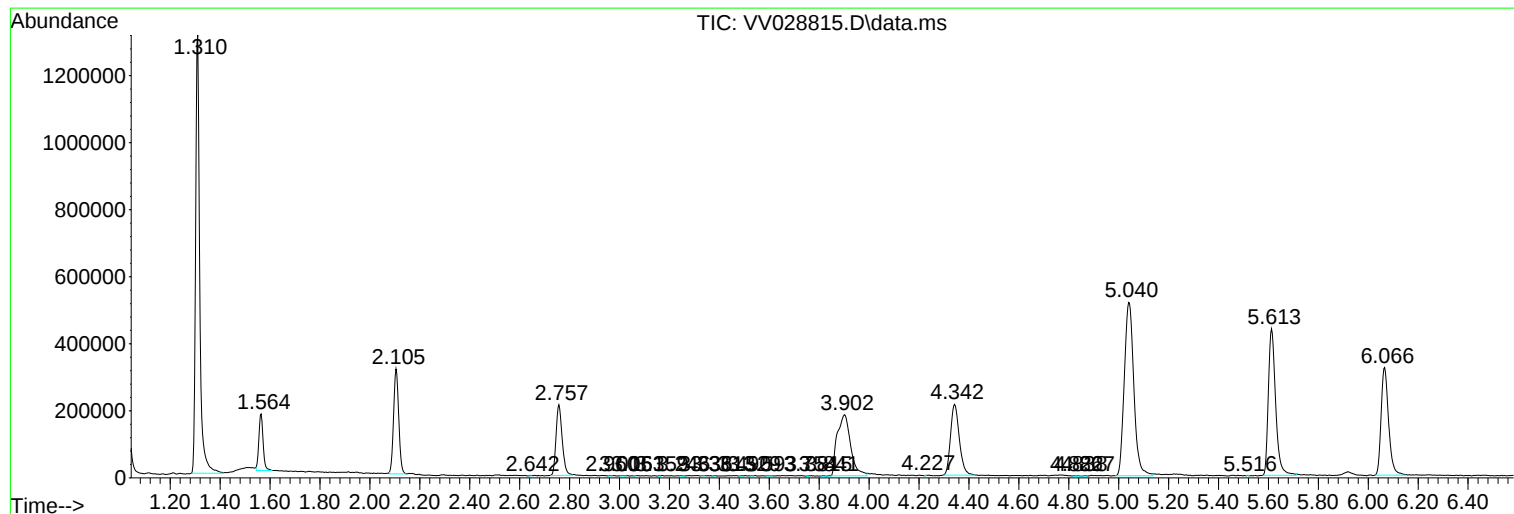

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110122\
Data File : VV028815.D
Acq On : 01 Nov 2022 14:50
Operator : SY/MD
Sample : N5353-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBWU7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110122\
Data File : VV028815.D
Acq On : 01 Nov 2022 14:50
Operator : SY/MD
Sample : N5353-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBWU7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc