

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110122\
 Data File : VV028817.D
 Acq On : 01 Nov 2022 15:39
 Operator : SY/MD
 Sample : N5353-12DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBVV2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis

Signal : TIC: VV028817.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	102	rBV	247184	274458	14.29%	1.785%
2	1.561	156	162	174	rVB	242756	282016	14.69%	1.834%
3	2.105	322	331	345	rVB	468303	669580	34.87%	4.355%
4	2.555	469	471	478	rVB7	2491	2256	0.12%	0.015%
5	2.580	478	479	480	rBV	1152	430	0.02%	0.003%
6	2.696	511	515	518	rBV5	1220	1151	0.06%	0.007%
7	2.761	521	535	548	rBV2	43655	82494	4.30%	0.537%
8	2.912	581	582	586	rBV4	1345	702	0.04%	0.005%
9	2.950	592	594	597	rVB3	1894	987	0.05%	0.006%
10	2.982	600	604	605	rBV3	1331	1016	0.05%	0.007%
11	3.082	632	635	638	rBV5	1473	1232	0.06%	0.008%
12	3.182	663	666	669	rBV5	1545	1075	0.06%	0.007%
13	3.217	674	677	680	rVV5	1193	570	0.03%	0.004%
14	3.233	680	682	685	rVV4	1370	855	0.04%	0.006%
15	3.262	689	691	694	rVB4	1626	722	0.04%	0.005%
16	3.281	694	697	698	rBV4	871	470	0.02%	0.003%
17	3.352	714	719	720	rBV5	1281	884	0.05%	0.006%
18	3.362	720	722	724	rBV3	1295	623	0.03%	0.004%
19	3.416	737	739	742	rBV4	2171	1293	0.07%	0.008%
20	3.526	771	773	776	rVB4	1753	846	0.04%	0.006%
21	3.542	776	778	779	rBV2	1284	471	0.02%	0.003%
22	3.551	779	781	785	rBV5	1789	1491	0.08%	0.010%
23	3.600	795	796	801	rVB5	1433	796	0.04%	0.005%
24	3.693	823	825	827	rBV3	1459	858	0.04%	0.006%
25	3.728	834	836	839	rBV4	1286	1025	0.05%	0.007%
26	3.744	839	841	843	rVV4	1502	737	0.04%	0.005%
27	3.764	845	847	849	rVV3	1020	600	0.03%	0.004%
28	3.799	853	858	859	rBV5	1318	977	0.05%	0.006%
29	3.873	871	881	922	rBV3	194508	812641	42.33%	5.285%
30	4.342	1012	1027	1058	rVB2	290307	726632	37.85%	4.726%
31	4.924	1205	1208	1209	rBV2	1694	996	0.05%	0.006%
32	5.040	1226	1244	1273	rBV2	734163	1919966	100.00%	12.487%
33	5.613	1410	1422	1447	rBV	596596	1195131	62.25%	7.773%
34	5.912	1504	1515	1542	rVB	322131	640515	33.36%	4.166%
35	6.063	1551	1562	1586	rVB	442898	893064	46.51%	5.808%
36	6.503	1698	1699	1702	rBV3	1232	871	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110122\
 Data File : VV028817.D
 Acq On : 01 Nov 2022 15:39
 Operator : SY/MD
 Sample : N5353-12DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBVV2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis

37	6.889	1816	1819	1821	rBV4	1825	1182	0.06%	0.008%
38	6.982	1837	1848	1876	rBV2	206808	383169	19.96%	2.492%
39	7.310	1939	1950	1978	rBV	809545	1410627	73.47%	9.174%
40	7.616	2037	2045	2064	rBV	130595	229999	11.98%	1.496%
41	8.085	2181	2191	2235	rBV	554921	1079316	56.22%	7.020%
42	8.847	2416	2428	2450	rBV	858210	1422254	74.08%	9.250%
43	9.230	2545	2547	2550	rBV4	1330	789	0.04%	0.005%
44	9.345	2580	2583	2586	rBV5	1787	1403	0.07%	0.009%
45	9.468	2619	2621	2622	rBV3	1134	474	0.02%	0.003%
46	9.561	2646	2650	2653	rBV4	1927	1931	0.10%	0.013%
47	9.706	2692	2695	2698	rBV5	1284	900	0.05%	0.006%
48	9.831	2731	2734	2736	rBV4	1577	986	0.05%	0.006%
49	9.895	2752	2754	2756	rBV3	1096	591	0.03%	0.004%
50	9.995	2783	2785	2786	rBV2	1396	539	0.03%	0.004%
51	10.111	2818	2821	2824	rBV5	1328	809	0.04%	0.005%
52	10.127	2824	2826	2832	rVB7	1862	1426	0.07%	0.009%
53	10.156	2832	2835	2837	rBV4	1217	689	0.04%	0.004%
54	10.207	2837	2851	2867	rBV	559806	892223	46.47%	5.803%
55	10.410	2913	2914	2919	rVB4	2255	1192	0.06%	0.008%
56	10.429	2919	2920	2921	rBV	1441	515	0.03%	0.003%
57	10.551	2956	2958	2960	rVB3	1534	545	0.03%	0.004%
58	10.622	2977	2980	2983	rBV5	1294	979	0.05%	0.006%
59	10.654	2987	2990	2994	rBV6	1595	1331	0.07%	0.009%
60	10.763	3018	3024	3026	rBV7	1895	1420	0.07%	0.009%
61	10.825	3041	3043	3046	rBV4	2333	1459	0.08%	0.009%
62	11.124	3132	3136	3139	rBV6	1473	1351	0.07%	0.009%
63	11.239	3162	3172	3193	rBV	785764	1225806	63.85%	7.972%
64	11.561	3270	3272	3275	rBV4	1610	993	0.05%	0.006%
65	11.615	3278	3289	3307	rVV	727016	1157228	60.27%	7.526%
66	12.191	3465	3468	3470	rBV4	2519	1433	0.07%	0.009%
67	12.249	3485	3486	3489	rVB3	1328	565	0.03%	0.004%
68	12.271	3492	3493	3497	rVB3	1117	641	0.03%	0.004%
69	12.294	3497	3500	3501	rBV3	1129	618	0.03%	0.004%
70	12.310	3501	3505	3508	rVB5	1204	1025	0.05%	0.007%
71	12.326	3508	3510	3511	rBV2	1828	812	0.04%	0.005%
72	12.349	3514	3517	3519	rBV4	985	577	0.03%	0.004%
73	12.496	3560	3563	3564	rBV3	2045	1066	0.06%	0.007%
74	12.628	3602	3604	3607	rBV3	1095	700	0.04%	0.005%
75	12.660	3611	3614	3616	rBV3	1361	796	0.04%	0.005%
76	12.673	3616	3618	3620	rVB3	1326	619	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110122\
 Data File : VV028817.D
 Acq On : 01 Nov 2022 15:39
 Operator : SY/MD
 Sample : N5353-12DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBVV2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis

77	12.734	3633	3637	3641	rVB7	1784	1696	0.09%	0.011%
78	12.760	3643	3645	3649	rVV5	1373	694	0.04%	0.005%
79	12.792	3653	3655	3660	rBV5	1500	1184	0.06%	0.008%
80	12.876	3677	3681	3683	rBV5	2315	1800	0.09%	0.012%
81	13.091	3746	3748	3752	rVB4	1890	1288	0.07%	0.008%
82	13.152	3765	3767	3768	rBV2	1183	466	0.02%	0.003%
83	13.194	3778	3780	3784	rVB4	2232	1317	0.07%	0.009%
84	13.220	3786	3788	3790	rVB3	1610	669	0.03%	0.004%
85	13.236	3790	3793	3795	rBV4	1632	1066	0.06%	0.007%
86	13.268	3801	3803	3808	rVB6	1354	890	0.05%	0.006%
87	13.307	3813	3815	3818	rBV3	1376	726	0.04%	0.005%
88	13.368	3831	3834	3837	rBV5	1495	976	0.05%	0.006%
89	13.496	3872	3874	3876	rBV3	1676	817	0.04%	0.005%
90	13.641	3916	3919	3921	rBV4	1436	1032	0.05%	0.007%
91	13.741	3948	3950	3952	rBV3	985	560	0.03%	0.004%
92	13.795	3965	3967	3969	rBV3	1060	655	0.03%	0.004%
93	13.882	3991	3994	3995	rBV3	1582	697	0.04%	0.005%
94	13.947	4010	4014	4016	rBV5	1171	860	0.04%	0.006%
95	14.078	4053	4055	4058	rBV3	1502	873	0.05%	0.006%
96	14.358	4140	4142	4146	rBV5	1490	1028	0.05%	0.007%
97	14.451	4168	4171	4175	rBV6	1368	1345	0.07%	0.009%
98	14.557	4199	4204	4207	rBV7	1667	1734	0.09%	0.011%
99	15.088	4367	4369	4371	rBV3	1593	824	0.04%	0.005%
100	15.255	4418	4421	4423	rBV4	2151	1328	0.07%	0.009%




Sum of corrected areas: 15375934

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110122\
Data File : VV028817.D
Acq On : 01 Nov 2022 15:39
Operator : SY/MD
Sample : N5353-12DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBVV2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

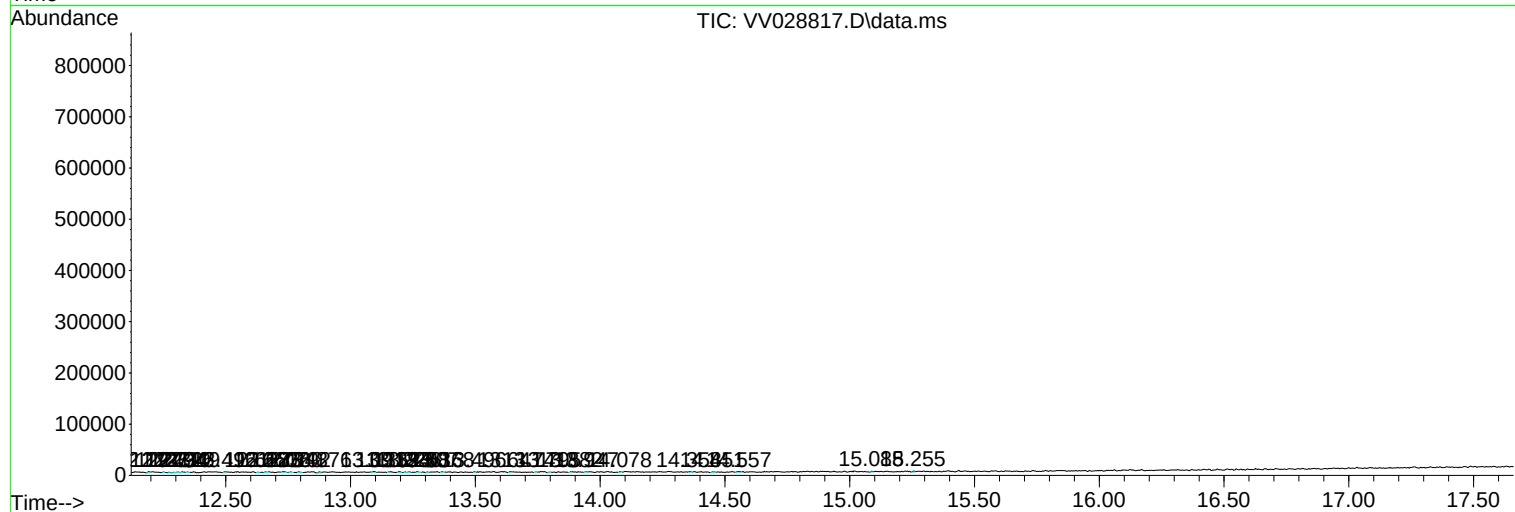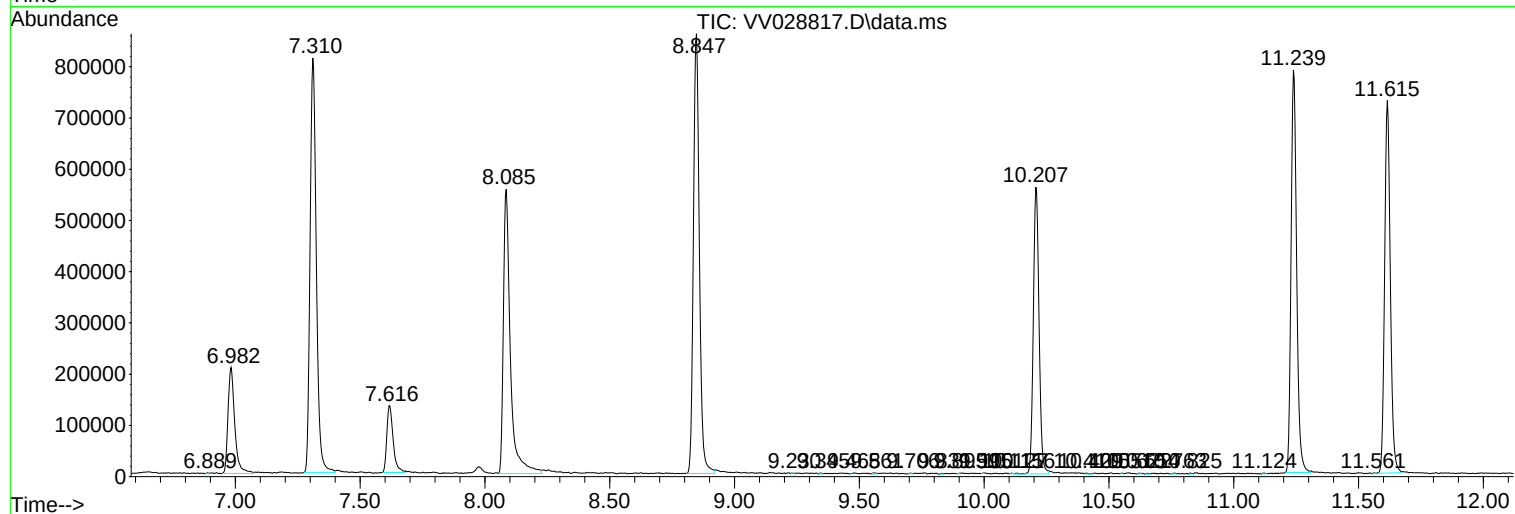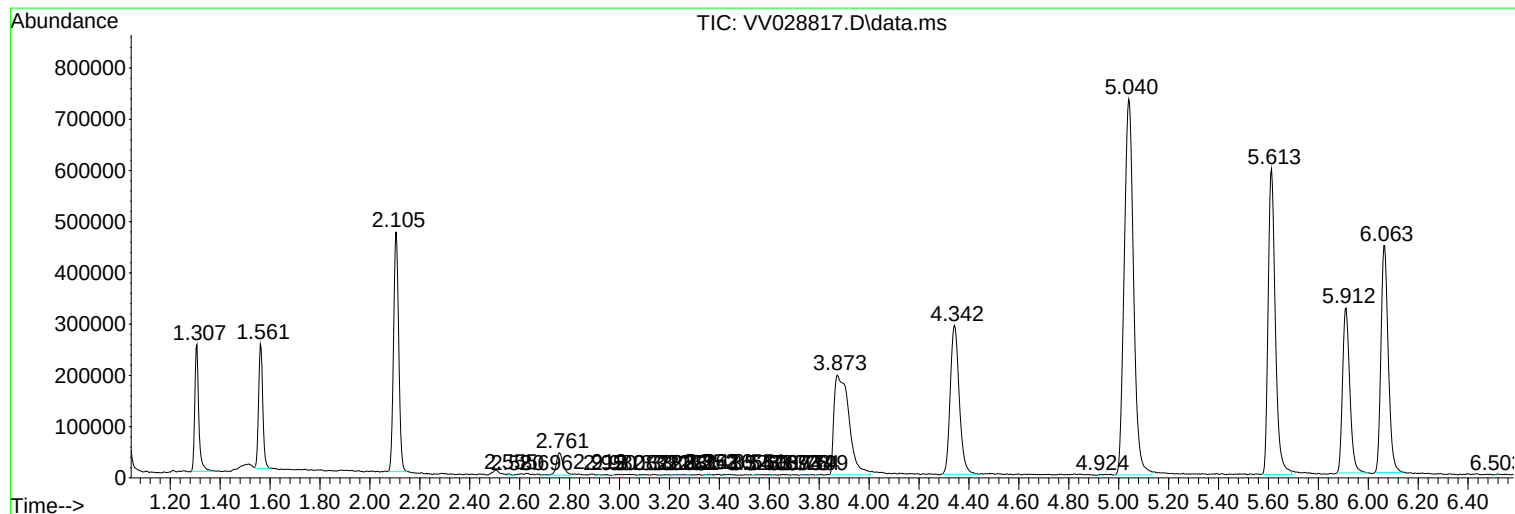

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110122\
Data File : VV028817.D
Acq On : 01 Nov 2022 15:39
Operator : SY/MD
Sample : N5353-12DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBVV2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110122\
Data File : VV028817.D
Acq On : 01 Nov 2022 15:39
Operator : SY/MD
Sample : N5353-12DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBVV2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------