

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110122\
 Data File : VV028818.D
 Acq On : 01 Nov 2022 16:27
 Operator : SY/MD
 Sample : N5321-12DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBWN6DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis

Signal : TIC: VV028818.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	102	rVB	182326	210110	13.18%	1.552%
2	1.561	156	162	178	rVB	190441	222620	13.96%	1.645%
3	2.105	322	331	344	rVB	359961	512258	32.13%	3.785%
4	2.757	525	534	552	rBV	114061	197158	12.36%	1.457%
5	2.915	582	583	585	rBV3	1436	668	0.04%	0.005%
6	2.941	588	591	593	rBV4	1954	1269	0.08%	0.009%
7	2.995	604	608	610	rBV4	1409	1157	0.07%	0.009%
8	3.102	639	641	643	rBV3	1137	583	0.04%	0.004%
9	3.192	665	669	673	rVV7	1715	1476	0.09%	0.011%
10	3.224	677	679	682	rBV4	829	506	0.03%	0.004%
11	3.265	691	692	694	rBV2	1538	826	0.05%	0.006%
12	3.278	694	696	698	rVB3	1493	658	0.04%	0.005%
13	3.323	707	710	712	rBV4	1169	659	0.04%	0.005%
14	3.352	716	719	723	rVB5	1387	727	0.05%	0.005%
15	3.378	725	727	729	rBV4	1100	590	0.04%	0.004%
16	3.442	743	747	749	rBV5	1741	1415	0.09%	0.010%
17	3.458	749	752	756	rVB4	1939	1318	0.08%	0.010%
18	3.516	766	770	771	rBV4	1619	881	0.06%	0.007%
19	3.712	828	831	832	rBV3	2344	1230	0.08%	0.009%
20	3.902	870	890	926	rBV2	315442	1115935	69.99%	8.245%
21	4.343	1013	1027	1047	rBV	245885	604549	37.91%	4.467%
22	4.748	1152	1153	1156	rVB3	1406	514	0.03%	0.004%
23	4.767	1156	1159	1161	rBV4	1544	940	0.06%	0.007%
24	4.870	1189	1191	1193	rVB3	1403	604	0.04%	0.004%
25	4.966	1217	1221	1223	rBV4	1875	1485	0.09%	0.011%
26	5.040	1228	1244	1272	rBV2	606226	1594516	100.00%	11.782%
27	5.391	1349	1353	1355	rBV5	1680	1578	0.10%	0.012%
28	5.452	1369	1372	1373	rBV3	1745	993	0.06%	0.007%
29	5.613	1408	1422	1452	rBV	519674	1056318	66.25%	7.805%
30	5.863	1498	1500	1502	rBV3	2601	979	0.06%	0.007%
31	5.912	1502	1515	1538	rBV	165584	339685	21.30%	2.510%
32	6.066	1551	1563	1591	rVB	378410	768002	48.17%	5.675%
33	6.925	1825	1830	1835	rBV8	2368	2255	0.14%	0.017%
34	6.982	1839	1848	1869	rVV	176730	323473	20.29%	2.390%
35	7.310	1939	1950	1973	rBV	673455	1182898	74.19%	8.740%
36	7.619	2035	2046	2075	rBV	111012	208591	13.08%	1.541%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110122\
 Data File : VV028818.D
 Acq On : 01 Nov 2022 16:27
 Operator : SY/MD
 Sample : N5321-12DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBWN6DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis

37	8.040	2175	2177	2179	rBV3	1031	582	0.04%	0.004%
38	8.085	2179	2191	2230	rBV	479448	959354	60.17%	7.089%
39	8.613	2351	2355	2360	rBV8	2410	2431	0.15%	0.018%
40	8.696	2379	2381	2385	rVB4	1871	973	0.06%	0.007%
41	8.748	2393	2397	2399	rBV5	2115	1624	0.10%	0.012%
42	8.847	2416	2428	2459	rBV	749572	1243314	77.97%	9.187%
43	9.243	2549	2551	2553	rBV3	1029	504	0.03%	0.004%
44	9.445	2609	2614	2616	rBV5	1828	1332	0.08%	0.010%
45	9.458	2616	2618	2621	rBV4	2061	1118	0.07%	0.008%
46	9.719	2693	2699	2702	rBV7	1805	2099	0.13%	0.016%
47	9.809	2721	2727	2728	rBV5	2050	1628	0.10%	0.012%
48	9.928	2757	2764	2768	rBV7	4362	6528	0.41%	0.048%
49	10.059	2800	2805	2808	rBV6	1863	1464	0.09%	0.011%
50	10.162	2834	2837	2838	rBV3	2259	845	0.05%	0.006%
51	10.207	2841	2851	2877	rVB	479954	782899	49.10%	5.785%
52	10.304	2877	2881	2883	rBV5	2043	1701	0.11%	0.013%
53	10.352	2893	2896	2897	rBV3	1288	731	0.05%	0.005%
54	10.535	2949	2953	2957	rBV5	2980	2839	0.18%	0.021%
55	10.593	2969	2971	2974	rVB4	1908	999	0.06%	0.007%
56	10.728	3010	3013	3018	rBV6	918	981	0.06%	0.007%
57	10.780	3024	3029	3033	rBV5	1732	1527	0.10%	0.011%
58	10.982	3088	3092	3093	rBV4	936	518	0.03%	0.004%
59	11.034	3104	3108	3110	rBV6	1916	1170	0.07%	0.009%
60	11.050	3111	3113	3116	rVB3	2407	1147	0.07%	0.008%
61	11.072	3116	3120	3123	rBV5	1517	1380	0.09%	0.010%
62	11.137	3137	3140	3142	rBV4	1407	869	0.05%	0.006%
63	11.185	3147	3155	3161	rVV10	5240	8048	0.50%	0.059%
64	11.239	3161	3172	3197	rVV	670338	1079782	67.72%	7.978%
65	11.529	3260	3262	3263	rBV3	1647	723	0.05%	0.005%
66	11.616	3278	3289	3314	rBV	628080	1001916	62.84%	7.403%
67	11.764	3330	3335	3338	rBV7	1948	1898	0.12%	0.014%
68	11.876	3368	3370	3375	rVB5	1868	1223	0.08%	0.009%
69	12.005	3404	3410	3415	rVB9	2561	2322	0.15%	0.017%
70	12.030	3415	3418	3423	rVB6	2149	1370	0.09%	0.010%
71	12.085	3431	3435	3437	rVB5	1229	885	0.06%	0.007%
72	12.101	3437	3440	3441	rBV3	1461	795	0.05%	0.006%
73	12.185	3463	3466	3468	rBV4	1118	813	0.05%	0.006%
74	12.230	3475	3480	3482	rVB5	1402	1122	0.07%	0.008%
75	12.243	3482	3484	3490	rBV7	1687	1340	0.08%	0.010%
76	12.275	3493	3494	3499	rBV5	1654	1377	0.09%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110122\
 Data File : VV028818.D
 Acq On : 01 Nov 2022 16:27
 Operator : SY/MD
 Sample : N5321-12DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBWN6DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis

77	12.481	3556	3558	3561	rBV4	1172	588	0.04%	0.004%
78	12.535	3572	3575	3577	rBV4	1789	1038	0.07%	0.008%
79	12.558	3579	3582	3584	rVV4	1928	999	0.06%	0.007%
80	12.600	3593	3595	3598	rBV3	1458	716	0.04%	0.005%
81	12.638	3602	3607	3619	rVB3	8693	14350	0.90%	0.106%
82	12.821	3659	3664	3665	rBV4	1824	1561	0.10%	0.012%
83	12.889	3683	3685	3690	rBV5	1247	904	0.06%	0.007%
84	12.960	3704	3707	3711	rBV6	1400	1288	0.08%	0.010%
85	13.001	3717	3720	3721	rBV3	1343	800	0.05%	0.006%
86	13.101	3749	3751	3752	rBV2	1246	611	0.04%	0.005%
87	13.165	3769	3771	3774	rBV4	1220	813	0.05%	0.006%
88	13.204	3780	3783	3785	rVB3	1431	772	0.05%	0.006%
89	13.255	3793	3799	3809	rBV10	8523	12959	0.81%	0.096%
90	13.352	3827	3829	3832	rBV2	1086	636	0.04%	0.005%
91	13.432	3851	3854	3855	rBV3	1654	895	0.06%	0.007%
92	13.853	3984	3985	3988	rVB3	1419	529	0.03%	0.004%
93	13.905	3997	4001	4004	rBV6	1971	1533	0.10%	0.011%
94	13.927	4006	4008	4011	rVB4	2525	1099	0.07%	0.008%
95	13.956	4011	4017	4020	rBV8	2282	2598	0.16%	0.019%
96	14.149	4075	4077	4079	rVB3	1954	825	0.05%	0.006%
97	14.165	4079	4082	4083	rBV2	1516	966	0.06%	0.007%
98	14.207	4093	4095	4099	rVB4	1296	802	0.05%	0.006%
99	14.291	4117	4121	4123	rBV6	2342	2052	0.13%	0.015%
100	14.323	4129	4131	4133	rBV3	1534	1018	0.06%	0.008%


Sum of corrected areas: 13533947

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110122\
Data File : VV028818.D
Acq On : 01 Nov 2022 16:27
Operator : SY/MD
Sample : N5321-12DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBWN6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

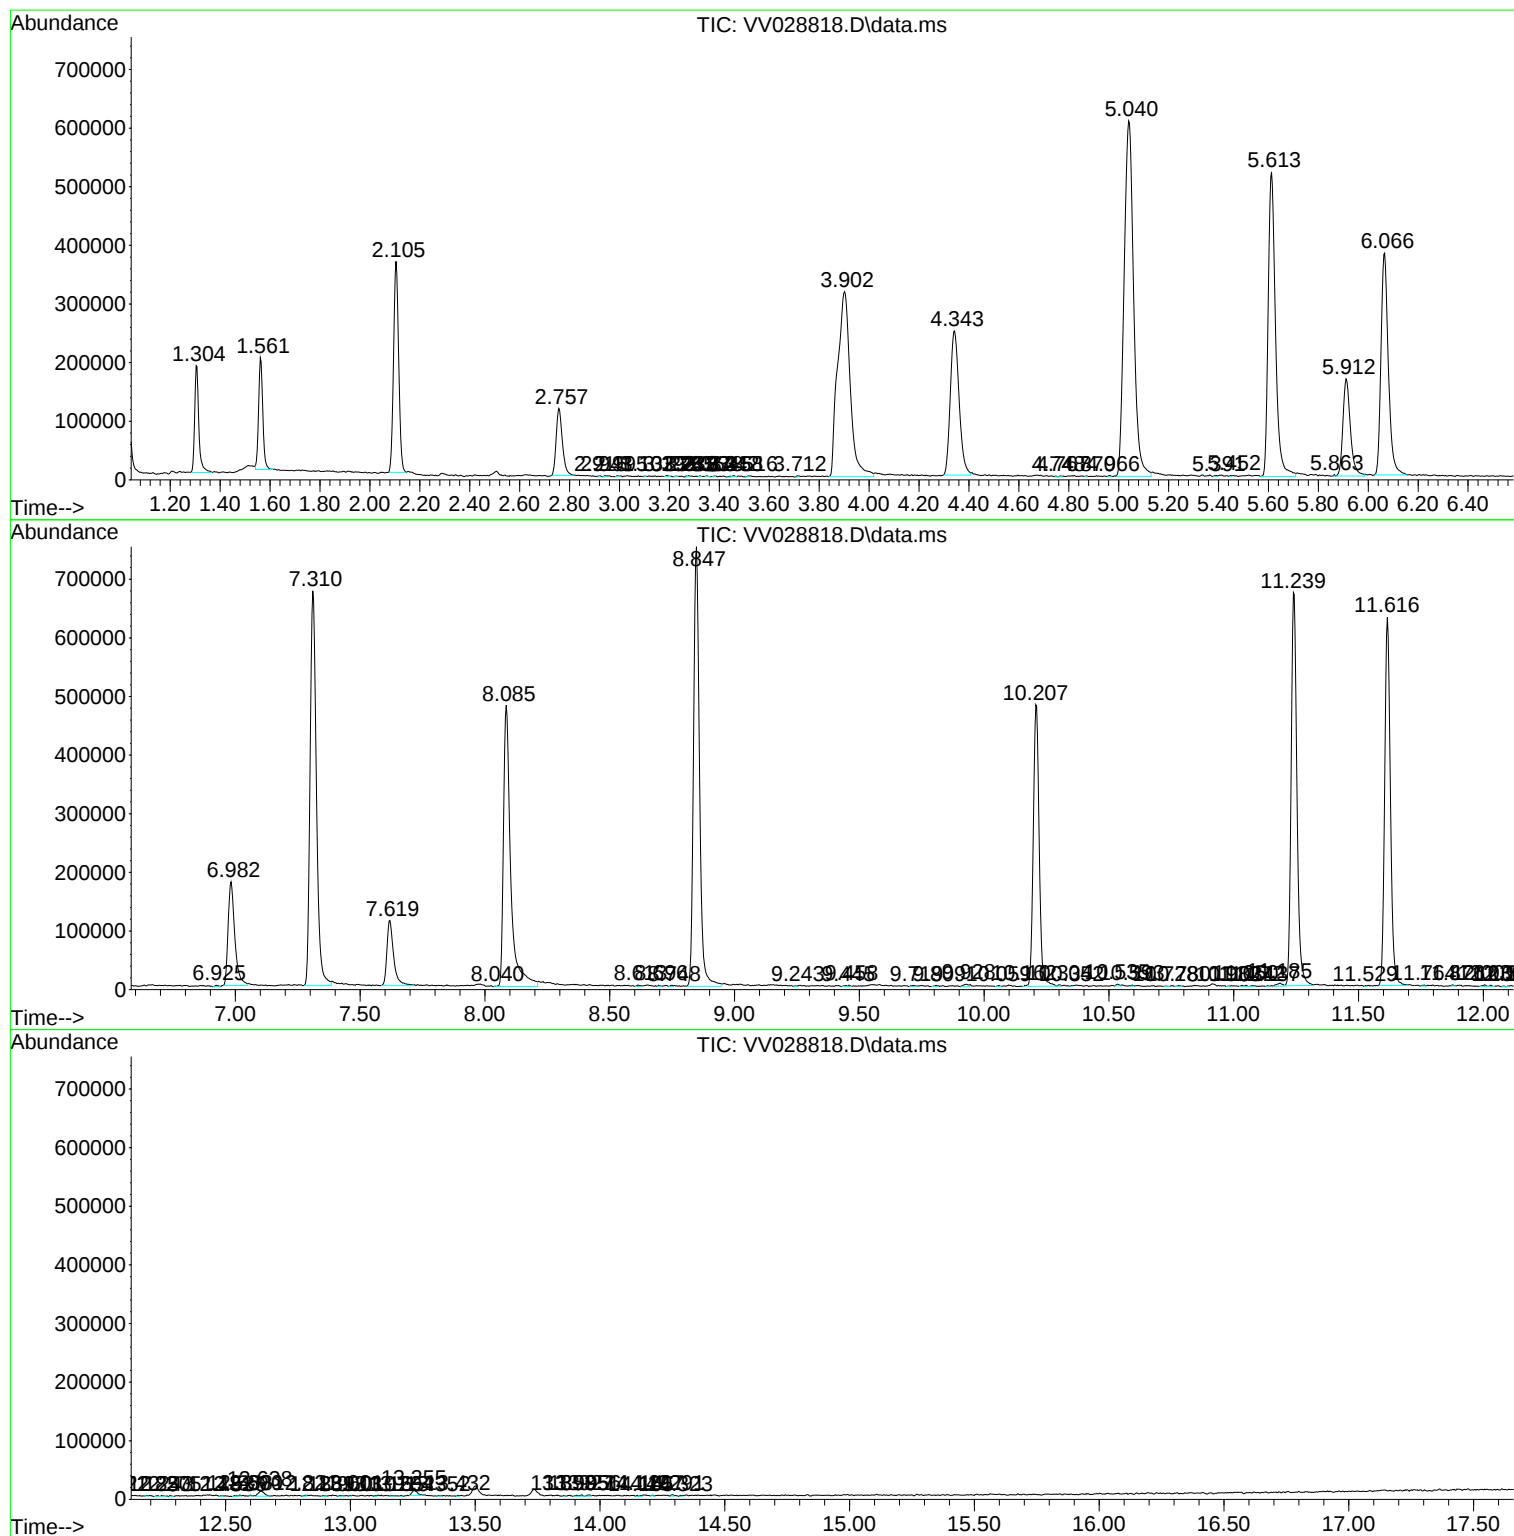

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110122\
Data File : VV028818.D
Acq On : 01 Nov 2022 16:27
Operator : SY/MD
Sample : N5321-12DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBWN6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110122\
Data File : VV028818.D
Acq On : 01 Nov 2022 16:27
Operator : SY/MD
Sample : N5321-12DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBWN6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------