

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110122\
 Data File : VV028819.D
 Acq On : 01 Nov 2022 16:51
 Operator : SY/MD
 Sample : N5354-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YBMP5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis

Signal : TIC: VV028819.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	96	rVB	175887	184489	11.55%	1.511%
2	1.561	157	162	178	rVB	193467	229406	14.37%	1.879%
3	2.105	322	331	343	rBV	359239	502401	31.47%	4.115%
4	2.381	414	417	420	rBV5	2062	1753	0.11%	0.014%
5	2.490	449	451	453	rBV3	1359	577	0.04%	0.005%
6	2.539	463	466	467	rBV2	1272	690	0.04%	0.006%
7	2.548	467	469	473	rVB4	1280	622	0.04%	0.005%
8	2.571	474	476	478	rBV2	1096	582	0.04%	0.005%
9	2.606	484	487	489	rBV4	1376	912	0.06%	0.007%
10	2.732	520	526	532	rBV	6469	8644	0.54%	0.071%
11	2.822	552	554	556	rBV3	971	585	0.04%	0.005%
12	2.838	556	559	562	rVB4	1562	1176	0.07%	0.010%
13	2.892	573	576	579	rBV5	1702	1088	0.07%	0.009%
14	2.950	590	594	597	rBV6	1316	938	0.06%	0.008%
15	3.079	629	634	636	rBV6	1461	1354	0.08%	0.011%
16	3.114	642	645	648	rBV6	1170	785	0.05%	0.006%
17	3.140	651	653	655	rBV3	1377	659	0.04%	0.005%
18	3.179	663	665	667	rBV3	1412	698	0.04%	0.006%
19	3.384	727	729	732	rBV3	1790	778	0.05%	0.006%
20	3.400	732	734	736	rBV3	1383	883	0.06%	0.007%
21	3.426	739	742	743	rBV3	1156	747	0.05%	0.006%
22	3.529	772	774	779	rBV5	1269	1403	0.09%	0.011%
23	3.626	800	804	809	rVB7	1434	1359	0.09%	0.011%
24	3.732	834	837	839	rBV4	1312	676	0.04%	0.006%
25	3.873	872	881	916	rBV	143170	410931	25.74%	3.366%
26	4.343	1012	1027	1048	rBV	249244	620676	38.87%	5.084%
27	4.603	1106	1108	1109	rBV2	1672	753	0.05%	0.006%
28	4.732	1146	1148	1150	rBV3	2005	949	0.06%	0.008%
29	4.834	1177	1180	1182	rBV4	1388	868	0.05%	0.007%
30	4.973	1219	1223	1224	rBV4	1116	749	0.05%	0.006%
31	5.040	1229	1244	1275	rVV2	608854	1596636	100.00%	13.079%
32	5.613	1411	1422	1446	rBV	513064	1036572	64.92%	8.491%
33	6.066	1550	1563	1585	rBV	383594	778777	48.78%	6.379%
34	6.359	1652	1654	1657	rBV4	1413	717	0.04%	0.006%
35	6.468	1685	1688	1691	rBV4	1852	1508	0.09%	0.012%
36	6.754	1775	1777	1778	rBV2	1510	681	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110122\
 Data File : VV028819.D
 Acq On : 01 Nov 2022 16:51
 Operator : SY/MD
 Sample : N5354-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YBMP5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis

37	6.870	1808	1813	1816	rBV6	1489	1415	0.09%	0.012%
38	6.934	1828	1833	1834	rBV3	811	593	0.04%	0.005%
39	6.982	1838	1848	1870	rBV	174681	324269	20.31%	2.656%
40	7.191	1909	1913	1914	rBV4	2004	1293	0.08%	0.011%
41	7.256	1928	1933	1936	rBV6	2652	2515	0.16%	0.021%
42	7.310	1939	1950	1983	rVV	672764	1203365	75.37%	9.858%
43	7.619	2036	2046	2069	rBV2	111890	204821	12.83%	1.678%
44	8.085	2181	2191	2229	rBV	451379	903727	56.60%	7.403%
45	8.551	2334	2336	2337	rBV2	1525	759	0.05%	0.006%
46	8.789	2407	2410	2415	rVB6	1103	667	0.04%	0.005%
47	8.847	2417	2428	2451	rBV	753521	1239564	77.64%	10.154%
48	9.140	2516	2519	2526	rBV9	2978	3609	0.23%	0.030%
49	9.204	2536	2539	2543	rBV6	2001	1900	0.12%	0.016%
50	9.407	2598	2602	2604	rBV5	1434	828	0.05%	0.007%
51	9.432	2608	2610	2613	rBV3	999	673	0.04%	0.006%
52	9.461	2617	2619	2620	rBV2	1515	637	0.04%	0.005%
53	9.493	2627	2629	2632	rVB4	1960	984	0.06%	0.008%
54	9.545	2632	2645	2654	rBV3	13581	26653	1.67%	0.218%
55	9.677	2682	2686	2690	rBV7	2891	2313	0.14%	0.019%
56	9.706	2693	2695	2696	rBV2	1506	647	0.04%	0.005%
57	9.786	2715	2720	2724	rBV5	2351	2819	0.18%	0.023%
58	9.931	2763	2765	2768	rVB4	1874	862	0.05%	0.007%
59	10.101	2813	2818	2820	rBV5	1620	1208	0.08%	0.010%
60	10.124	2823	2825	2828	rBV4	1181	813	0.05%	0.007%
61	10.207	2840	2851	2871	rBV	494502	778995	48.79%	6.381%
62	10.436	2919	2922	2925	rBV5	1780	1265	0.08%	0.010%
63	10.500	2938	2942	2944	rBV4	1531	1243	0.08%	0.010%
64	10.625	2978	2981	2983	rBV4	1423	1082	0.07%	0.009%
65	10.673	2992	2996	2999	rBV6	1449	960	0.06%	0.008%
66	10.760	3016	3023	3024	rBV7	1951	1606	0.10%	0.013%
67	10.879	3056	3060	3062	rBV4	1864	1539	0.10%	0.013%
68	10.976	3086	3090	3092	rBV5	1131	816	0.05%	0.007%
69	11.046	3108	3112	3115	rBV5	1664	1373	0.09%	0.011%
70	11.239	3162	3172	3192	rBV	661038	1061540	66.49%	8.696%
71	11.480	3244	3247	3250	rBV5	2344	1798	0.11%	0.015%
72	11.616	3277	3289	3309	rBV	622264	1001707	62.74%	8.206%
73	11.966	3394	3398	3401	rBV5	2150	1908	0.12%	0.016%
74	12.085	3433	3435	3438	rBV4	1346	1047	0.07%	0.009%
75	12.130	3447	3449	3451	rBV3	1153	604	0.04%	0.005%
76	12.236	3478	3482	3487	rBV8	1471	1359	0.09%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110122\
 Data File : VV028819.D
 Acq On : 01 Nov 2022 16:51
 Operator : SY/MD
 Sample : N5354-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YBMP5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis

77	12.316	3502	3507	3508	rBV5	1750	1453	0.09%	0.012%
78	12.535	3570	3575	3577	rBV6	2253	1478	0.09%	0.012%
79	12.574	3585	3587	3591	rBV5	1004	617	0.04%	0.005%
80	12.802	3654	3658	3661	rBV6	1592	1473	0.09%	0.012%
81	12.850	3669	3673	3676	rBV6	2161	1308	0.08%	0.011%
82	12.889	3680	3685	3688	rBV6	1146	968	0.06%	0.008%
83	12.921	3691	3695	3697	rBV5	1336	1119	0.07%	0.009%
84	12.969	3708	3710	3715	rBV5	1572	1680	0.11%	0.014%
85	13.143	3759	3764	3769	rBV7	2089	2205	0.14%	0.018%
86	13.207	3782	3784	3789	rBV4	1334	1287	0.08%	0.011%
87	13.236	3791	3793	3794	rBV2	1571	689	0.04%	0.006%
88	13.300	3811	3813	3817	rVB5	1684	1299	0.08%	0.011%
89	13.326	3817	3821	3823	rBV4	1454	929	0.06%	0.008%
90	13.435	3852	3855	3858	rBV5	2181	1637	0.10%	0.013%
91	13.628	3913	3915	3917	rBV3	1035	708	0.04%	0.006%
92	13.818	3970	3974	3975	rBV3	1177	689	0.04%	0.006%
93	13.850	3980	3984	3989	rBV6	2260	2147	0.13%	0.018%
94	13.988	4025	4027	4028	rBV2	1644	593	0.04%	0.005%
95	14.017	4033	4036	4038	rBV3	2767	1629	0.10%	0.013%
96	14.230	4100	4102	4104	rBV3	1567	912	0.06%	0.007%
97	14.487	4180	4182	4185	rBV5	1339	732	0.05%	0.006%
98	14.503	4185	4187	4189	rBV2	1528	825	0.05%	0.007%
99	14.570	4205	4208	4210	rBV4	1422	867	0.05%	0.007%
100	14.911	4311	4314	4318	rBV5	1806	1559	0.10%	0.013%




Sum of corrected areas: 12207601

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110122\
Data File : VV028819.D
Acq On : 01 Nov 2022 16:51
Operator : SY/MD
Sample : N5354-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YBMP5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

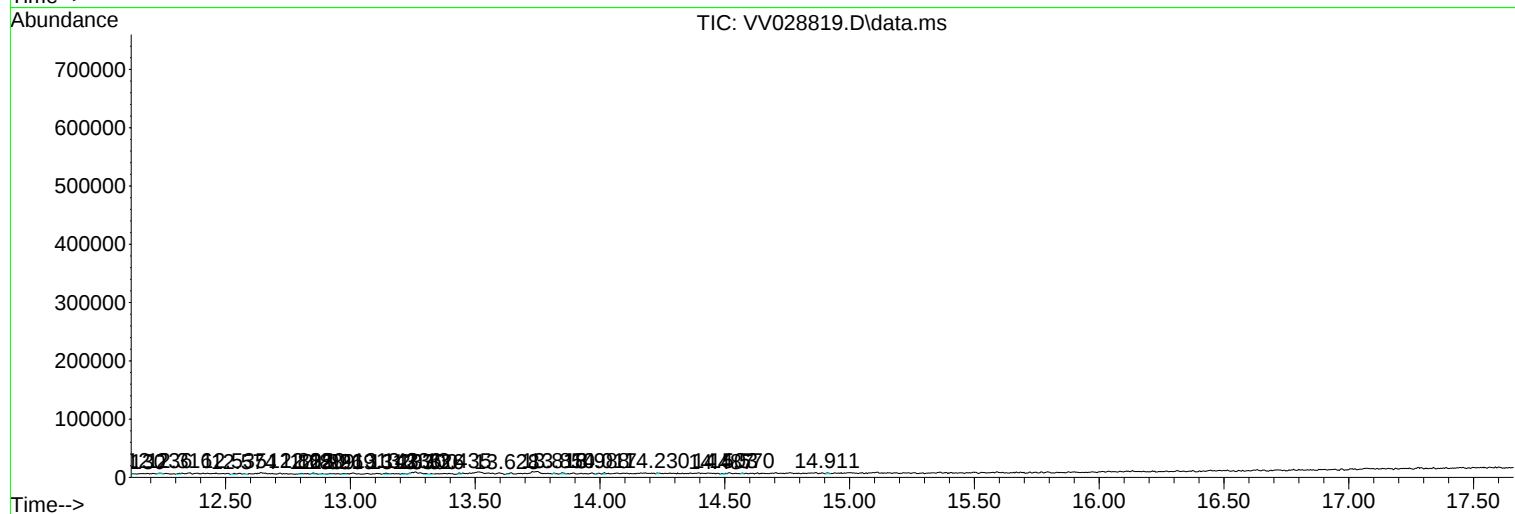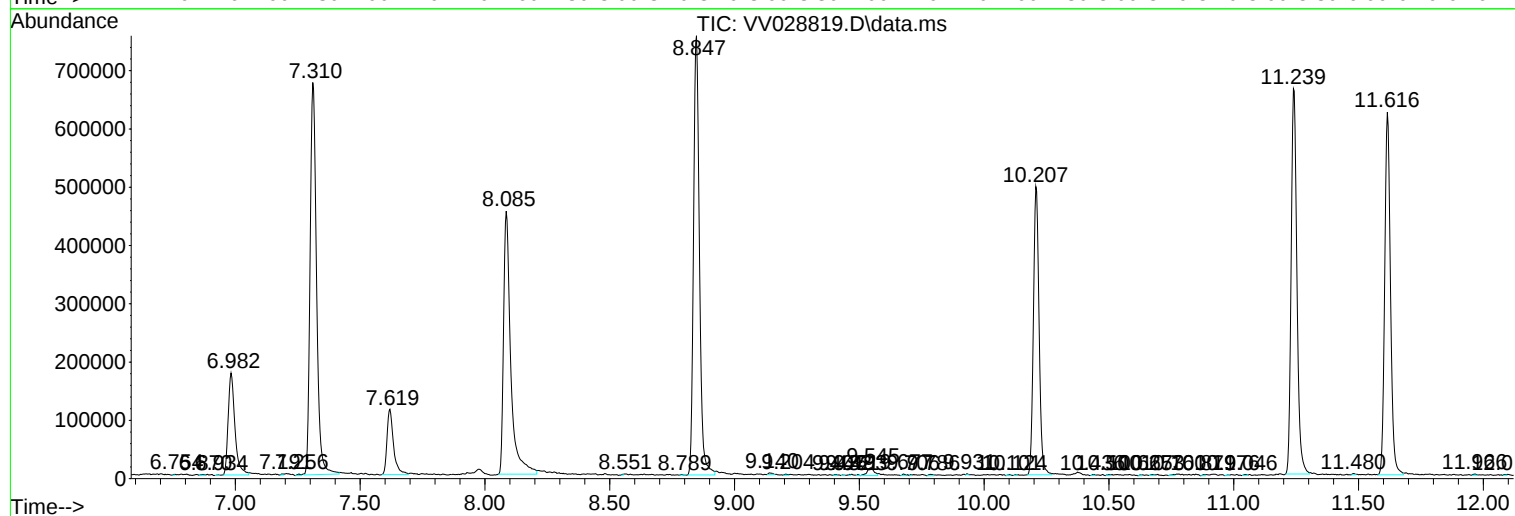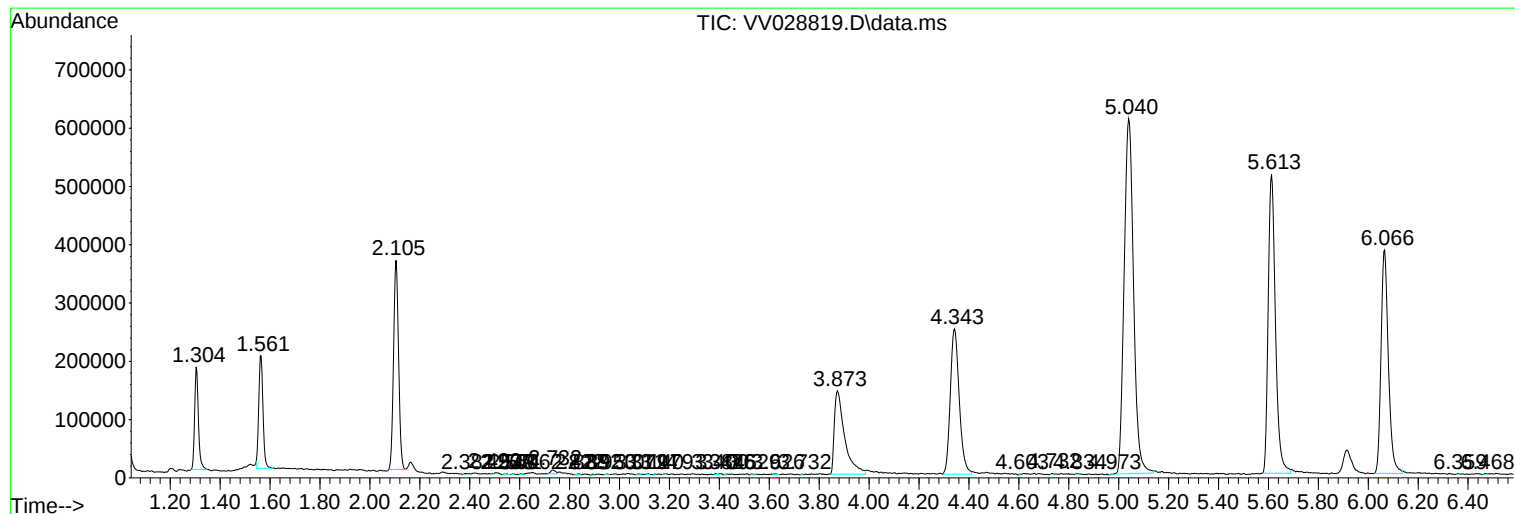

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110122\
Data File : VV028819.D
Acq On : 01 Nov 2022 16:51
Operator : SY/MD
Sample : N5354-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YBMP5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110122\
Data File : VV028819.D
Acq On : 01 Nov 2022 16:51
Operator : SY/MD
Sample : N5354-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YBMP5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc