

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110122\
 Data File : VV028823.D
 Acq On : 01 Nov 2022 18:28
 Operator : SY/MD
 Sample : N5354-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YBMP9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis

Signal : TIC: VV028823.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	99	rBV	227953	249411	14.98%	1.916%
2	1.564	156	163	179	rVB	225337	268481	16.13%	2.063%
3	2.105	322	331	343	rBV	427543	610487	36.67%	4.691%
4	2.471	444	445	448	rBV3	1175	760	0.05%	0.006%
5	2.908	578	581	582	rBV2	2028	1040	0.06%	0.008%
6	3.015	612	614	616	rBV3	1561	873	0.05%	0.007%
7	3.079	632	634	635	rBV2	1484	663	0.04%	0.005%
8	3.182	661	666	667	rBV4	3505	2714	0.16%	0.021%
9	3.359	718	721	722	rBV3	1339	767	0.05%	0.006%
10	3.439	743	746	748	rVB3	2549	1457	0.09%	0.011%
11	3.455	748	751	752	rBV3	1397	718	0.04%	0.006%
12	3.484	759	760	762	rVB2	1542	517	0.03%	0.004%
13	3.500	762	765	768	rBV5	1631	1176	0.07%	0.009%
14	3.584	787	791	793	rBV5	1440	1057	0.06%	0.008%
15	3.597	793	795	798	rBV3	1491	977	0.06%	0.008%
16	3.744	839	841	843	rBV2	2042	1261	0.08%	0.010%
17	3.796	855	857	860	rVB4	1120	440	0.03%	0.003%
18	3.876	872	882	885	rBV	149754	243895	14.65%	1.874%
19	4.342	1014	1027	1052	rVB	254290	624127	37.49%	4.796%
20	4.760	1155	1157	1159	rBV2	1506	752	0.05%	0.006%
21	5.040	1228	1244	1273	rBV2	635222	1664757	100.00%	12.792%
22	5.613	1409	1422	1450	rBV	503748	1025784	61.62%	7.882%
23	5.912	1503	1515	1536	rBV	456522	897993	53.94%	6.900%
24	6.066	1551	1563	1583	rBV2	387603	778583	46.77%	5.983%
25	6.931	1831	1832	1835	rBV2	992	520	0.03%	0.004%
26	6.982	1837	1848	1865	rBV	172567	320893	19.28%	2.466%
27	7.310	1939	1950	1978	rBV	705372	1233385	74.09%	9.477%
28	7.619	2037	2046	2063	rBV	112128	199191	11.97%	1.531%
29	8.085	2182	2191	2231	rBV	446774	869161	52.21%	6.679%
30	8.719	2383	2388	2390	rBV5	2131	2074	0.12%	0.016%
31	8.847	2417	2428	2447	rBV	733661	1187363	71.32%	9.124%
32	9.458	2616	2618	2620	rBV3	1242	480	0.03%	0.004%
33	9.545	2638	2645	2656	rBV3	8817	15699	0.94%	0.121%
34	9.638	2672	2674	2676	rBV3	1598	695	0.04%	0.005%
35	9.670	2682	2684	2686	rBV2	1623	884	0.05%	0.007%
36	9.706	2692	2695	2697	rBV4	1533	824	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110122\
 Data File : VV028823.D
 Acq On : 01 Nov 2022 18:28
 Operator : SY/MD
 Sample : N5354-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YBMP9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis

37	9.860	2740	2743	2744	rBV3	1778	987	0.06%	0.008%
38	10.024	2792	2794	2795	rBV	1144	337	0.02%	0.003%
39	10.207	2840	2851	2872	rBV	471552	755585	45.39%	5.806%
40	10.342	2892	2893	2894	rBV	1075	238	0.01%	0.002%
41	10.583	2966	2968	2971	rBV4	1222	797	0.05%	0.006%
42	10.651	2986	2989	2993	rBV6	2122	1726	0.10%	0.013%
43	10.947	3079	3081	3087	rBV6	1240	1353	0.08%	0.010%
44	11.124	3132	3136	3140	rBV5	1690	1811	0.11%	0.014%
45	11.140	3140	3141	3143	rVV3	1035	385	0.02%	0.003%
46	11.243	3162	3173	3193	rBV	640775	1030952	61.93%	7.922%
47	11.471	3241	3244	3246	rBV4	1436	1017	0.06%	0.008%
48	11.616	3278	3289	3316	rBV	619389	992467	59.62%	7.626%
49	11.895	3374	3376	3378	rBV4	1512	890	0.05%	0.007%
50	11.940	3385	3390	3393	rBV6	1532	1600	0.10%	0.012%
51	12.024	3413	3416	3421	rBV7	1999	1951	0.12%	0.015%
52	12.233	3479	3481	3484	rBV4	1203	979	0.06%	0.008%
53	12.294	3497	3500	3501	rBV3	1277	740	0.04%	0.006%
54	12.513	3566	3568	3572	rBV5	1371	730	0.04%	0.006%
55	12.937	3698	3700	3704	rVB5	1714	853	0.05%	0.007%
56	13.345	3821	3827	3828	rBV6	2056	1929	0.12%	0.015%
57	14.085	4055	4057	4059	rBV3	1494	673	0.04%	0.005%
58	14.159	4077	4080	4086	rBV7	2216	2658	0.16%	0.020%
59	14.422	4160	4162	4167	rVB5	2316	1784	0.11%	0.014%
60	14.541	4198	4199	4200	rBV	1599	480	0.03%	0.004%
61	15.789	4584	4587	4588	rBV3	2352	1400	0.08%	0.011%




Sum of corrected areas: 13014181

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110122\
Data File : VV028823.D
Acq On : 01 Nov 2022 18:28
Operator : SY/MD
Sample : N5354-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YBMP9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

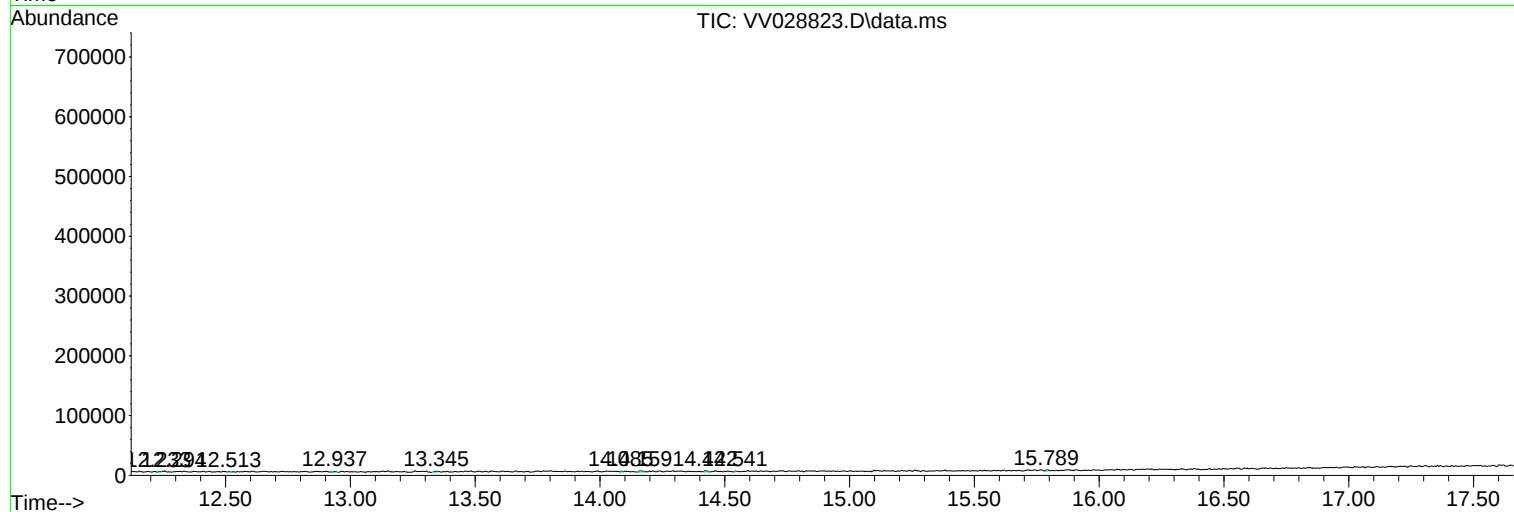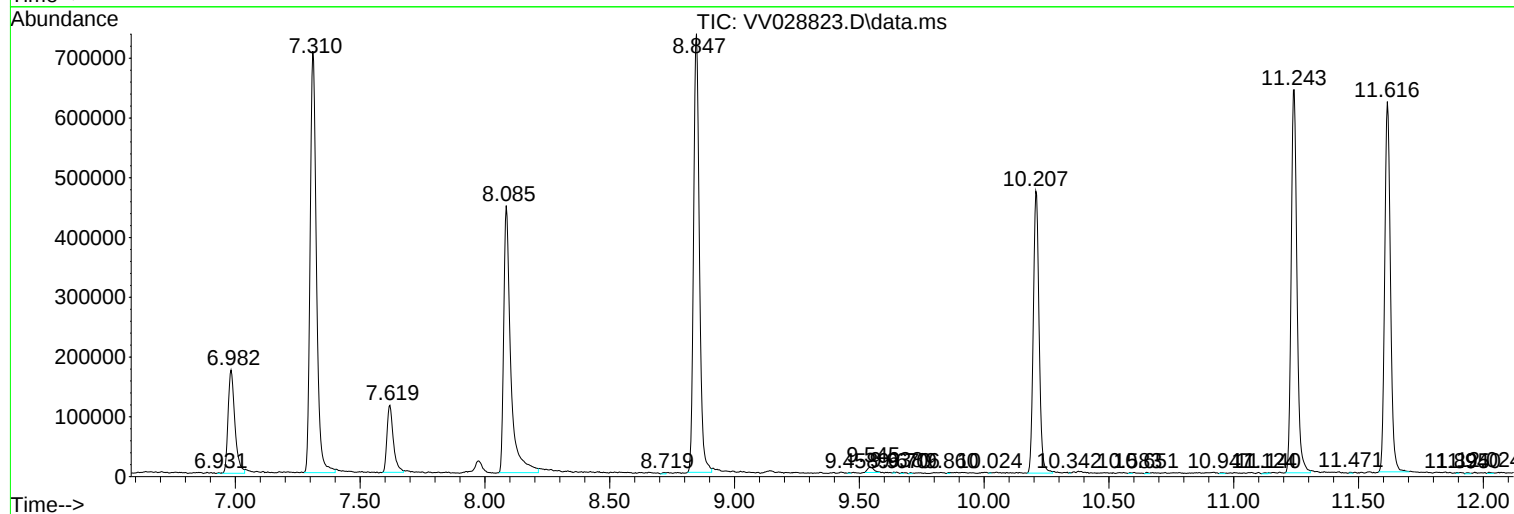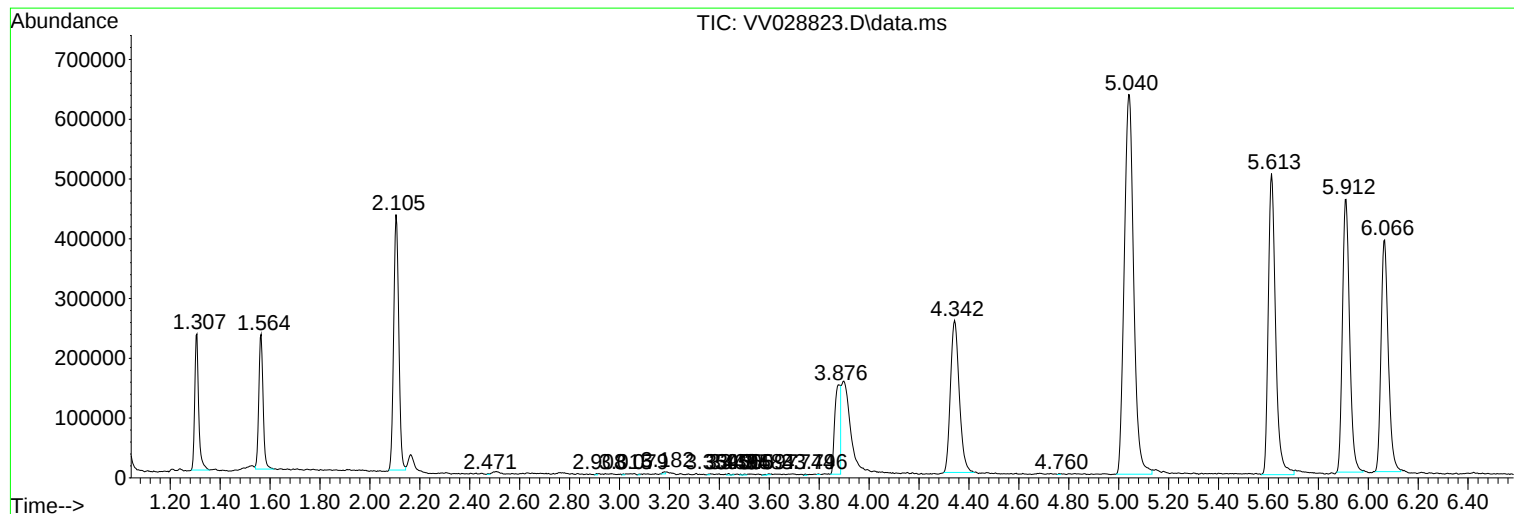

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110122\
Data File : VV028823.D
Acq On : 01 Nov 2022 18:28
Operator : SY/MD
Sample : N5354-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YBMP9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110122\
Data File : VV028823.D
Acq On : 01 Nov 2022 18:28
Operator : SY/MD
Sample : N5354-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YBMP9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc