

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110122\
 Data File : VV028825.D
 Acq On : 01 Nov 2022 19:16
 Operator : SY/MD
 Sample : N5353-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBVV2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis

Signal : TIC: VV028825.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.108	17	21	26	rVB2	15685	13546	0.20%	0.058%
2	1.304	76	82	102	rVB	243480	272474	4.03%	1.175%
3	1.564	156	163	178	rVB	215946	252480	3.73%	1.089%
4	2.105	322	331	346	rVB2	427272	618303	9.14%	2.667%
5	2.490	449	451	454	rBV4	1504	885	0.01%	0.004%
6	2.757	522	534	557	rVV	460971	797406	11.79%	3.440%
7	2.921	582	585	586	rBV3	2246	1239	0.02%	0.005%
8	3.252	685	688	694	rVB8	1198	814	0.01%	0.004%
9	3.326	709	711	714	rVB4	1672	971	0.01%	0.004%
10	3.394	730	732	736	rVB5	1847	1201	0.02%	0.005%
11	3.416	736	739	741	rBV4	1378	920	0.01%	0.004%
12	3.484	758	760	764	rVB5	1758	967	0.01%	0.004%
13	3.506	764	767	770	rBV5	1404	1094	0.02%	0.005%
14	3.529	770	774	777	rVV6	1642	1446	0.02%	0.006%
15	3.613	798	800	805	rBV4	1187	1043	0.02%	0.004%
16	3.648	809	811	813	rVV3	1452	715	0.01%	0.003%
17	3.799	856	858	862	rVB5	1853	957	0.01%	0.004%
18	3.825	862	866	868	rBV5	1700	1165	0.02%	0.005%
19	3.902	871	890	919	rBV2	1308487	3439299	50.85%	14.837%
20	4.342	1011	1027	1052	rBV	253365	631451	9.34%	2.724%
21	4.706	1137	1140	1141	rBV3	1479	777	0.01%	0.003%
22	4.748	1150	1153	1157	rBV6	2017	1641	0.02%	0.007%
23	4.940	1210	1213	1214	rBV3	1062	696	0.01%	0.003%
24	4.966	1217	1221	1227	rVB9	2731	2853	0.04%	0.012%
25	5.040	1227	1244	1273	rBV2	634422	1677454	24.80%	7.237%
26	5.612	1410	1422	1453	rBV	496012	1020493	15.09%	4.402%
27	5.908	1500	1514	1546	rBV	3564999	6764126	100.00%	29.181%
28	6.066	1552	1563	1590	rVB	387322	781168	11.55%	3.370%
29	6.510	1697	1701	1703	rBV5	1778	1304	0.02%	0.006%
30	6.551	1711	1714	1718	rBV6	1770	1388	0.02%	0.006%
31	6.567	1718	1719	1725	rVB5	1438	858	0.01%	0.004%
32	6.600	1725	1729	1732	rBV6	1158	1132	0.02%	0.005%
33	6.632	1737	1739	1740	rBV2	1913	669	0.01%	0.003%
34	6.866	1808	1812	1816	rBV7	1879	2104	0.03%	0.009%
35	6.895	1819	1821	1824	rVB4	1447	758	0.01%	0.003%
36	6.982	1837	1848	1868	rBV	175271	328749	4.86%	1.418%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110122\
 Data File : VV028825.D
 Acq On : 01 Nov 2022 19:16
 Operator : SY/MD
 Sample : N5353-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBVV2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis

37	7.310	1938	1950	1976	rBV	692197	1224495	18.10%	5.283%
38	7.616	2036	2045	2066	rBV	111057	202915	3.00%	0.875%
39	7.973	2147	2156	2170	rVB2	110105	185973	2.75%	0.802%
40	8.085	2182	2191	2233	rBV	428490	826298	12.22%	3.565%
41	8.368	2277	2279	2281	rBV3	1518	717	0.01%	0.003%
42	8.522	2325	2327	2331	rVB5	1218	825	0.01%	0.004%
43	8.693	2376	2380	2382	rBV5	1578	938	0.01%	0.004%
44	8.847	2414	2428	2452	rBV	729080	1204618	17.81%	5.197%
45	9.082	2500	2501	2504	rBV3	1487	672	0.01%	0.003%
46	9.185	2531	2533	2537	rBV5	1321	1019	0.02%	0.004%
47	9.210	2540	2541	2546	rVB5	1485	1037	0.02%	0.004%
48	9.275	2557	2561	2565	rBV5	1869	1679	0.02%	0.007%
49	9.644	2673	2676	2679	rBV5	1313	1167	0.02%	0.005%
50	9.780	2713	2718	2721	rBV6	2239	2498	0.04%	0.011%
51	9.841	2735	2737	2740	rBV4	1074	691	0.01%	0.003%
52	9.857	2740	2742	2747	rVB6	1853	1290	0.02%	0.006%
53	9.918	2758	2761	2762	rBV3	1340	764	0.01%	0.003%
54	9.989	2779	2783	2786	rVB5	1451	937	0.01%	0.004%
55	10.079	2805	2811	2818	rBV5	2437	3609	0.05%	0.016%
56	10.207	2839	2851	2872	rBV	468478	753129	11.13%	3.249%
57	10.429	2918	2920	2925	rVB5	1417	1030	0.02%	0.004%
58	10.497	2939	2941	2945	rBV5	1414	1239	0.02%	0.005%
59	10.538	2948	2954	2958	rVV8	1701	1877	0.03%	0.008%
60	10.651	2986	2989	2993	rVB5	1630	1268	0.02%	0.005%
61	10.670	2993	2995	2998	rBV4	1665	1080	0.02%	0.005%
62	10.728	3010	3013	3016	rVV5	1693	1269	0.02%	0.005%
63	10.744	3016	3018	3022	rVV5	1384	870	0.01%	0.004%
64	10.763	3022	3024	3027	rVB4	1529	787	0.01%	0.003%
65	10.821	3038	3042	3044	rBV5	1156	862	0.01%	0.004%
66	10.902	3065	3067	3070	rBV4	1529	967	0.01%	0.004%
67	11.127	3134	3137	3141	rBV6	1194	1100	0.02%	0.005%
68	11.239	3161	3172	3194	rBV	657480	1057301	15.63%	4.561%
69	11.615	3278	3289	3311	rBV	618293	1037016	15.33%	4.474%
70	11.889	3372	3374	3377	rVB5	1970	931	0.01%	0.004%
71	11.934	3384	3388	3389	rBV4	1991	1056	0.02%	0.005%
72	12.101	3437	3440	3443	rBV5	1813	1354	0.02%	0.006%
73	12.297	3499	3501	3503	rBV3	1287	722	0.01%	0.003%
74	12.371	3520	3524	3527	rBV6	1061	1011	0.01%	0.004%
75	12.426	3537	3541	3543	rBV5	1033	707	0.01%	0.003%
76	12.631	3601	3605	3608	rBV6	1587	1415	0.02%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110122\
 Data File : VV028825.D
 Acq On : 01 Nov 2022 19:16
 Operator : SY/MD
 Sample : N5353-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBVV2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis

77	12.722	3627	3633	3636	rBV7	2104	2401	0.04%	0.010%
78	12.821	3660	3664	3665	rBV4	1299	717	0.01%	0.003%
79	12.892	3684	3686	3689	rBV3	1097	722	0.01%	0.003%
80	12.969	3707	3710	3713	rBV5	1050	706	0.01%	0.003%
81	13.040	3728	3732	3737	rBV8	1405	1647	0.02%	0.007%
82	13.207	3782	3784	3786	rBV3	1166	665	0.01%	0.003%
83	13.291	3807	3810	3813	rBV4	1538	1363	0.02%	0.006%
84	13.361	3830	3832	3835	rVB3	1426	677	0.01%	0.003%
85	13.548	3885	3890	3892	rBV6	1202	1273	0.02%	0.005%
86	13.599	3904	3906	3909	rBV4	2041	1217	0.02%	0.005%
87	13.615	3909	3911	3913	rBV3	1596	687	0.01%	0.003%
88	13.660	3922	3925	3927	rBV3	1482	887	0.01%	0.004%
89	13.683	3930	3932	3935	rBV4	1502	1069	0.02%	0.005%
90	13.728	3942	3946	3947	rBV5	1195	965	0.01%	0.004%
91	13.914	4002	4004	4006	rBV3	1347	690	0.01%	0.003%
92	13.956	4013	4017	4021	rBV8	1193	1137	0.02%	0.005%
93	14.046	4042	4045	4049	rBV5	1359	1048	0.02%	0.005%
94	14.069	4049	4052	4054	rBV4	1557	955	0.01%	0.004%
95	14.188	4086	4089	4091	rBV3	1300	838	0.01%	0.004%
96	14.403	4154	4156	4161	rVB5	1658	1159	0.02%	0.005%
97	14.429	4161	4164	4167	rBV4	1478	1270	0.02%	0.005%
98	14.702	4244	4249	4252	rBV6	2246	2327	0.03%	0.010%
99	14.908	4311	4313	4316	rBV4	1563	724	0.01%	0.003%
100	15.062	4359	4361	4365	rBV5	1506	1169	0.02%	0.005%




Sum of corrected areas: 23179992

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110122\
Data File : VV028825.D
Acq On : 01 Nov 2022 19:16
Operator : SY/MD
Sample : N5353-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBVV2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

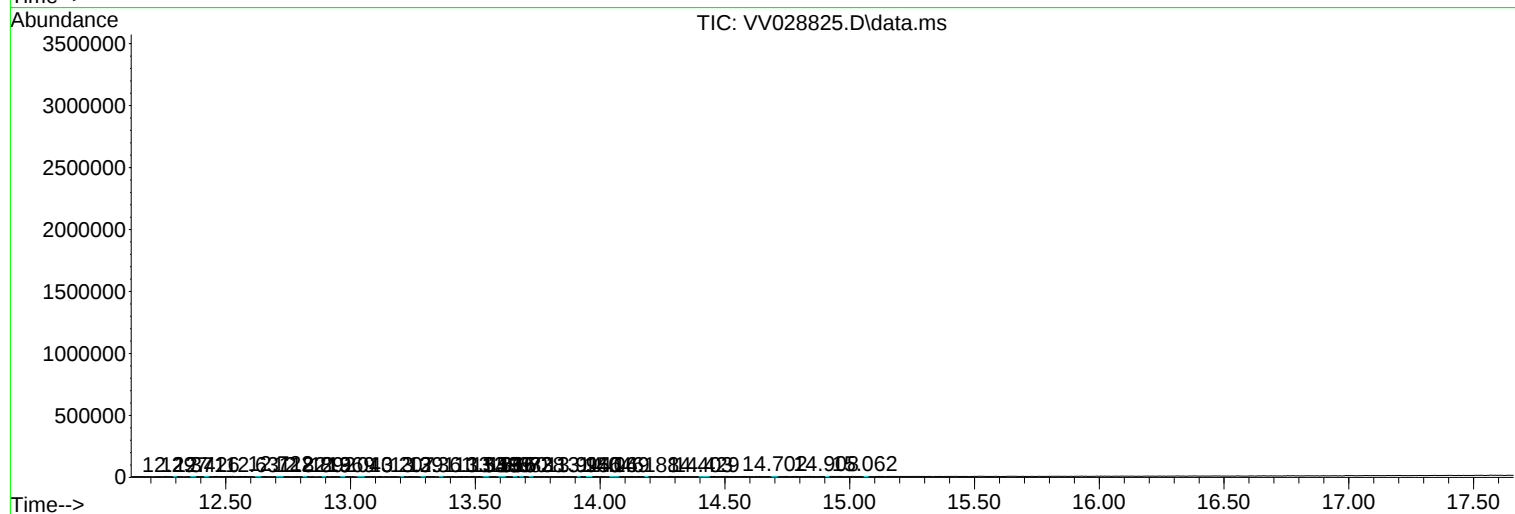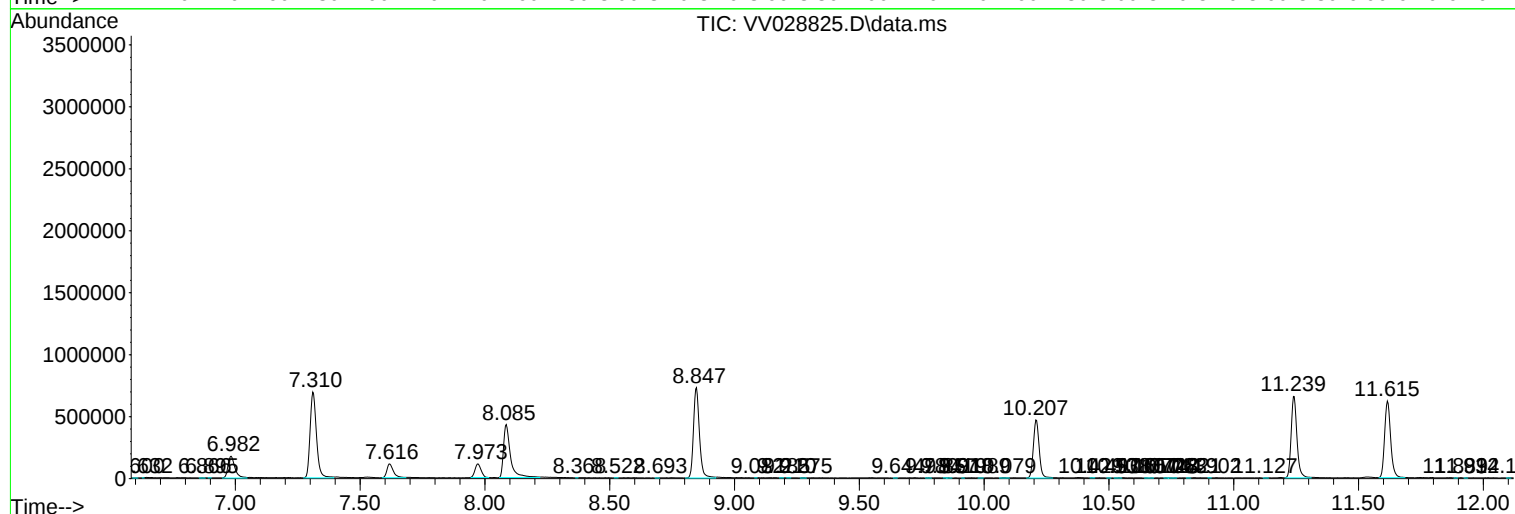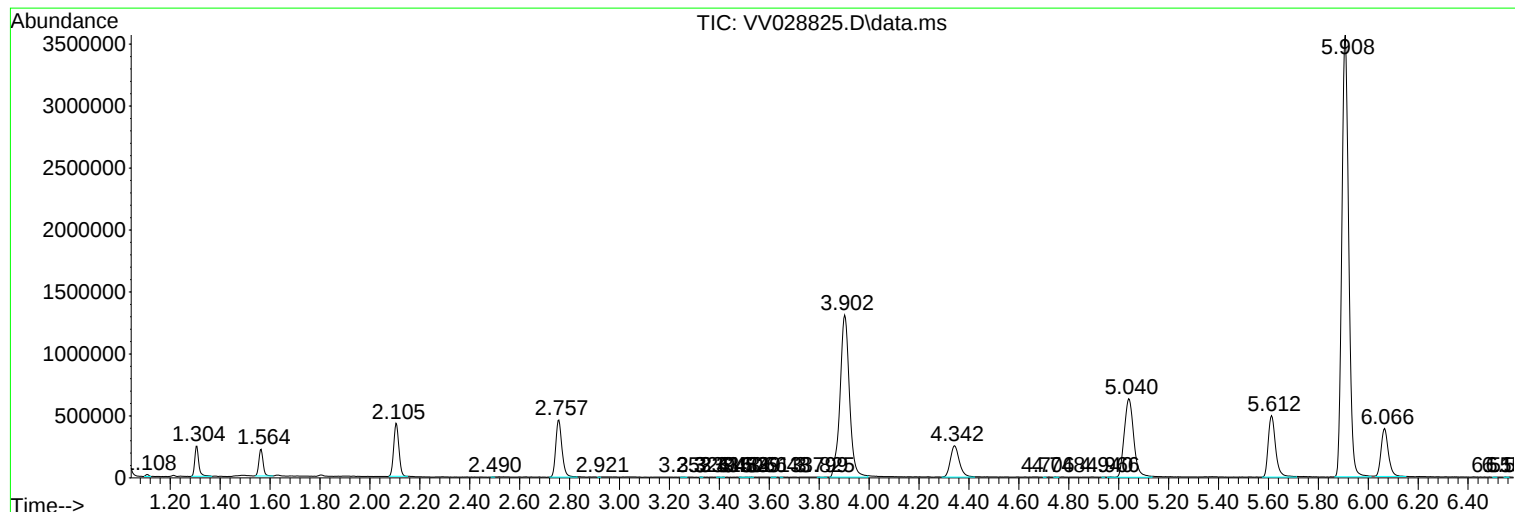

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110122\
Data File : VV028825.D
Acq On : 01 Nov 2022 19:16
Operator : SY/MD
Sample : N5353-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBVV2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110122\
Data File : VV028825.D
Acq On : 01 Nov 2022 19:16
Operator : SY/MD
Sample : N5353-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBVV2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc