

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110122\
 Data File : VV028826.D
 Acq On : 01 Nov 2022 19:40
 Operator : SY/MD
 Sample : N5354-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis

Signal : TIC: VV028826.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	102	rBV	216971	246800	15.06%	1.998%
2	1.561	156	162	180	rVB	221817	269054	16.42%	2.178%
3	2.105	322	331	346	rVB	417934	593776	36.24%	4.807%
4	2.686	510	512	519	rBV6	2386	2365	0.14%	0.019%
5	2.883	570	573	574	rBV3	1554	910	0.06%	0.007%
6	2.969	598	600	604	rVB3	1708	805	0.05%	0.007%
7	3.104	638	642	643	rBV4	1627	1180	0.07%	0.010%
8	3.149	652	656	659	rBV6	1924	1482	0.09%	0.012%
9	3.169	659	662	664	rVB4	1471	984	0.06%	0.008%
10	3.185	664	667	669	rBV3	1924	1114	0.07%	0.009%
11	3.288	696	699	704	rBV7	1925	1519	0.09%	0.012%
12	3.323	705	710	714	rVV6	1166	1210	0.07%	0.010%
13	3.384	727	729	732	rBV4	1451	923	0.06%	0.007%
14	3.410	735	737	741	rBV5	1185	881	0.05%	0.007%
15	3.497	759	764	766	rBV6	1871	1687	0.10%	0.014%
16	3.616	798	801	807	rVB7	1939	1532	0.09%	0.012%
17	3.645	807	810	813	rBV4	1439	1022	0.06%	0.008%
18	3.677	817	820	823	rVB5	1791	1095	0.07%	0.009%
19	3.706	823	829	835	rBV10	1746	2661	0.16%	0.022%
20	3.738	837	839	842	rVB3	1254	771	0.05%	0.006%
21	3.809	859	861	864	rVB4	1729	877	0.05%	0.007%
22	3.873	870	881	925	rBV	148449	452943	27.65%	3.667%
23	4.342	1014	1027	1052	rVB	251995	614196	37.49%	4.973%
24	4.744	1150	1152	1154	rBV3	1486	782	0.05%	0.006%
25	4.796	1164	1168	1171	rBV5	1452	1164	0.07%	0.009%
26	4.860	1183	1188	1189	rBV5	1240	949	0.06%	0.008%
27	4.973	1220	1223	1226	rBV4	1189	798	0.05%	0.006%
28	5.040	1229	1244	1272	rVV2	623559	1638343	100.00%	13.265%
29	5.407	1356	1358	1359	rBV	1603	776	0.05%	0.006%
30	5.442	1366	1369	1371	rBV4	1989	914	0.06%	0.007%
31	5.564	1402	1407	1408	rBV4	1037	959	0.06%	0.008%
32	5.612	1410	1422	1451	rVV	495111	1009606	61.62%	8.174%
33	5.911	1505	1515	1524	rBV	12506	28316	1.73%	0.229%
34	6.066	1551	1563	1586	rBV	384500	781209	47.68%	6.325%
35	6.365	1654	1656	1659	rBV4	1785	1048	0.06%	0.008%
36	6.381	1659	1661	1663	rBV3	2025	898	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110122\
 Data File : VV028826.D
 Acq On : 01 Nov 2022 19:40
 Operator : SY/MD
 Sample : N5354-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis

37	6.526	1704	1706	1710	rVB5	1485	876	0.05%	0.007%
38	6.596	1726	1728	1733	rVB6	2001	1239	0.08%	0.010%
39	6.638	1734	1741	1742	rBV7	2909	3191	0.19%	0.026%
40	6.786	1785	1787	1791	rVB5	1692	923	0.06%	0.007%
41	6.908	1819	1825	1827	rBV7	1234	1220	0.07%	0.010%
42	6.950	1834	1838	1839	rBV4	1955	1391	0.08%	0.011%
43	6.982	1839	1848	1875	rVV	169810	319767	19.52%	2.589%
44	7.178	1907	1909	1912	rBV3	1965	1537	0.09%	0.012%
45	7.310	1940	1950	1976	rBV	693816	1211277	73.93%	9.807%
46	7.619	2035	2046	2065	rBV	109274	201174	12.28%	1.629%
47	8.037	2173	2176	2180	rBV6	1650	1160	0.07%	0.009%
48	8.085	2181	2191	2226	rBV	461822	907946	55.42%	7.351%
49	8.516	2322	2325	2328	rBV5	1308	947	0.06%	0.008%
50	8.783	2403	2408	2409	rBV3	1489	1225	0.07%	0.010%
51	8.847	2416	2428	2452	rBV	728373	1199712	73.23%	9.713%
52	9.143	2518	2520	2522	rBV3	1331	783	0.05%	0.006%
53	9.329	2576	2578	2582	rBV5	1168	1251	0.08%	0.010%
54	9.538	2640	2643	2647	rBV6	1542	1228	0.07%	0.010%
55	9.564	2647	2651	2654	rBV5	1548	1578	0.10%	0.013%
56	9.767	2711	2714	2715	rBV3	1357	789	0.05%	0.006%
57	9.837	2733	2736	2738	rBV4	1267	687	0.04%	0.006%
58	9.911	2755	2759	2762	rBV6	2111	2004	0.12%	0.016%
59	9.943	2767	2769	2774	rVB5	2405	1495	0.09%	0.012%
60	9.969	2774	2777	2781	rBV6	2081	1708	0.10%	0.014%
61	9.998	2781	2786	2790	rBV	13905	9787	0.60%	0.079%
62	10.098	2814	2817	2819	rBV3	1694	870	0.05%	0.007%
63	10.146	2828	2832	2834	rBV4	1880	1381	0.08%	0.011%
64	10.207	2839	2851	2871	rVV	472430	757033	46.21%	6.129%
65	10.496	2939	2941	2945	rVB5	1953	1199	0.07%	0.010%
66	10.567	2960	2963	2964	rBV4	1319	697	0.04%	0.006%
67	10.622	2978	2980	2985	rVV5	1298	917	0.06%	0.007%
68	10.683	2997	2999	3003	rBV5	1123	862	0.05%	0.007%
69	10.850	3046	3051	3055	rVB8	2336	2286	0.14%	0.019%
70	10.876	3055	3059	3060	rBV4	1189	684	0.04%	0.006%
71	10.905	3067	3068	3073	rVV5	1231	1121	0.07%	0.009%
72	11.111	3129	3132	3134	rVB3	1326	699	0.04%	0.006%
73	11.159	3144	3147	3148	rBV3	1110	733	0.04%	0.006%
74	11.239	3162	3172	3192	rBV	630456	1027627	62.72%	8.320%
75	11.615	3277	3289	3309	rBV	619933	987741	60.29%	7.997%
76	11.815	3347	3351	3353	rBV5	1898	1400	0.09%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110122\
 Data File : VV028826.D
 Acq On : 01 Nov 2022 19:40
 Operator : SY/MD
 Sample : N5354-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis

77	12.201	3468	3471	3472	rBV3	1786	1110	0.07%	0.009%
78	12.458	3549	3551	3556	rVB5	1273	948	0.06%	0.008%
79	12.512	3562	3568	3570	rBV5	1115	1167	0.07%	0.009%
80	12.686	3618	3622	3624	rBV5	1149	790	0.05%	0.006%
81	12.747	3637	3641	3643	rBV5	1124	840	0.05%	0.007%
82	12.892	3684	3686	3688	rBV3	1305	684	0.04%	0.006%
83	13.004	3717	3721	3722	rBV3	1349	925	0.06%	0.007%
84	13.088	3745	3747	3751	rBV5	1587	1228	0.07%	0.010%
85	13.168	3769	3772	3776	rBV7	1606	991	0.06%	0.008%
86	13.207	3779	3784	3788	rBV7	1466	1313	0.08%	0.011%
87	13.233	3788	3792	3795	rBV4	1518	1180	0.07%	0.010%
88	13.365	3829	3833	3836	rBV6	1779	1521	0.09%	0.012%
89	13.525	3881	3883	3886	rBV4	1459	828	0.05%	0.007%
90	13.580	3897	3900	3902	rBV4	1188	790	0.05%	0.006%
91	13.590	3902	3903	3910	rVB6	1611	1405	0.09%	0.011%
92	13.619	3910	3912	3914	rBV3	1533	913	0.06%	0.007%
93	13.792	3961	3966	3967	rBV4	1425	1119	0.07%	0.009%
94	13.998	4026	4030	4032	rBV5	2158	1771	0.11%	0.014%
95	14.030	4038	4040	4042	rBV3	1762	779	0.05%	0.006%
96	14.239	4100	4105	4107	rBV4	1795	1577	0.10%	0.013%
97	14.274	4114	4116	4118	rBV3	1154	719	0.04%	0.006%
98	14.397	4152	4154	4157	rBV3	1944	963	0.06%	0.008%
99	14.474	4176	4178	4182	rBV5	1066	795	0.05%	0.006%
100	14.596	4213	4216	4218	rBV4	1527	1085	0.07%	0.009%




Sum of corrected areas: 12351135

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110122\
Data File : VV028826.D
Acq On : 01 Nov 2022 19:40
Operator : SY/MD
Sample : N5354-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

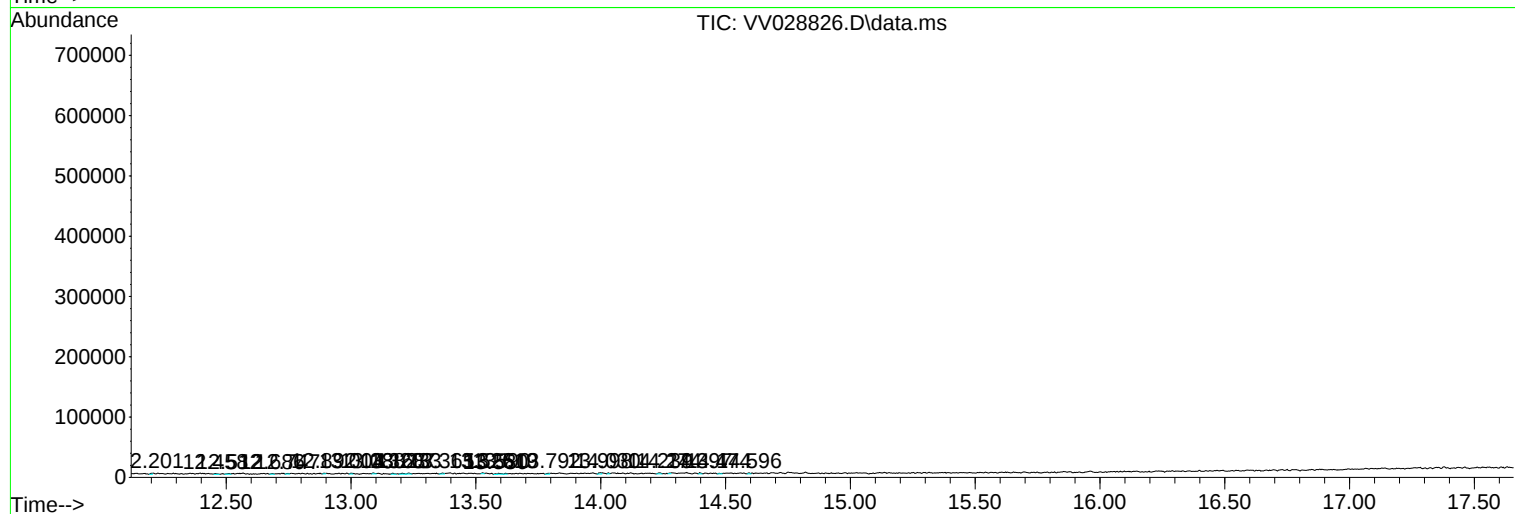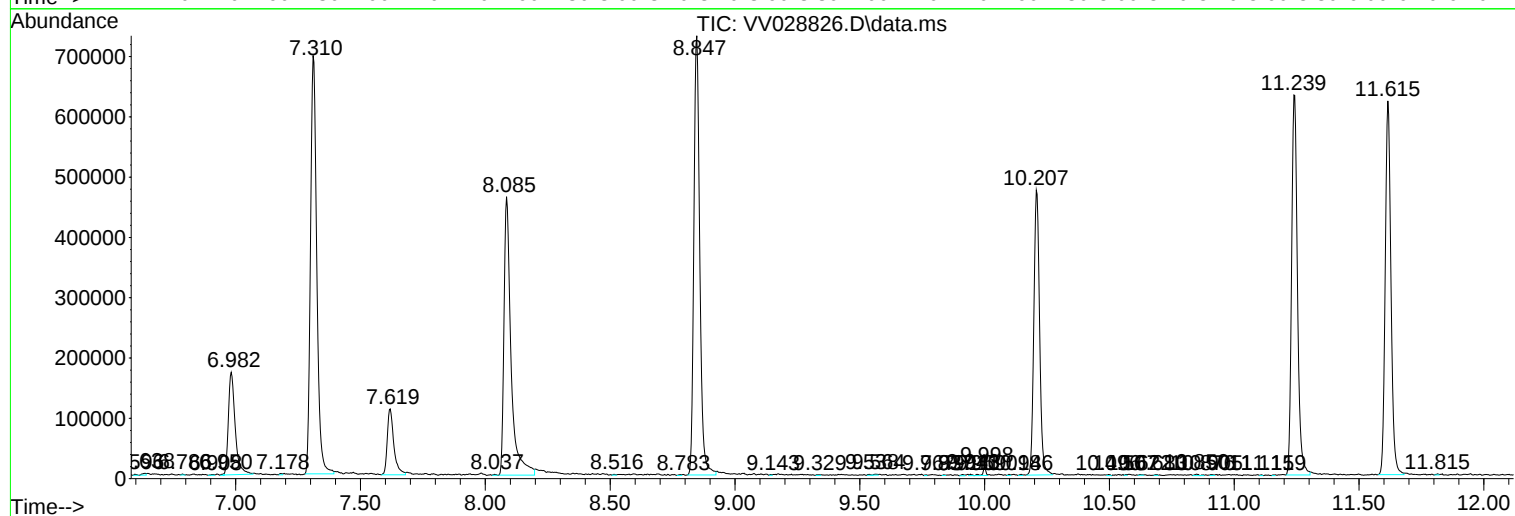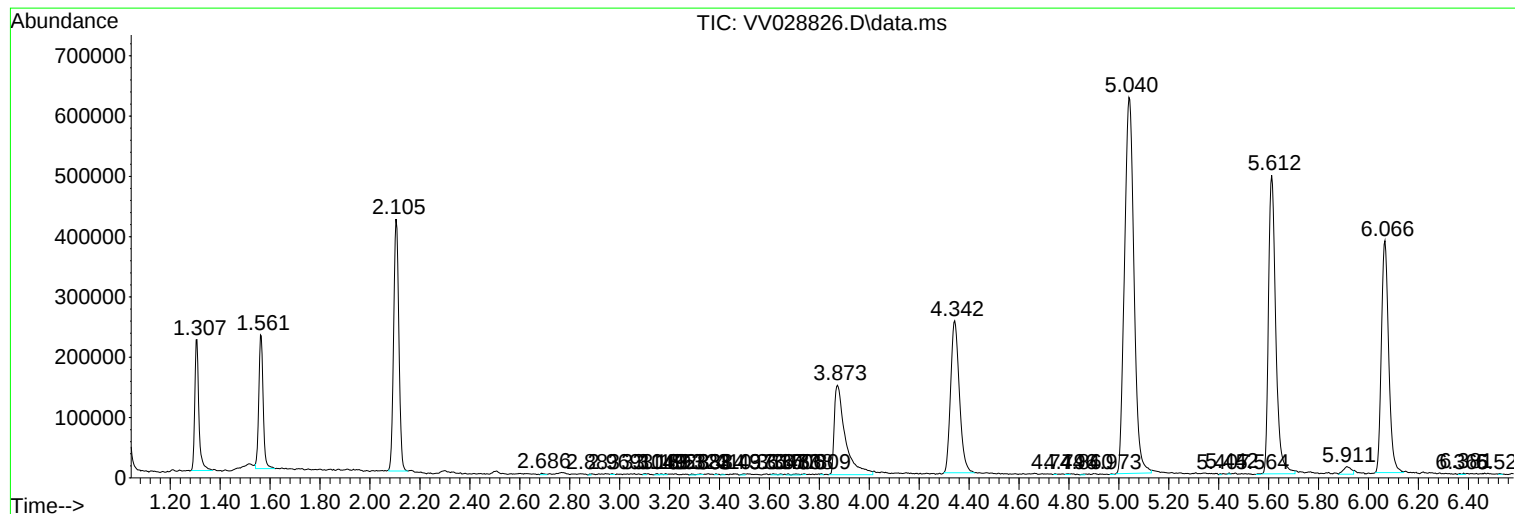

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110122\
Data File : VV028826.D
Acq On : 01 Nov 2022 19:40
Operator : SY/MD
Sample : N5354-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110122\
Data File : VV028826.D
Acq On : 01 Nov 2022 19:40
Operator : SY/MD
Sample : N5354-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc