
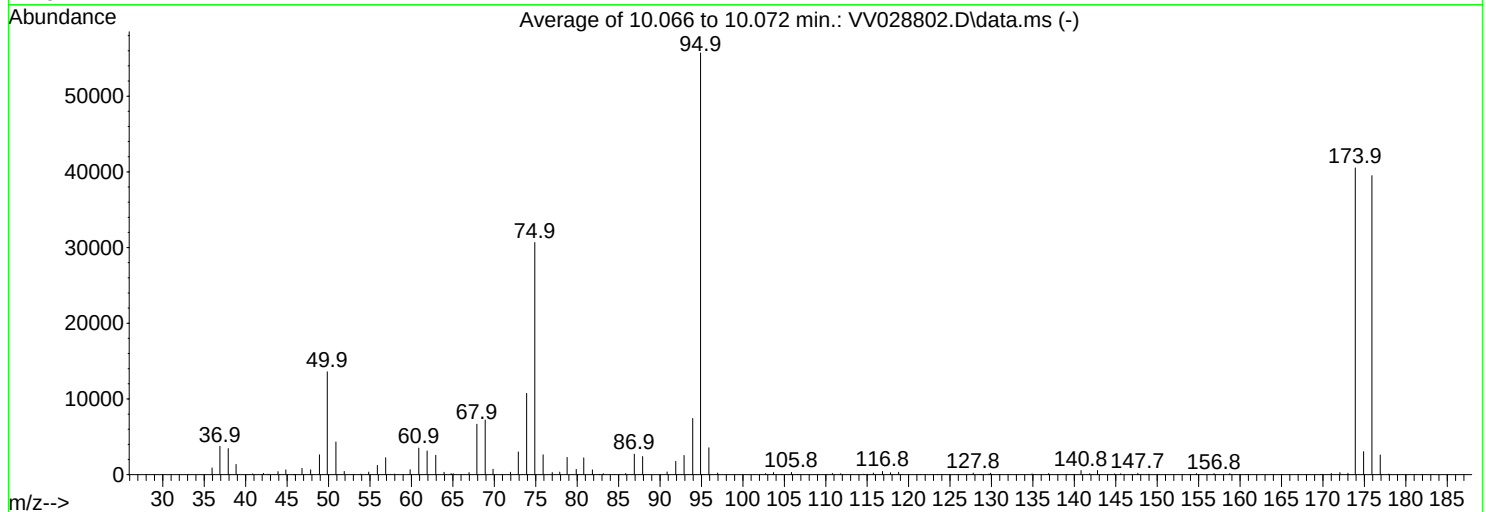


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110122\
 Data File : VV028802.D
 Acq On : 01 Nov 2022 09:28
 Operator : SY/MD
 Sample : BFB333
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB333

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis
 Last Update : Wed Nov 02 05:10:28 2022

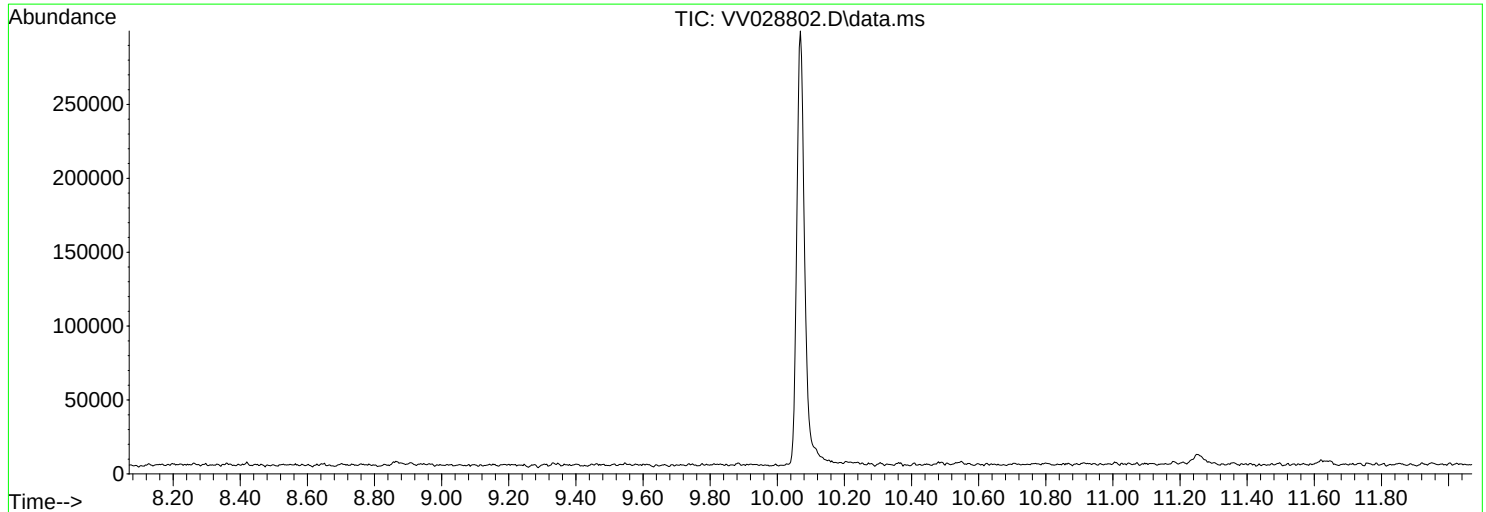

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.4	13587	PASS
75	95	30	80	55.0	30667	PASS
95	95	100	100	100.0	55725	PASS
96	95	5	9	6.4	3557	PASS
173	174	0.00	2	0.5	192	PASS
174	95	50	120	72.7	40520	PASS
175	174	5	9	7.5	3045	PASS
176	174	95	105	97.5	39499	PASS
177	176	5	10	6.6	2595	PASS

m/z	Abundance
35.30	229.0
36.00	214.0
37.00	177.0
38.10	153.0
38.80	162.0
39.90	1215.0
40.90	122.0
41.40	134.0
42.60	134.0
43.90	558.0
44.90	155.0
45.80	187.0
46.70	140.0
47.60	116.0
48.30	104.0
48.90	146.0
49.80	147.0
50.60	112.0
53.00	106.0
53.80	113.0
55.40	126.0
57.90	124.0
60.60	106.0
62.00	133.0
64.00	101.0
67.20	118.0
69.70	102.0
70.60	112.0
75.90	137.0
77.10	115.0
79.10	111.0
82.40	103.0
83.60	122.0
93.40	104.0
97.70	117.0
103.70	109.0
122.70	114.0
133.00	106.0
161.10	150.0

Instrument :
MSVOA_V
ClientSampleId :
BFB333

m/z	Abundance
35.10	123.0
35.90	1023.0
36.90	3953.0
37.90	3512.0
38.90	1606.0
39.90	848.0
40.90	244.0
42.20	164.0
42.90	186.0
43.90	884.0
44.90	756.0
45.80	173.0
46.80	978.0
47.80	661.0
48.90	2807.0
49.90	13813.0
50.90	4400.0
51.90	319.0
53.20	120.0
54.00	145.0
54.90	325.0
55.90	1145.0
56.90	2297.0
57.90	204.0
59.80	711.0
60.90	3446.0
61.90	3310.0
63.00	2599.0
64.00	445.0
64.80	247.0
67.00	328.0
67.90	6740.0
68.90	7442.0
69.90	755.0
72.00	298.0
72.90	3039.0
73.90	10619.0
74.90	30800.0
75.90	2821.0
77.00	388.0
77.90	319.0
78.80	2283.0
79.90	688.0
80.80	2259.0
81.90	606.0
82.70	122.0
83.10	116.0
84.50	109.0
85.90	149.0
86.90	2639.0
87.90	2498.0
90.80	352.0
91.90	1908.0
92.90	2646.0
93.90	7256.0
94.90	55528.0
95.90	3568.0
96.90	244.0
102.80	141.0
103.80	396.0
104.70	132.0
105.80	301.0
106.60	123.0
110.80	148.0
111.80	110.0
114.60	101.0
115.70	224.0
116.90	390.0
117.80	223.0
118.80	373.0
121.40	109.0
123.50	103.0
127.80	218.0
128.60	121.0
129.70	228.0
134.90	109.0
136.90	174.0
140.80	616.0
141.80	120.0
142.80	541.0
145.70	124.0
147.70	188.0
149.00	106.0
154.70	139.0
156.90	166.0
158.70	167.0
160.70	119.0
161.10	108.0
169.70	103.0
171.00	136.0
172.00	297.0
173.00	576.0

Instrument :
MSVOA_V
ClientSampleId :
BFB333

173.90	39664.0
174.90	3155.0
175.90	37816.0
176.90	2474.0
177.90	145.0

Instrument :
MSVOA_V
ClientSampleId :
BFB333

m/z	Abundance
35.90	1173.0
36.90	4008.0
37.90	3770.0
38.90	1602.0
39.80	916.0
40.80	239.0
41.60	155.0
42.20	178.0
42.80	208.0
43.90	977.0
44.90	793.0
45.80	197.0
46.90	1020.0
47.90	660.0
48.90	2875.0
49.90	14180.0
50.90	4507.0
51.90	442.0
53.20	131.0
53.90	139.0
54.10	138.0
54.80	354.0
55.90	1271.0
56.90	2337.0
58.00	210.0
59.80	643.0
60.90	3622.0
61.90	3356.0
63.00	2628.0
63.90	463.0
64.80	208.0
65.00	189.0
67.00	280.0
67.90	6871.0
68.90	7493.0
69.90	882.0
72.00	328.0
72.90	3114.0
73.90	11086.0
74.90	31592.0
76.00	2844.0
77.00	362.0
77.90	303.0
78.80	2316.0
79.90	729.0
80.80	2272.0
81.80	658.0
83.20	126.0
85.80	171.0
86.90	2805.0
87.90	2401.0
90.90	370.0
91.90	1786.0
92.90	2587.0
94.00	7771.0
94.90	57576.0
95.90	3609.0
97.00	237.0
102.70	174.0
103.80	382.0
105.80	313.0
110.80	185.0
111.80	127.0
115.00	122.0
115.80	225.0
116.80	449.0
117.80	234.0
118.80	328.0
127.80	220.0
129.90	261.0
134.90	123.0
136.90	160.0
139.20	100.0
140.80	568.0
141.90	135.0
142.80	582.0
144.90	128.0
145.60	140.0
147.70	184.0
148.90	113.0
154.80	169.0
156.80	173.0
158.70	173.0
161.10	113.0
169.90	103.0
171.00	171.0
172.10	306.0
173.90	42064.0
174.90	3126.0
175.90	41088.0
176.90	2679.0
178.00	104.0

Instrument :
MSVOA_V
ClientSampleId :
BFB333

m/z	Abundance
36.00	1094.0
36.90	3789.0
37.90	3524.0
38.90	1366.0
39.80	1070.0
40.80	216.0
41.60	187.0
42.10	194.0
42.70	229.0
43.90	1018.0
44.80	819.0
45.80	197.0
46.90	895.0
47.90	591.0
48.90	2624.0
49.90	13208.0
50.90	4058.0
51.90	496.0
53.20	123.0
53.80	140.0
54.80	333.0
55.90	1275.0
56.90	2086.0
58.10	215.0
59.90	590.0
60.90	3463.0
61.90	3097.0
62.90	2475.0
63.90	353.0
65.10	187.0
66.80	231.0
67.90	6362.0
68.90	6769.0
69.90	843.0
71.90	361.0
72.90	2843.0
73.90	10521.0
74.90	29608.0
76.00	2633.0
77.00	396.0
77.90	398.0
78.80	2234.0
79.90	680.0
80.80	2138.0
81.80	656.0
83.10	114.0
83.50	123.0
85.80	143.0
86.90	2649.0
87.90	2279.0
90.90	358.0
91.90	1592.0
92.90	2405.0
94.00	7249.0
94.90	54072.0
95.90	3494.0
97.00	183.0
102.70	137.0
103.70	368.0
105.90	297.0
106.90	104.0
110.80	182.0
111.80	150.0
114.60	105.0
115.80	193.0
116.80	461.0
117.80	276.0
118.80	284.0
127.80	216.0
128.80	128.0
129.90	300.0
131.00	104.0
134.90	116.0
136.90	107.0
140.00	154.0
140.80	489.0
141.80	145.0
142.80	537.0
144.80	165.0
145.50	153.0
147.60	182.0
154.80	149.0
156.80	136.0
158.80	132.0
171.00	158.0
172.10	259.0
173.90	39832.0
174.90	2853.0
175.90	39592.0
176.90	2631.0

Instrument :
MSVOA_V
ClientSampleId :
BFB333