




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112322\
 Data File : VV029321.D
 Acq On : 24 Nov 2022 02:22
 Operator : SY/MD
 Sample : N5725-16
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHB69

Manual IntegrationsAPPROVED

Quant Time: Nov 24 03:42:57 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Nov 24 01:40:30 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 11/25/2022
 Supervised By :Mahesh Dadoda 11/25/2022

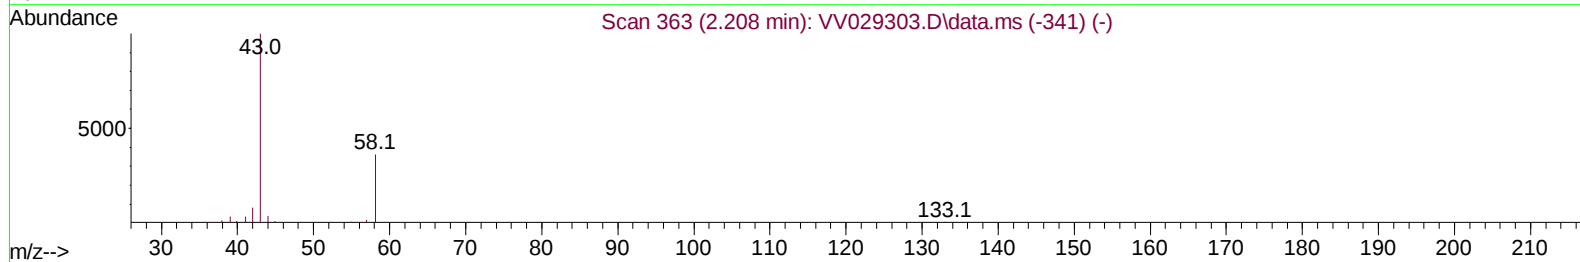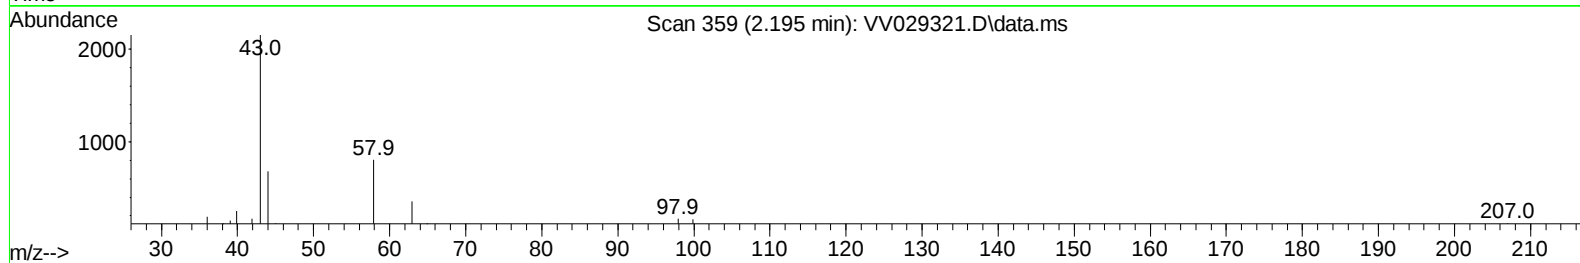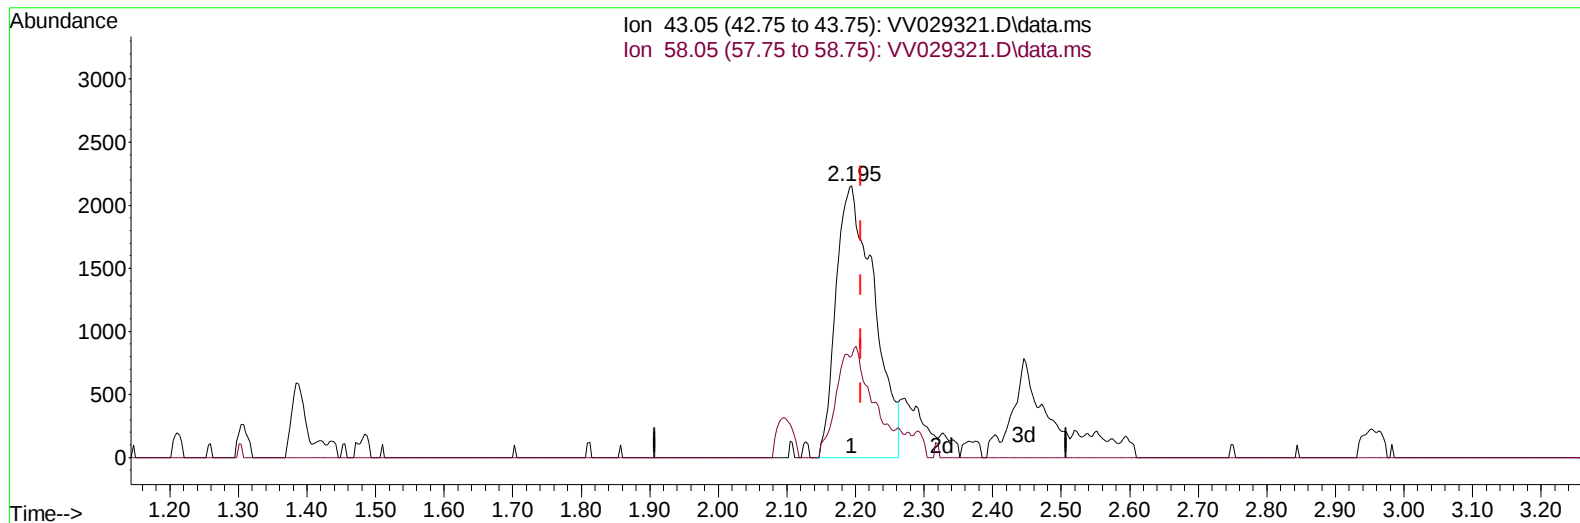

TIC: VV029321.D\data.ms

(13) Acetone (T)

2.195min (-0.013) 3.79 ug/L

response 8295

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	35.40	15.24
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112322\
Data File : VV029321.D
Acq On : 24 Nov 2022 02:22
Operator : SY/MD
Sample : N5725-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHB69

Manual IntegrationsAPPROVED

Quant Time: Nov 24 03:42:57 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Nov 24 01:40:30 2022
Response via : Initial Calibration

Reviewed By :John Carlone 11/25/2022
Supervised By :Mahesh Dadoda 11/25/2022

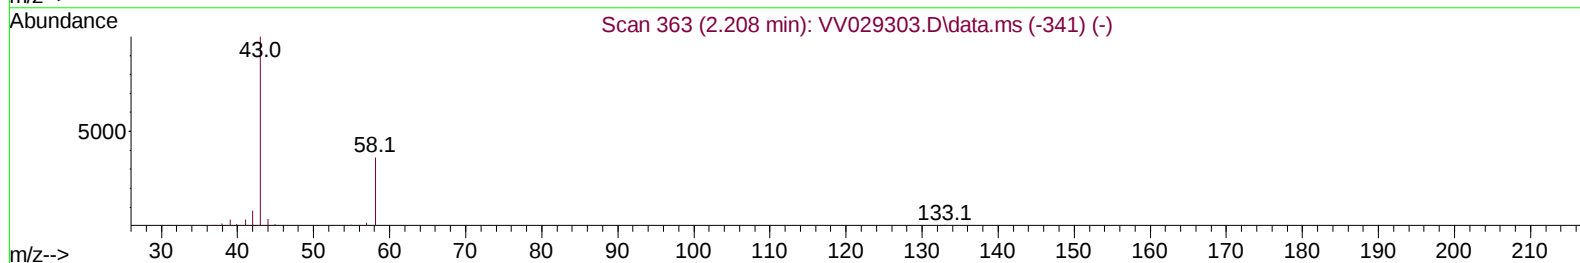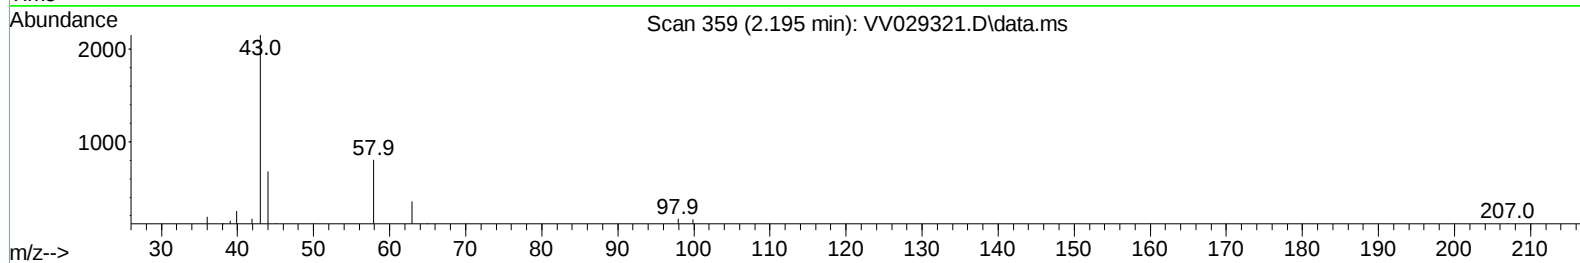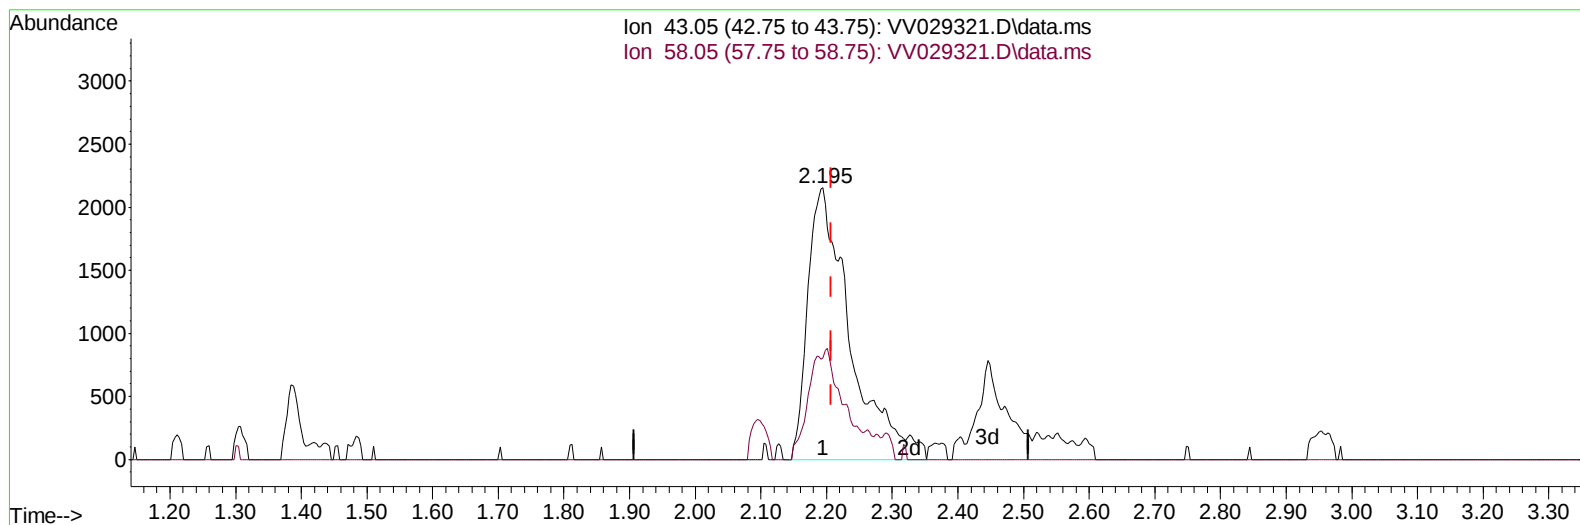

TIC: VV029321.D\data.ms

(13) Acetone (T)

2.195min (-0.013) 4.41 ug/L m

response 9662

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	35.40	13.08
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112322\
 Data File : VV029321.D
 Acq On : 24 Nov 2022 02:22
 Operator : SY/MD
 Sample : N5725-16
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHB69

Manual IntegrationsAPPROVED

Quant Time: Nov 24 03:42:57 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Nov 24 01:40:30 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 11/25/2022
 Supervised By :Mahesh Dadoda 11/25/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.609	114		292504	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.844	117		260131	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.239	152		133638	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.304	65		87390	4.855	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130		Recovery	=	97.000%	
7) Chloroethane-d5	1.565	69		67841	5.148	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130		Recovery	=	103.000%	
11) 1,1-Dichloroethene-d2	2.105	63		107567	3.734	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125		Recovery	=	74.600%	
20) 2-Butanone-d5	3.896	46		156678	52.030	ug/L	-0.02
Spiked Amount 50.000	Range 40	- 130		Recovery	=	104.060%	
24) Chloroform-d	4.339	84		157457	4.901	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	98.000%	
26) 1,2-Dichloroethane-d4	5.024	65		75262	5.324	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	106.400%	
32) Benzene-d6	5.044	84		355429	4.944	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	98.800%	
36) 1,2-Dichloropropane-d6	6.063	67		103449	5.121	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140		Recovery	=	102.400%	
41) Toluene-d8	7.307	98		331969	4.892	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	97.800%	
43) trans-1,3-Dichloroprop...	7.616	79		37332	4.793	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130		Recovery	=	95.800%	
46) 2-Hexanone-d5	8.085	63		136471	49.155	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130		Recovery	=	98.320%	
56) 1,1,2,2-Tetrachloroeth...	10.207	84		64635	5.185	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120		Recovery	=	103.800%	
66) 1,2-Dichlorobenzene-d4	11.612	152		123816	5.304	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120		Recovery	=	106.000%	
Target Compounds							
13) Acetone	2.195	43		9662m	4.413	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112322\
Data File : VV029321.D
Acq On : 24 Nov 2022 02:22
Operator : SY/MD
Sample : N5725-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 3

Instrument :
MSVOA_V
ClientSampleId :
BHB69

Manual IntegrationsAPPROVED

Quant Time: Nov 24 03:42:57 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Nov 24 01:40:30 2022
Response via : Initial Calibration

Reviewed By :John Carlone 11/25/2022
Supervised By :Mahesh Dadoda 11/25/2022

