




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112322\
 Data File : VV029322.D
 Acq On : 24 Nov 2022 02:47
 Operator : SY/MD
 Sample : N5725-17
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHB70

Manual IntegrationsAPPROVED

Quant Time: Nov 24 03:43:11 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Nov 24 01:40:30 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 11/25/2022
 Supervised By :Mahesh Dadoda 11/25/2022

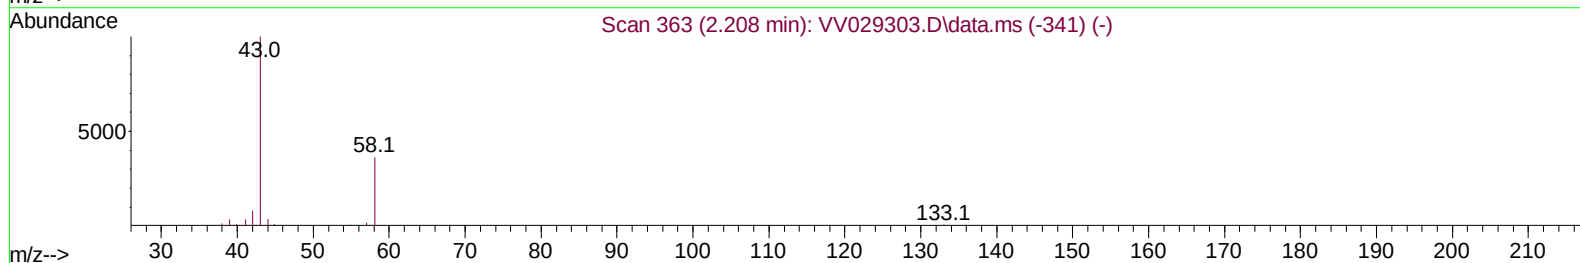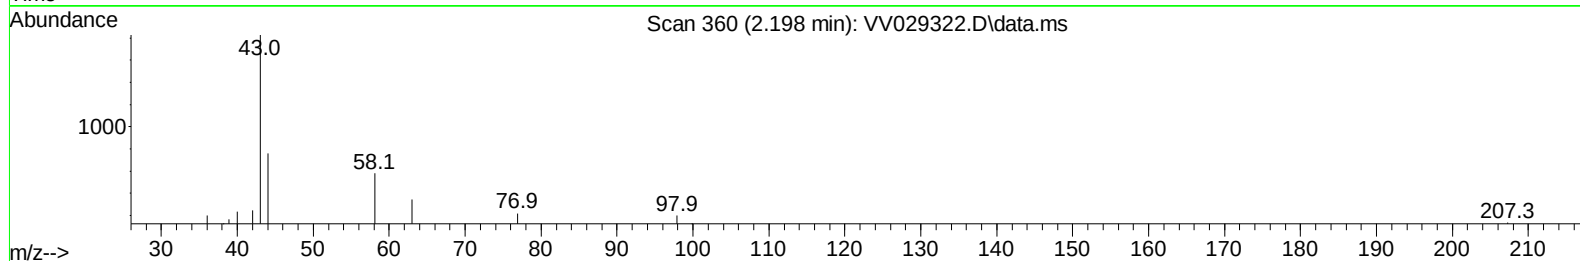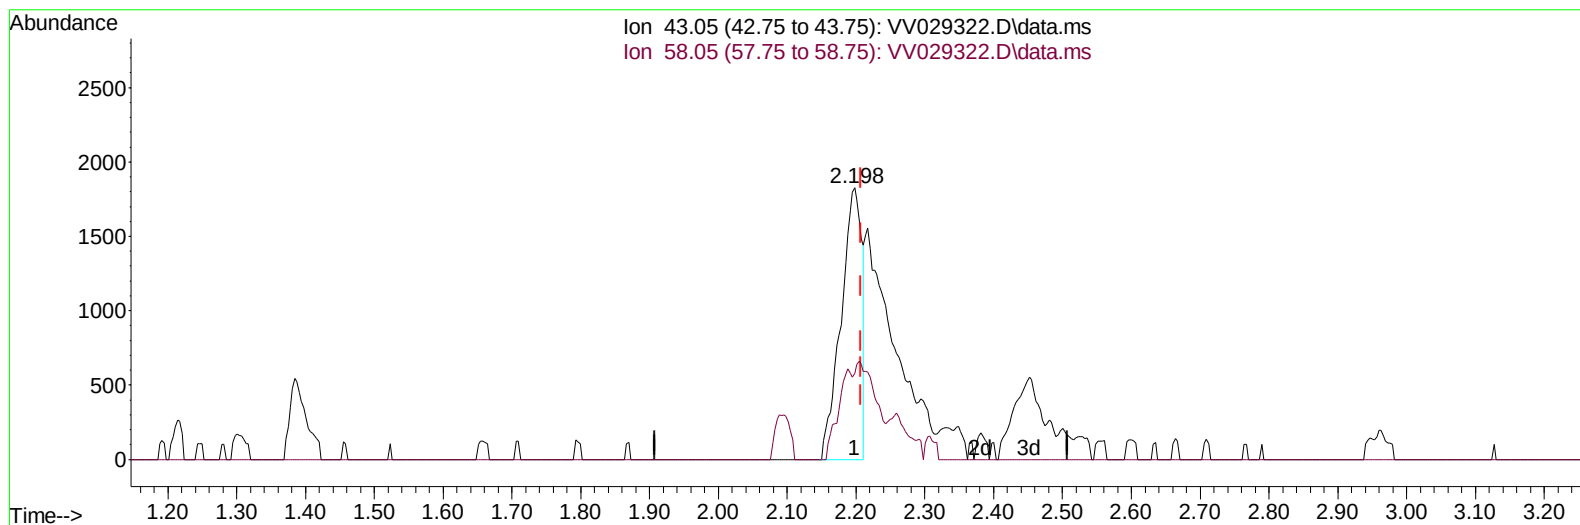

TIC: VV029322.D\data.ms

(13) Acetone (T)

2.198min (-0.010) 1.92 ug/L

response 3851

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	35.40	36.67
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112322\
 Data File : VV029322.D
 Acq On : 24 Nov 2022 02:47
 Operator : SY/MD
 Sample : N5725-17
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHB70

Manual IntegrationsAPPROVED

Quant Time: Nov 24 03:43:11 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Nov 24 01:40:30 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 11/25/2022
 Supervised By :Mahesh Dadoda 11/25/2022

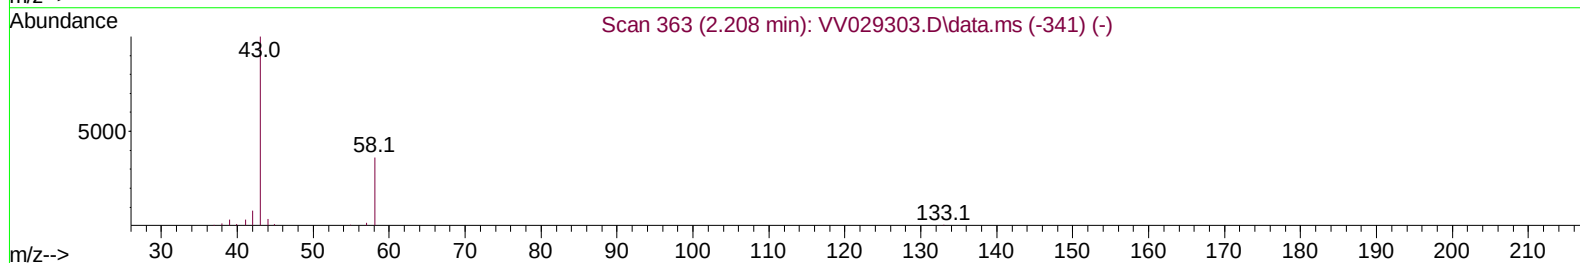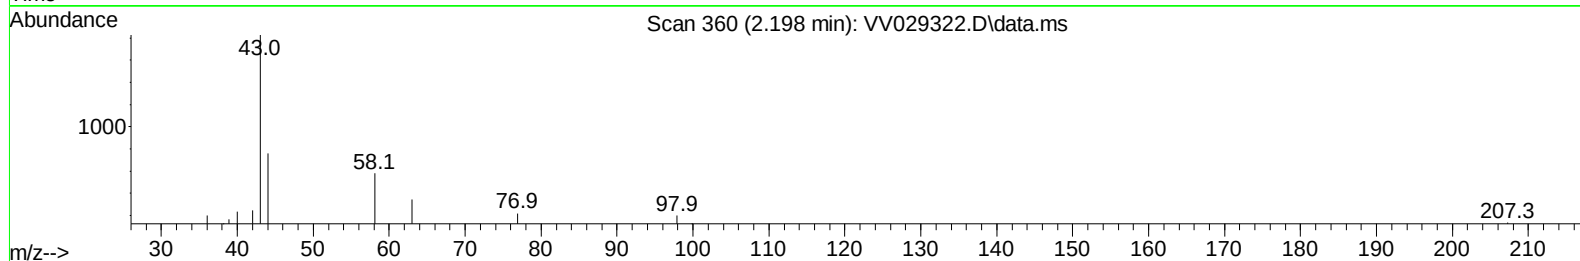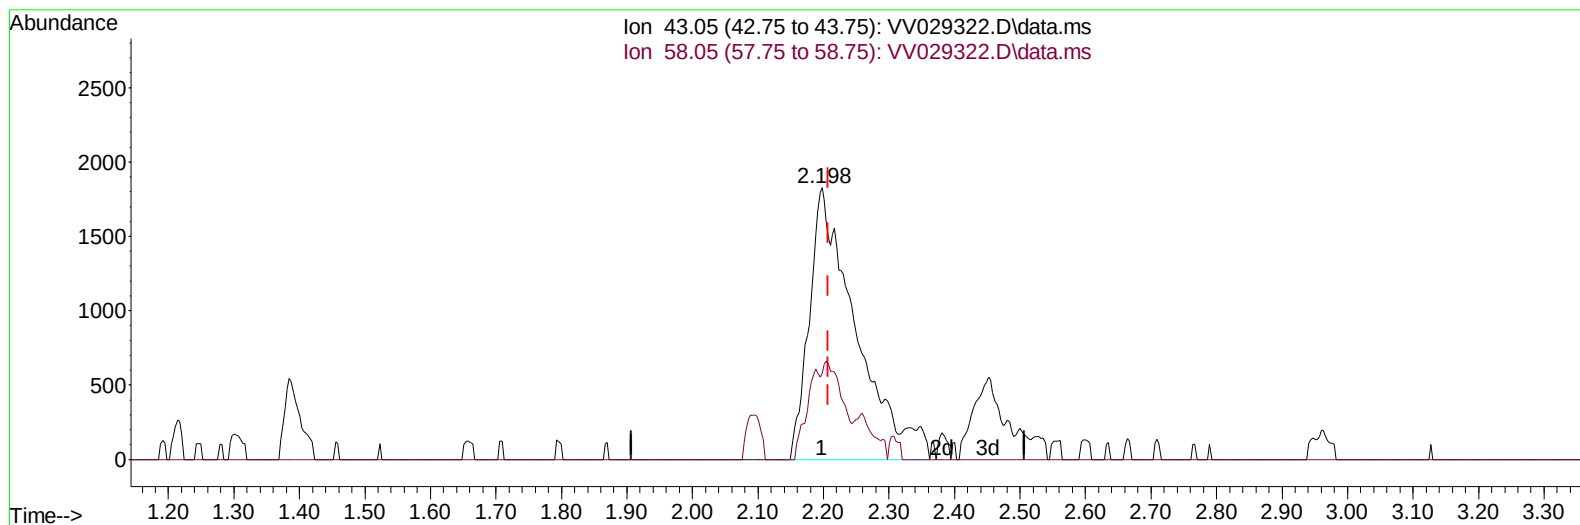

TIC: VV029322.D\data.ms

(13) Acetone (T)

2.198min (-0.010) 4.48 ug/L m

response 8997

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	35.40	15.69
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112322\
 Data File : VV029322.D
 Acq On : 24 Nov 2022 02:47
 Operator : SY/MD
 Sample : N5725-17
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHB70

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 11/25/2022
 Supervised By :Mahesh Dadoda 11/25/2022

Quant Time: Nov 24 03:43:11 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Nov 24 01:40:30 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.609	114		268053	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.844	117		242278	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.239	152		124248	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.304	65		73531	4.458	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130		Recovery	=	89.200%	
7) Chloroethane-d5	1.564	69		56525	4.681	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130		Recovery	=	93.600%	
11) 1,1-Dichloroethene-d2	2.105	63		88060	3.336	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125		Recovery	=	66.800%	
20) 2-Butanone-d5	3.905	46		143659	52.058	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130		Recovery	=	104.120%	
24) Chloroform-d	4.339	84		137473	4.669	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	93.400%	
26) 1,2-Dichloroethane-d4	5.027	65		67808	5.234	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	104.600%	
32) Benzene-d6	5.043	84		306829	4.582	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	91.600%	
36) 1,2-Dichloropropane-d6	6.063	67		87900	4.672	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140		Recovery	=	93.400%	
41) Toluene-d8	7.307	98		284191	4.497	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	90.000%	
43) trans-1,3-Dichloroprop...	7.616	79		32221	4.442	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130		Recovery	=	88.800%	
46) 2-Hexanone-d5	8.085	63		132333	51.177	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130		Recovery	=	102.360%	
56) 1,1,2,2-Tetrachloroeth...	10.207	84		60400	5.202	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120		Recovery	=	104.000%	
66) 1,2-Dichlorobenzene-d4	11.612	152		108980	5.021	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120		Recovery	=	100.400%	
Target Compounds							
13) Acetone	2.198	43		8997m	4.484	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112322\
Data File : VV029322.D
Acq On : 24 Nov 2022 02:47
Operator : SY/MD
Sample : N5725-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 3

Instrument :
MSVOA_V
ClientSampleId :
BHB70

Manual IntegrationsAPPROVED

Quant Time: Nov 24 03:43:11 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Nov 24 01:40:30 2022
Response via : Initial Calibration

Reviewed By :John Carlone 11/25/2022
Supervised By :Mahesh Dadoda 11/25/2022

