

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW112322\
 Data File : VW029321.D
 Acq On : 24 Nov 2022 02:22
 Operator : SY/MD
 Sample : N5725-16
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHB69

Manual Integrations
 APPROVED

Reviewed By : John Carlone 11/25/2022
 Supervised By : Mahesh Dadoda 11/25/2022

Quant Time: Nov 24 03:42:57 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Nov 24 01:40:30 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	292504	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.844	117	260131	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.239	152	133638	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	87390	4.855	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	97.000%	
7) Chloroethane-d5	1.565	69	67841	5.148	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	103.000%	
11) 1,1-Dichloroethene-d2	2.105	63	107567	3.734	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	74.600%	
20) 2-Butanone-d5	3.896	46	156678	52.030	ug/L	-0.02
Spiked Amount	50.000	Range 40 - 130	Recovery	=	104.060%	
24) Chloroform-d	4.339	84	157457	4.901	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	98.000%	
26) 1,2-Dichloroethane-d4	5.024	65	75262	5.324	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	106.400%	
32) Benzene-d6	5.044	84	355429	4.944	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	98.800%	
36) 1,2-Dichloropropane-d6	6.063	67	103449	5.121	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	102.400%	
41) Toluene-d8	7.307	98	331969	4.892	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	97.800%	
43) trans-1,3-Dichloroprop...	7.616	79	37332	4.793	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	95.800%	
46) 2-Hexanone-d5	8.085	63	136471	49.155	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	98.320%	
56) 1,1,2,2-Tetrachloroeth...	10.207	84	64635	5.185	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	103.800%	
66) 1,2-Dichlorobenzene-d4	11.612	152	123816	5.304	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	106.000%	
Target Compounds					Qvalue	
13) Acetone	2.195	43	9662m	4.413	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112322\
Data File : VV029321.D
Acq On : 24 Nov 2022 02:22
Operator : SY/MD
Sample : N5725-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
BHB69

Manual Integrations
APPROVED

Reviewed By :John Carlone 11/25/2022
Supervised By :Mahesh Dadoda 11/25/2022


Quant Time: Nov 24 03:42:57 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Nov 24 01:40:30 2022
Response via : Initial Calibration

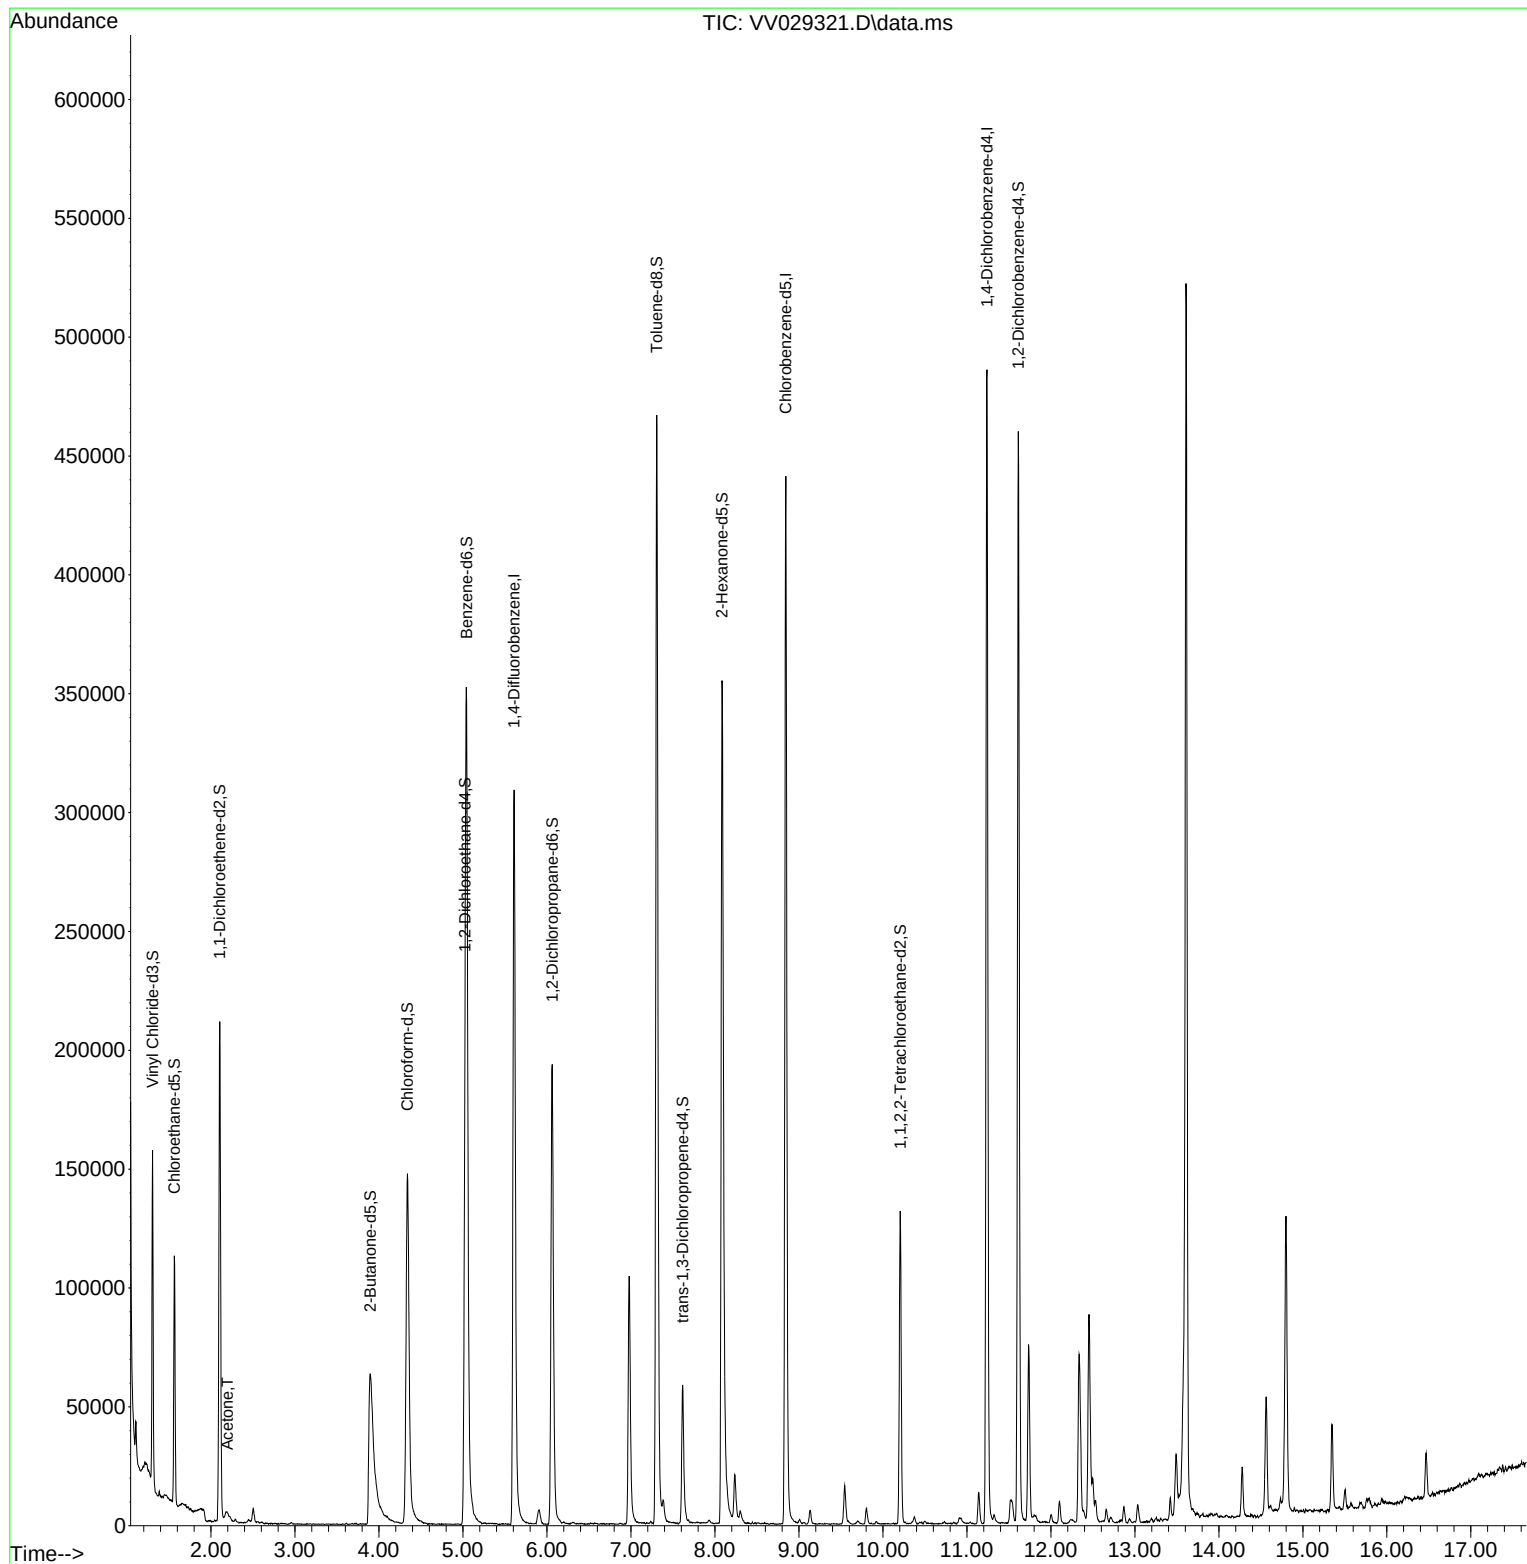

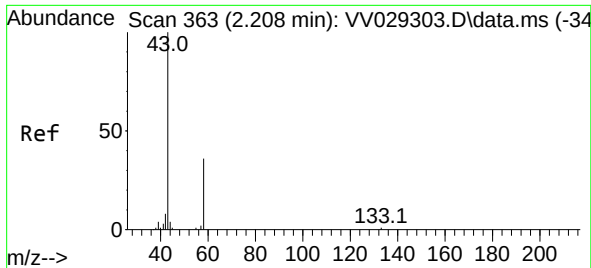

#13
 Acetone
 Concen: 4.413 ug/L m
 RT: 2.195 min Scan# 31
 Delta R.T. -0.013 min
 Lab File: VV029321.D
 Acq: 24 Nov 2022 02:22

Instrument :
 MSVOA_V
 ClientSampleId :
 BHB69

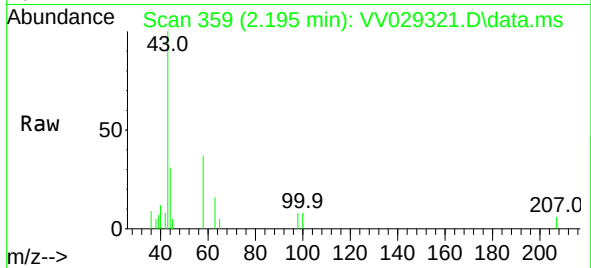

Tgt Ion: 43 Resp: 966
 Ion Ratio Lower Upper
 43 100
 58 13.1 0.0 70.8

Manual Integrations
 APPROVED

Reviewed By :John Carlone 11/25/2022
 Supervised By :Mahesh Dadoda 11/25/2022

