

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112322\
 Data File : VV029305.D
 Acq On : 23 Nov 2022 19:50
 Operator : SY/MD
 Sample : N5680-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV029305.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	101	rVB	147549	157796	18.13%	2.150%
2	1.565	156	163	177	rVB	103877	119639	13.75%	1.630%
3	2.105	320	331	346	rBV	203965	293977	33.78%	4.006%
4	3.909	877	892	941	rBV2	49696	259972	29.87%	3.542%
5	4.339	1009	1026	1053	rBV2	136300	355684	40.87%	4.846%
6	5.040	1227	1244	1277	rBV2	343690	870304	100.00%	11.859%
7	5.609	1407	1421	1459	rBV	318732	649866	74.67%	8.855%
8	5.902	1499	1512	1529	rVB7	6600	15286	1.76%	0.208%
9	6.063	1548	1562	1589	rBV	185704	391096	44.94%	5.329%
10	6.979	1836	1847	1872	rBV	101297	193888	22.28%	2.642%
11	7.307	1937	1949	1967	rBV	449828	802356	92.19%	10.933%
12	7.616	2035	2045	2068	rBV	58377	106334	12.22%	1.449%
13	8.088	2179	2192	2224	rBV3	336789	708899	81.45%	9.659%
14	8.844	2414	2427	2448	rBV	447197	741609	85.21%	10.105%
15	10.207	2839	2851	2870	rBV	127817	202950	23.32%	2.765%
16	10.374	2892	2903	2915	rBV	6458	10712	1.23%	0.146%
17	11.239	3160	3172	3195	rBV	491242	755849	86.85%	10.299%
18	11.612	3276	3288	3310	rBV	426632	679298	78.05%	9.256%
19	11.796	3337	3345	3357	rBV3	6683	11093	1.27%	0.151%
20	15.368	4449	4456	4465	rVB8	9008	12445	1.43%	0.170%




Sum of corrected areas: 7339053

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112322\
Data File : VV029305.D
Acq On : 23 Nov 2022 19:50
Operator : SY/MD
Sample : N5680-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

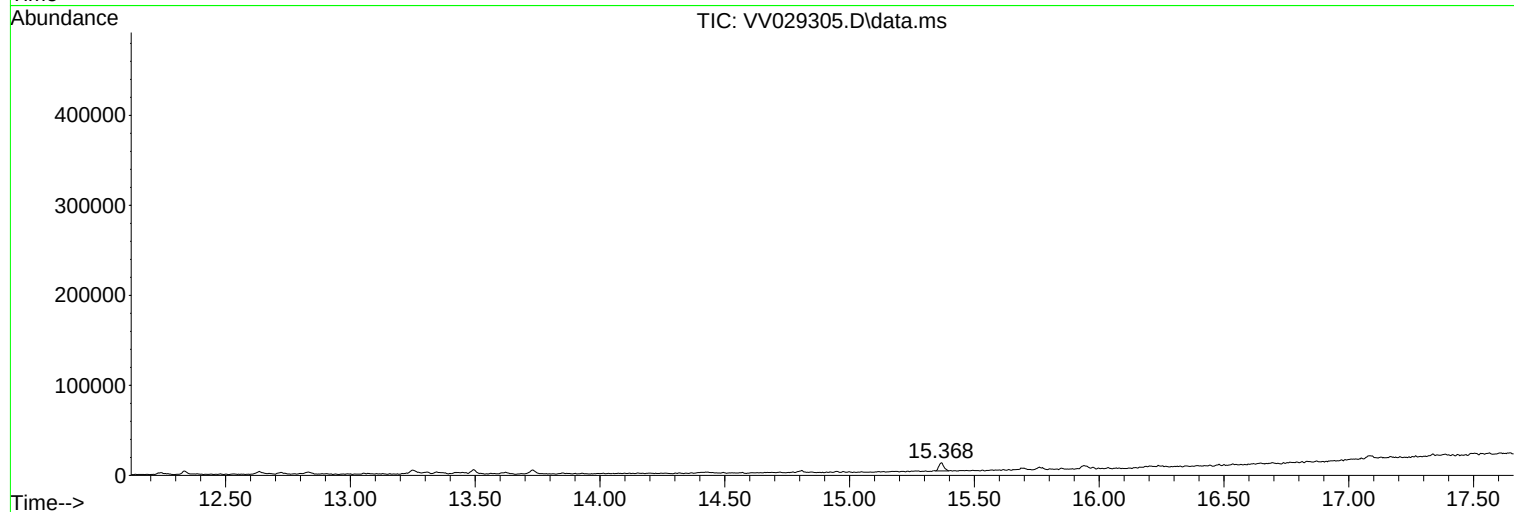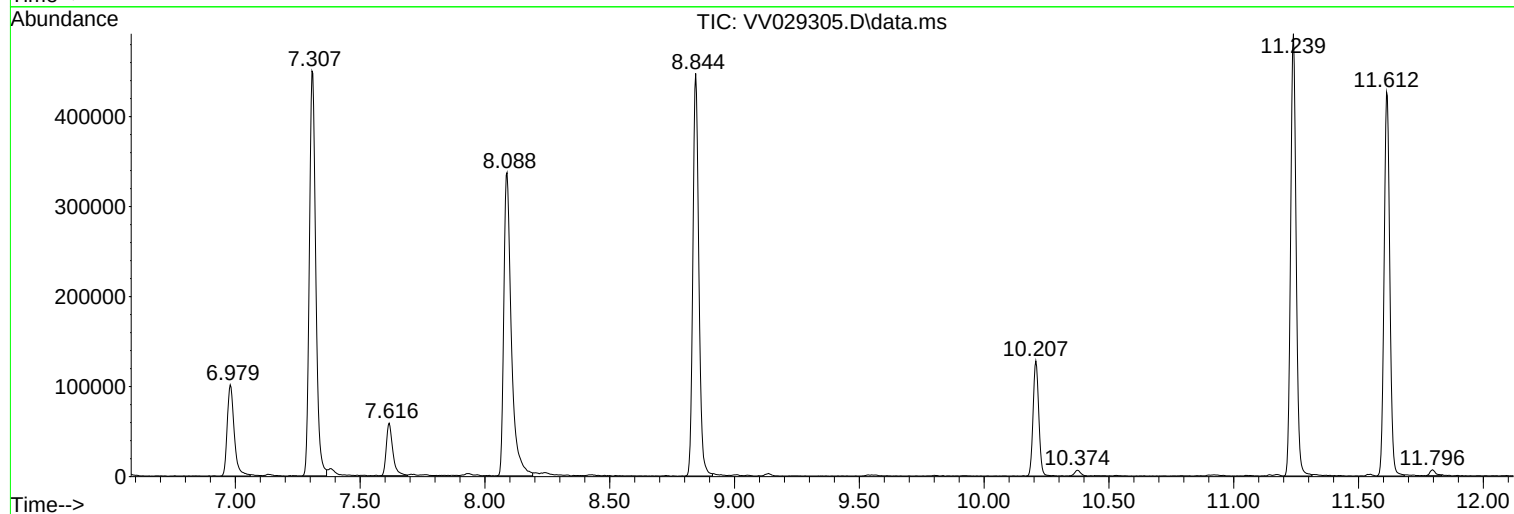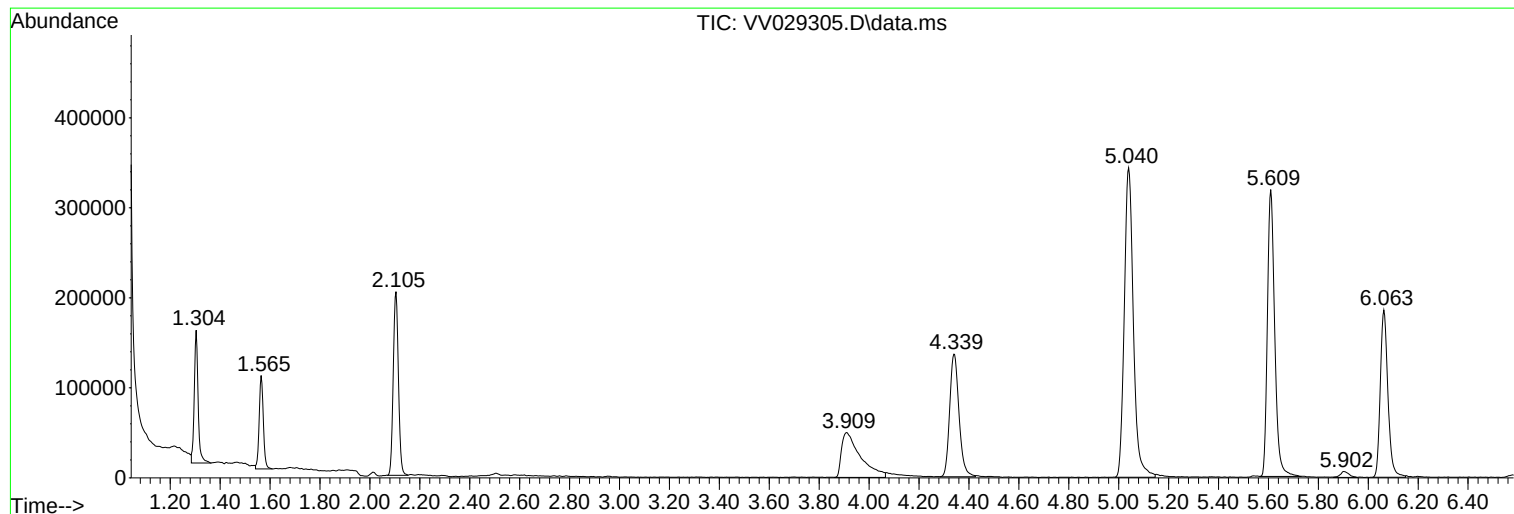

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112322\
Data File : VV029305.D
Acq On : 23 Nov 2022 19:50
Operator : SY/MD
Sample : N5680-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112322\
Data File : VV029305.D
Acq On : 23 Nov 2022 19:50
Operator : SY/MD
Sample : N5680-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
