

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112322\
 Data File : VV029316.D
 Acq On : 24 Nov 2022 00:20
 Operator : SY/MD
 Sample : N5652-18
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV029316.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	94	rVB	141406	146420	17.04%	2.070%
2	1.565	156	163	172	rVB	100122	112291	13.07%	1.587%
3	2.105	320	331	346	rBV	201355	290539	33.82%	4.107%
4	3.905	875	891	934	rBV	56524	257628	29.99%	3.642%
5	4.339	1008	1026	1050	rBV	135880	341751	39.78%	4.831%
6	5.040	1225	1244	1283	rBV2	337728	859064	100.00%	12.143%
7	5.609	1408	1421	1463	rBV	295359	609441	70.94%	8.614%
8	5.908	1502	1514	1529	rBV7	7375	17358	2.02%	0.245%
9	6.063	1548	1562	1589	rBV	186724	388669	45.24%	5.494%
10	6.979	1835	1847	1869	rBV	99153	186033	21.66%	2.630%
11	7.310	1936	1950	1969	rBV	444923	789270	91.88%	11.156%
12	7.616	2035	2045	2067	rBV	55979	102258	11.90%	1.445%
13	7.934	2131	2144	2153	rBV3	5767	10333	1.20%	0.146%
14	8.088	2177	2192	2227	rBV2	339974	704075	81.96%	9.952%
15	8.844	2415	2427	2450	rBV	414978	692129	80.57%	9.783%
16	10.207	2840	2851	2869	rBV	125314	196978	22.93%	2.784%
17	10.374	2889	2903	2918	rBV	19613	31701	3.69%	0.448%
18	11.239	3159	3172	3200	rBV	427584	672178	78.25%	9.501%
19	11.542	3255	3266	3276	rBV	12729	21850	2.54%	0.309%
20	11.612	3276	3288	3312	rVB	398698	634798	73.89%	8.973%
21	12.239	3470	3483	3495	rBV2	5670	9906	1.15%	0.140%




Sum of corrected areas: 7074670

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112322\
Data File : VV029316.D
Acq On : 24 Nov 2022 00:20
Operator : SY/MD
Sample : N5652-18
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

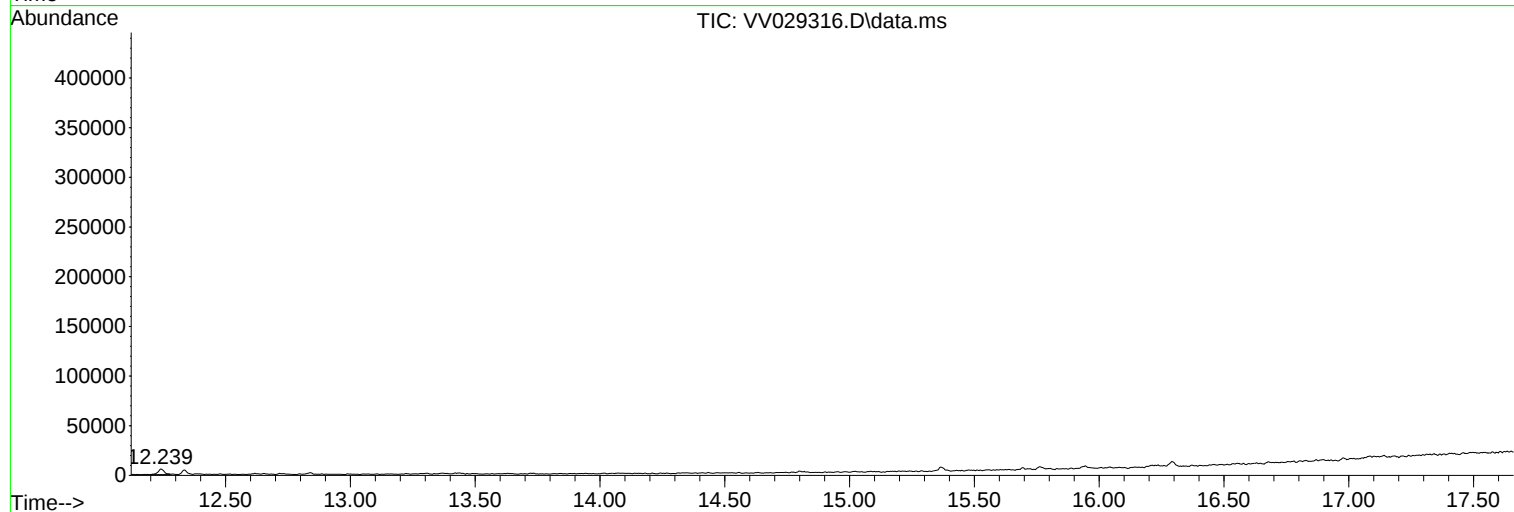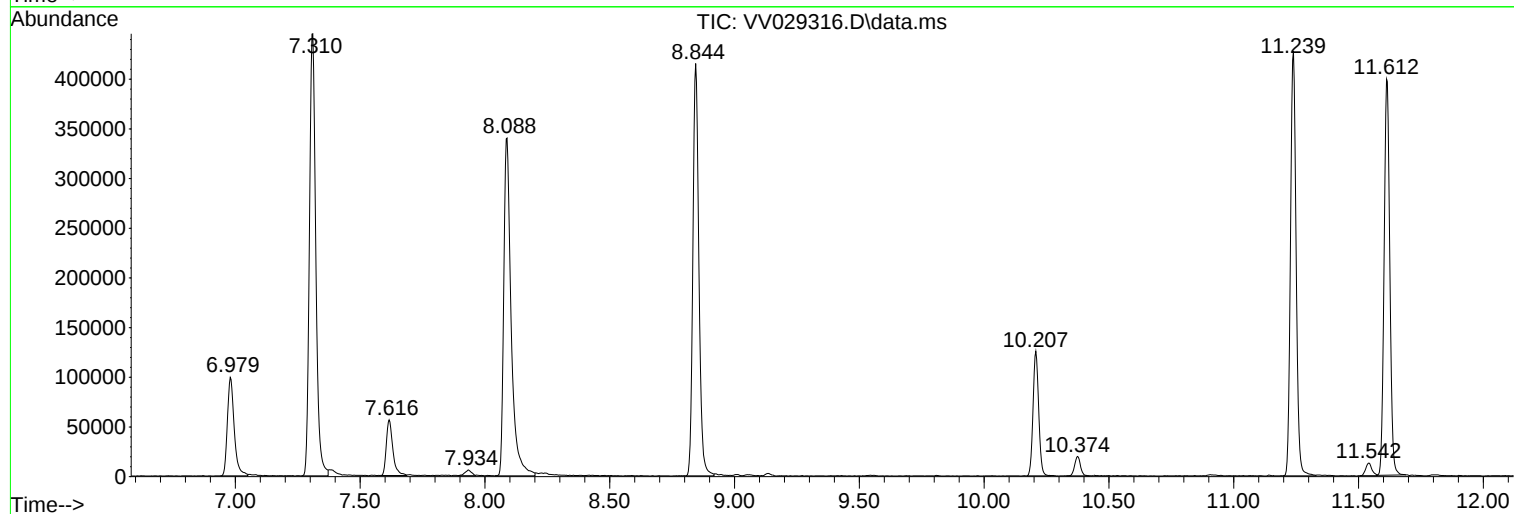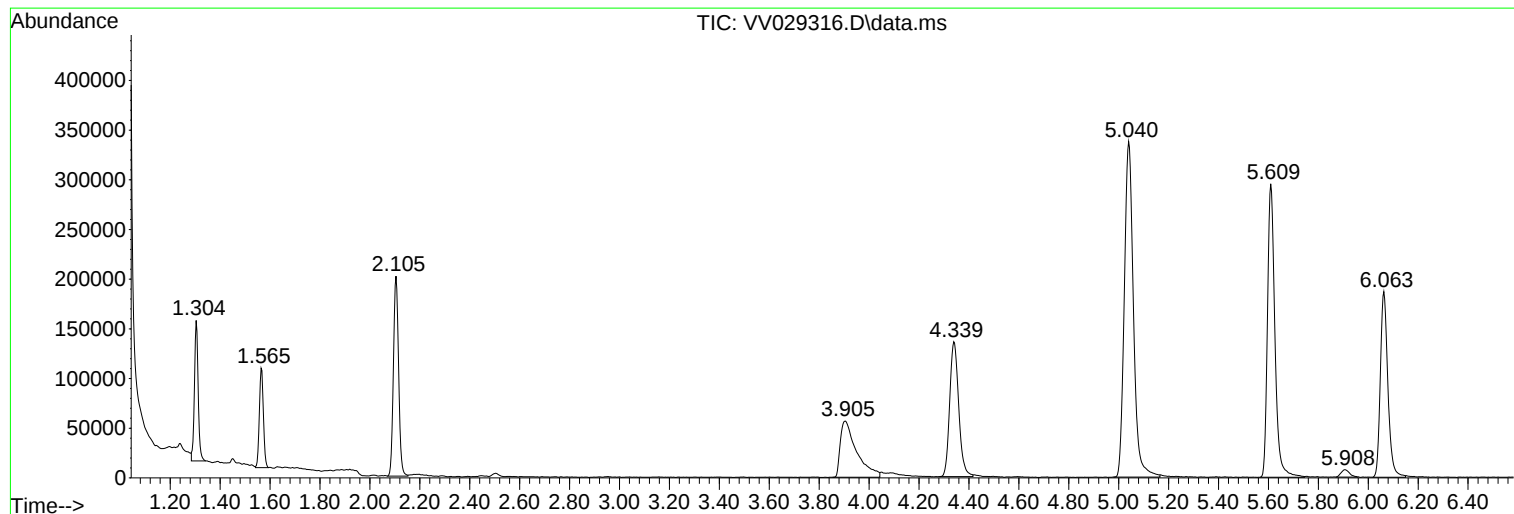

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112322\
Data File : VV029316.D
Acq On : 24 Nov 2022 00:20
Operator : SY/MD
Sample : N5652-18
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112322\
Data File : VV029316.D
Acq On : 24 Nov 2022 00:20
Operator : SY/MD
Sample : N5652-18
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc