

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112322\
 Data File : VV029325.D
 Acq On : 24 Nov 2022 04:25
 Operator : SY/MD
 Sample : VV1123WBL02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK277

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV029325.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	102	rVB	148823	154353	17.25%	2.142%
2	1.565	156	163	175	rVB	104832	118382	13.23%	1.643%
3	2.105	318	331	345	rBV	212514	303686	33.95%	4.215%
4	3.902	877	890	921	rBV2	39072	161114	18.01%	2.236%
5	4.339	1008	1026	1055	rBV2	139272	356646	39.87%	4.950%
6	5.040	1220	1244	1291	rBV2	346639	894604	100.00%	12.415%
7	5.609	1406	1421	1453	rBV	296029	613488	68.58%	8.514%
8	5.905	1497	1513	1528	rVB5	4304	9465	1.06%	0.131%
9	6.063	1548	1562	1591	rBV	188997	397413	44.42%	5.515%
10	6.979	1833	1847	1875	rBV	100371	191777	21.44%	2.661%
11	7.310	1934	1950	1982	rBV	451872	824608	92.18%	11.444%
12	7.616	2030	2045	2067	rBV2	56570	105014	11.74%	1.457%
13	8.085	2179	2191	2253	rBV2	283991	711016	79.48%	9.868%
14	8.844	2415	2427	2460	rBV	420809	706479	78.97%	9.805%
15	10.207	2837	2851	2873	rBV	124580	208605	23.32%	2.895%
16	11.239	3160	3172	3194	rBV	459879	718924	80.36%	9.977%
17	11.612	3275	3288	3311	rBV	433798	693984	77.57%	9.631%
18	13.493	3866	3873	3883	rVB2	5812	9475	1.06%	0.131%
19	13.612	3900	3910	3922	rVB	8306	14210	1.59%	0.197%
20	15.355	4442	4452	4461	rBV5	6475	12376	1.38%	0.172%




Sum of corrected areas: 7205619

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112322\
Data File : VV029325.D
Acq On : 24 Nov 2022 04:25
Operator : SY/MD
Sample : VV1123WBL02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK277

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

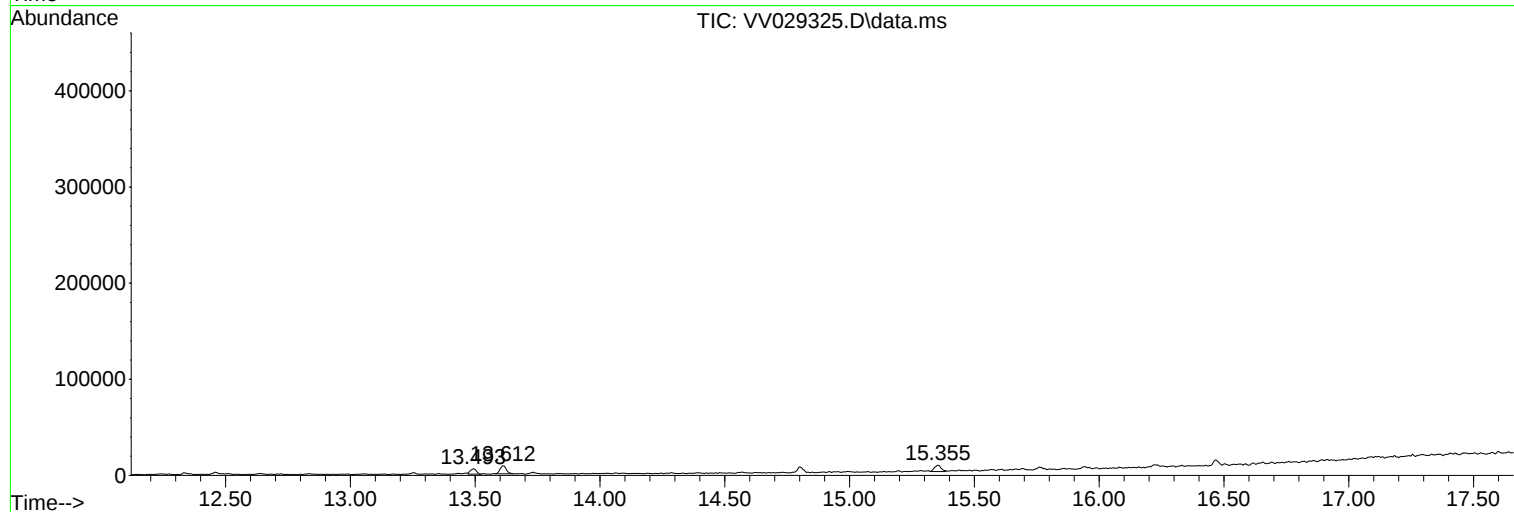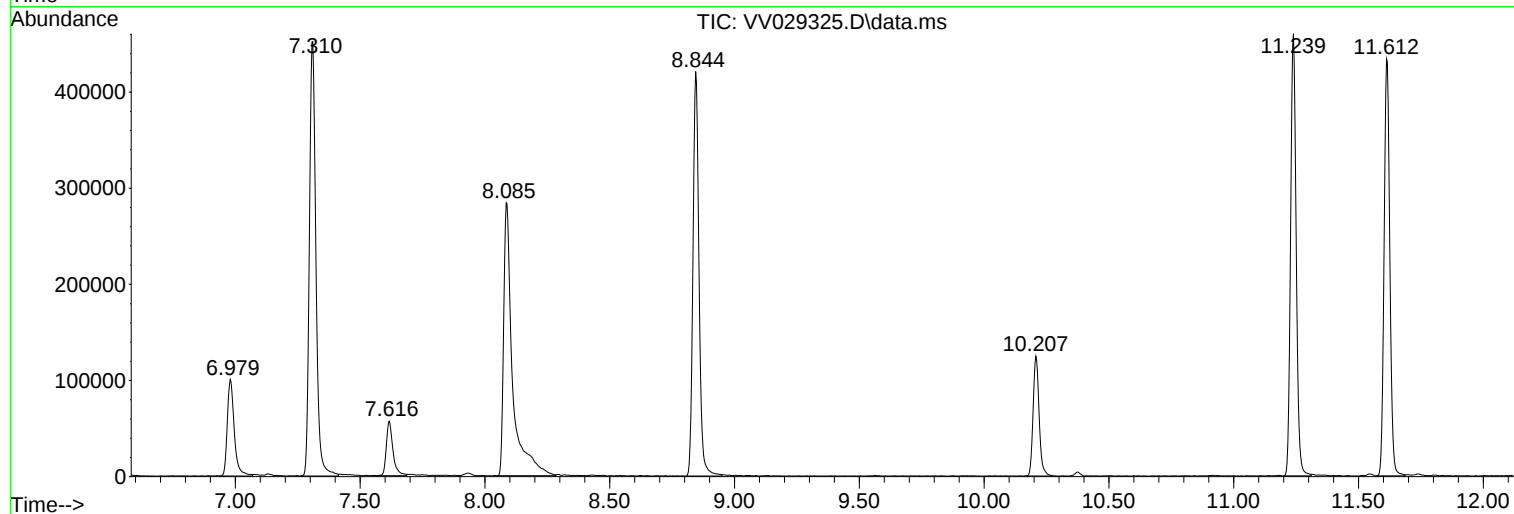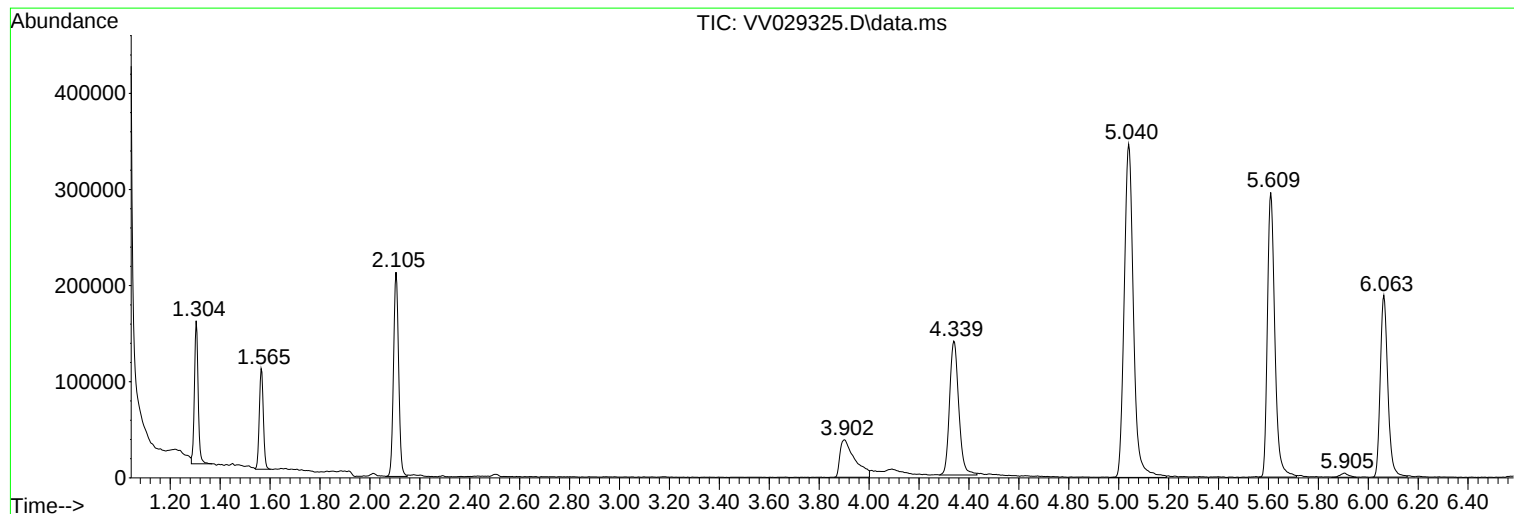

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112322\
Data File : VV029325.D
Acq On : 24 Nov 2022 04:25
Operator : SY/MD
Sample : VV1123WBL02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK277

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112322\
Data File : VV029325.D
Acq On : 24 Nov 2022 04:25
Operator : SY/MD
Sample : VV1123WBL02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK277

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------