

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112322\
 Data File : VV029333.D
 Acq On : 24 Nov 2022 07:41
 Operator : SY/MD
 Sample : N5725-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHB55

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV029333.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.214	50	54	60	rVB2	11324	10229	1.12%	0.126%
2	1.304	76	82	101	rVB	146883	157852	17.26%	1.939%
3	1.384	103	107	118	rVB	8348	10551	1.15%	0.130%
4	1.568	156	164	176	rVB	111194	126705	13.86%	1.556%
5	2.105	320	331	345	rBV	213172	307791	33.66%	3.781%
6	2.182	345	355	382	rVB2	13275	40274	4.40%	0.495%
7	2.503	445	455	470	rVB2	14698	26659	2.92%	0.327%
8	2.761	525	535	547	rBV2	13263	22863	2.50%	0.281%
9	3.892	875	887	929	rBV	71604	280302	30.65%	3.443%
10	4.339	1009	1026	1059	rBV	148906	406627	44.47%	4.995%
11	5.040	1226	1244	1287	rBV2	351845	914387	100.00%	11.232%
12	5.609	1409	1421	1449	rBV	278441	571333	62.48%	7.018%
13	5.908	1501	1514	1535	rVB5	14916	34244	3.75%	0.421%
14	6.063	1546	1562	1594	rBV	197169	411489	45.00%	5.054%
15	6.979	1831	1847	1870	rBV	94254	180021	19.69%	2.211%
16	7.310	1937	1950	1963	rBV	463204	821873	89.88%	10.095%
17	7.381	1963	1972	1998	rVB	117877	221860	24.26%	2.725%
18	7.616	2035	2045	2068	rBV2	53605	97887	10.71%	1.202%
19	7.969	2147	2155	2169	rVB2	23407	40604	4.44%	0.499%
20	8.085	2181	2191	2222	rBV2	359434	727886	79.60%	8.941%
21	8.239	2230	2239	2250	rVV2	14132	25002	2.73%	0.307%
22	8.301	2250	2258	2271	rVB3	7051	13785	1.51%	0.169%
23	8.844	2414	2427	2454	rBV	392904	652643	71.37%	8.017%
24	8.953	2454	2461	2469	rVV4	6496	10214	1.12%	0.125%
25	9.008	2469	2478	2488	rVV2	10169	15925	1.74%	0.196%
26	9.133	2504	2517	2535	rVB2	30168	49954	5.46%	0.614%
27	9.535	2630	2642	2659	rBV3	13646	28365	3.10%	0.348%
28	9.799	2714	2724	2738	rBV7	5193	9737	1.06%	0.120%
29	10.207	2838	2851	2868	rBV	128231	203542	22.26%	2.500%
30	10.374	2888	2903	2917	rBV	31699	52111	5.70%	0.640%
31	11.143	3134	3142	3152	rBV3	9863	15243	1.67%	0.187%
32	11.239	3158	3172	3193	rBV	432729	681086	74.49%	8.366%
33	11.519	3246	3259	3277	rBV4	30903	69259	7.57%	0.851%
34	11.612	3277	3288	3307	rVB	430955	690120	75.47%	8.477%
35	12.239	3472	3483	3498	rBV2	11926	22410	2.45%	0.275%
36	12.333	3502	3512	3528	rBV2	29254	48227	5.27%	0.592%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112322\
Data File : VV029333.D
Acq On : 24 Nov 2022 07:41
Operator : SY/MD
Sample : N5725-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHB55

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.1

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Title : TRACE VOA SFAM1.0

37	12.661	3602	3614	3624	rVV4	11234	17037	1.86%	0.209%
38	13.423	3844	3851	3858	rBV5	7747	11402	1.25%	0.140%
39	13.490	3858	3872	3885	rVB2	16535	38017	4.16%	0.467%
40	13.612	3894	3910	3926	rVB2	20292	41289	4.52%	0.507%
41	14.619	4214	4223	4234	rBV	11907	17617	1.93%	0.216%
42	14.802	4270	4280	4291	rVB3	9818	16754	1.83%	0.206%




Sum of corrected areas: 8141176

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112322\
Data File : VV029333.D
Acq On : 24 Nov 2022 07:41
Operator : SY/MD
Sample : N5725-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHB55

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

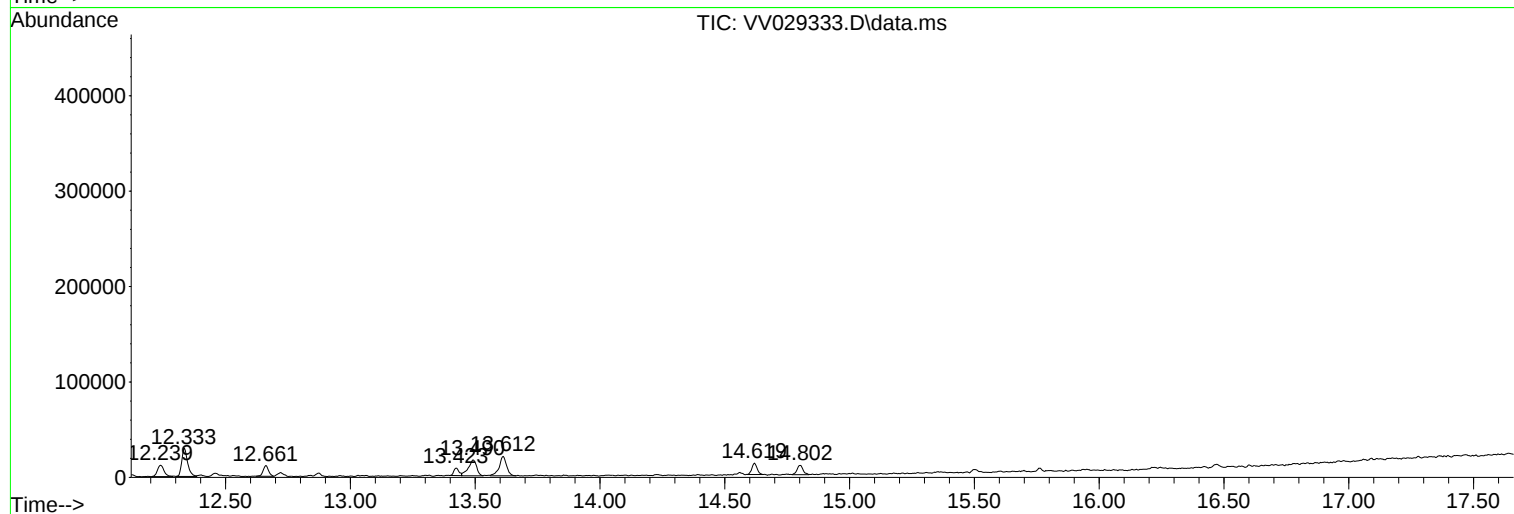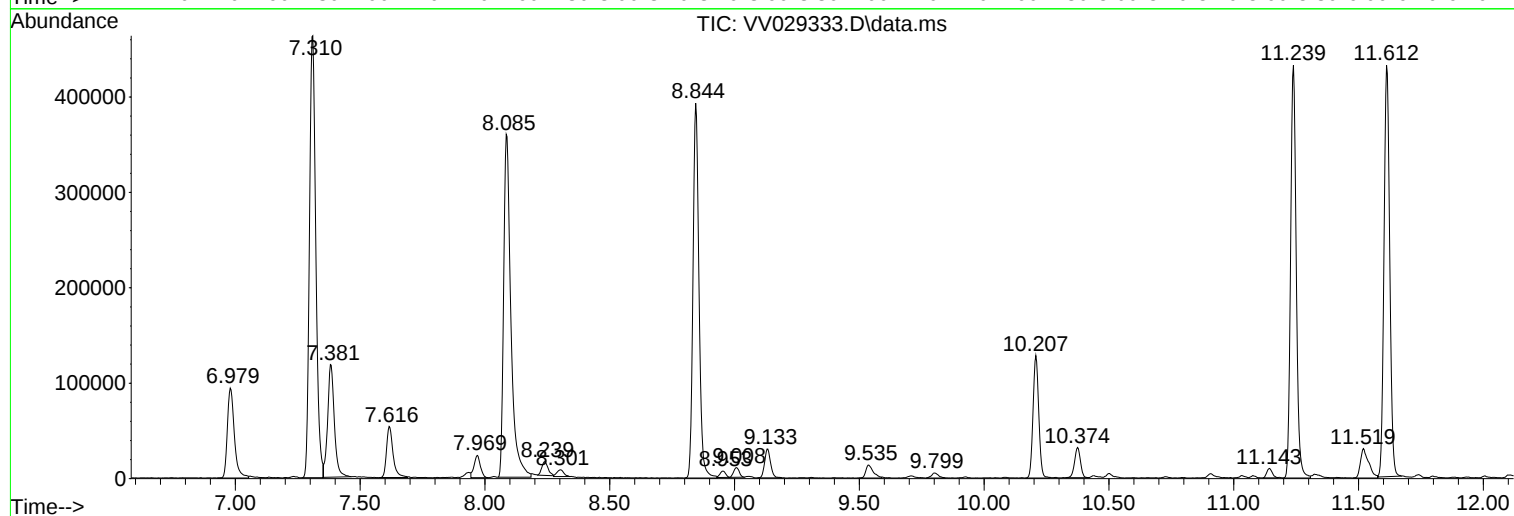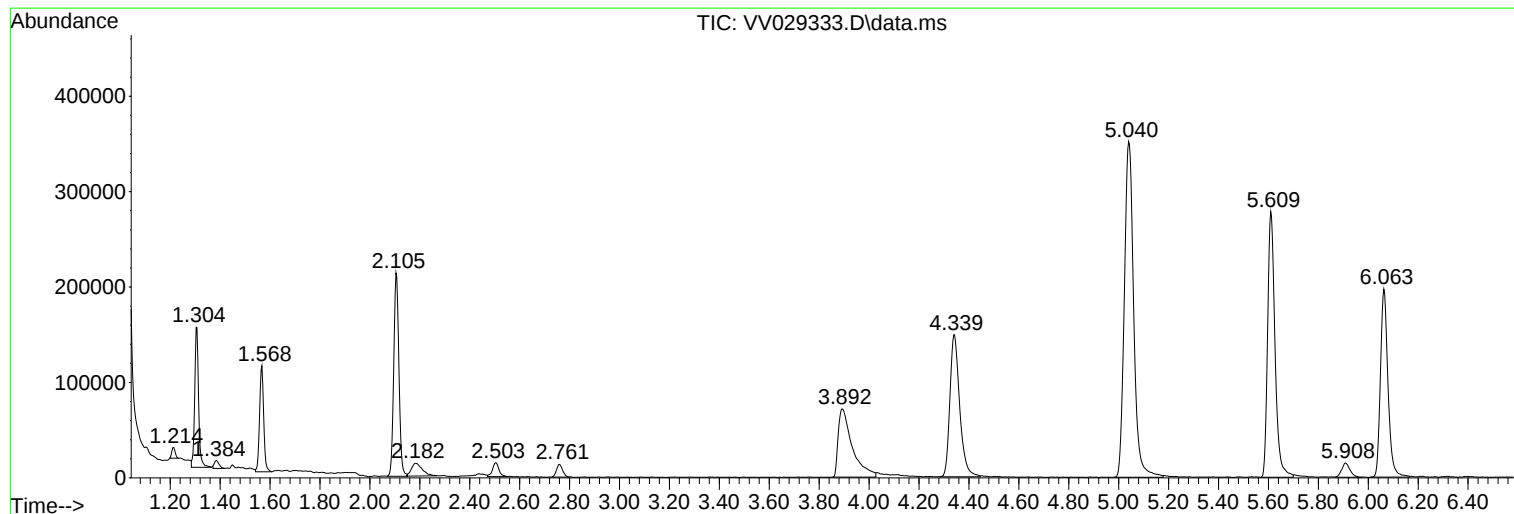

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112322\
Data File : VV029333.D
Acq On : 24 Nov 2022 07:41
Operator : SY/MD
Sample : N5725-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHB55










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Indane Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
11.519	0.51 ug/L	69259	1,4-Dichlorobenzene-d4	11.239

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Indane			118	C9H10	000496-11-7	92
2	Indane			118	C9H10	000496-11-7	91
3	Benzene, 2-propenyl-			118	C9H10	000300-57-2	87
4	Indane			118	C9H10	000496-11-7	87
5	Benzene, cyclopropyl-			118	C9H10	000873-49-4	81

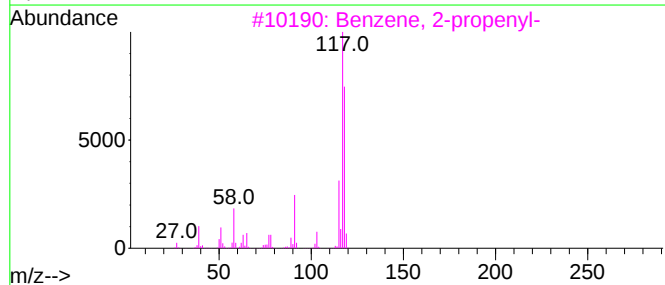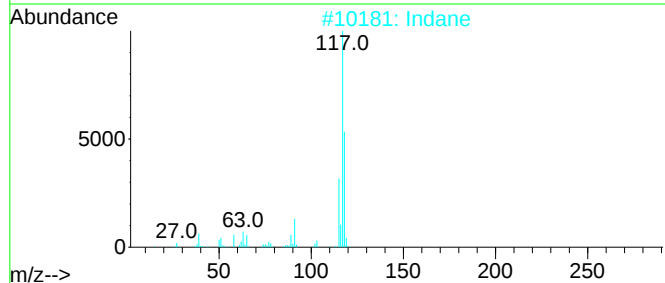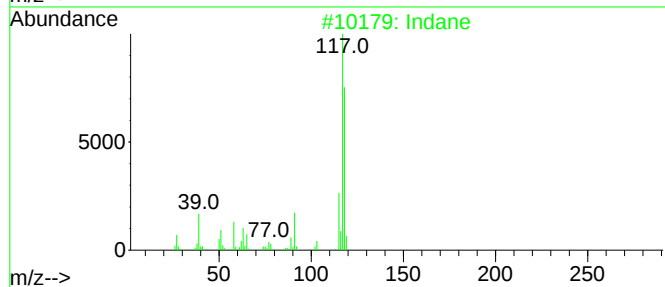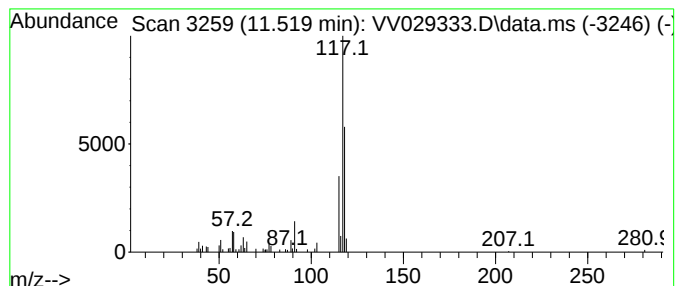

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112322\
Data File : VV029333.D
Acq On : 24 Nov 2022 07:41
Operator : SY/MD
Sample : N5725-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHB55

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Indane	11.519	0.5	ug/L	69259	3	11.239	681086	5.0