


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012022\
 Data File : VV024408.D
 Acq On : 20 Jan 2022 10:36
 Operator : SY/MD
 Sample : BFB259
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB259

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
 Title : VOC Analysis
 Last Update : Fri Jan 21 00:04:44 2022

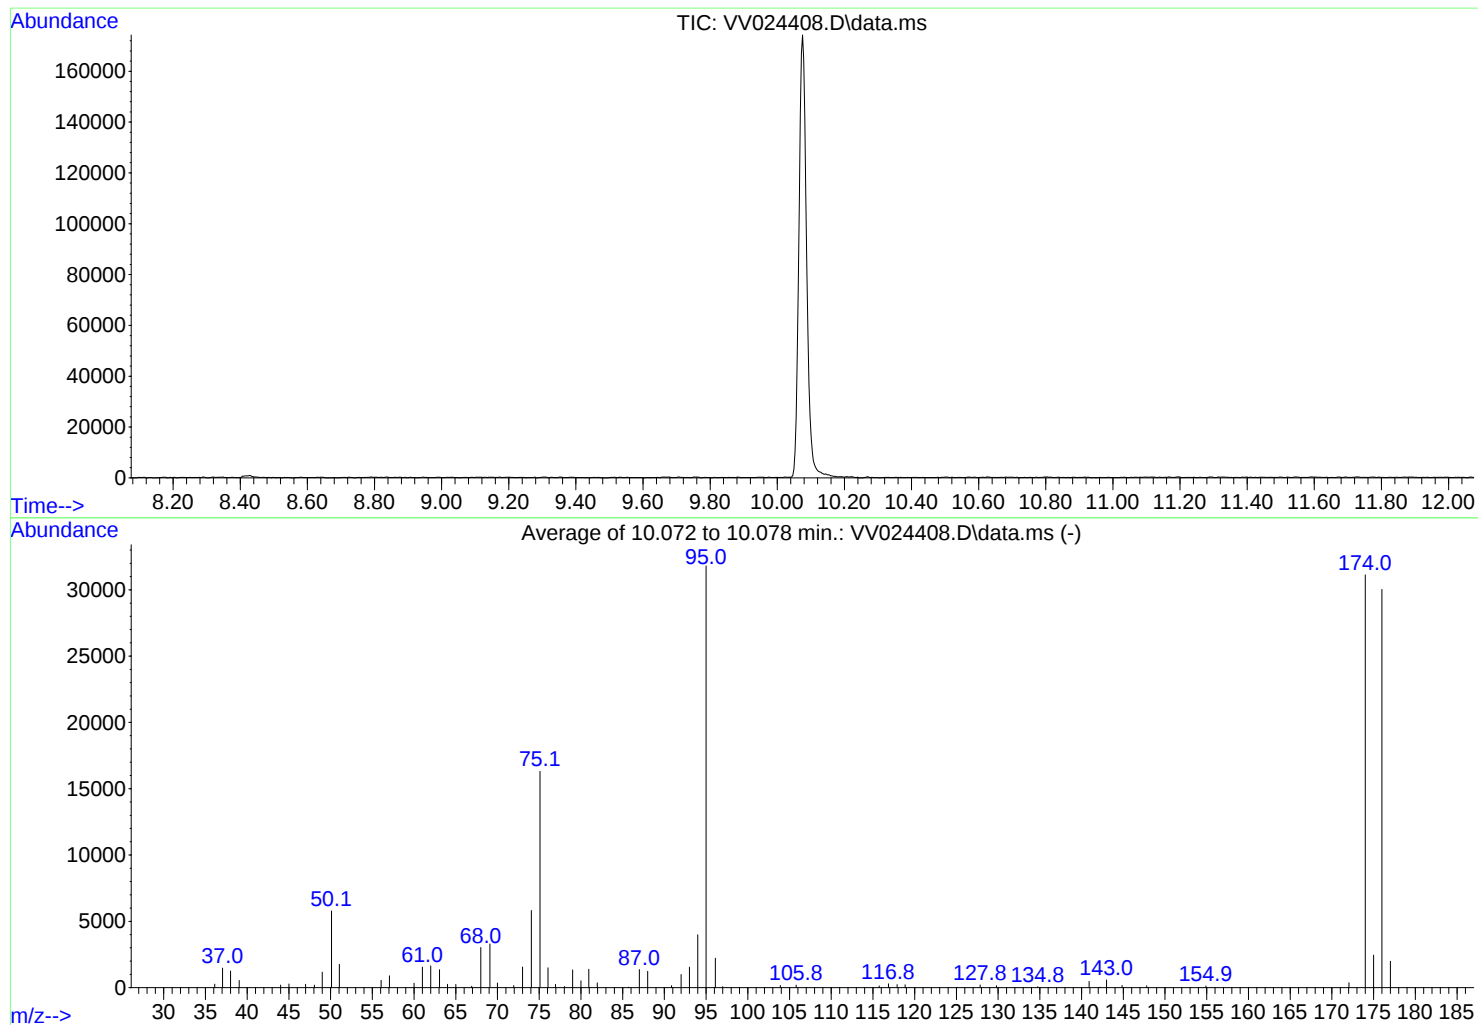

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2798

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.2	5784	PASS
75	95	30	80	51.3	16316	PASS
95	95	100	100	100.0	31808	PASS
96	95	5	9	7.0	2226	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	97.9	31131	PASS
175	174	5	9	7.9	2449	PASS
176	174	95	105	96.5	30029	PASS
177	176	5	10	6.6	1988	PASS

m/z	Abundance
40.20	116.0
44.00	135.0

Instrument :
MSVOA_V
ClientSampleId :
BFB259

m/z	Abundance
36.10	249.0
37.10	1516.0
38.00	1387.0
39.10	529.0
44.00	322.0
45.00	332.0
47.00	233.0
48.10	229.0
49.00	1245.0
50.10	5594.0
51.00	1713.0
56.10	638.0
57.10	857.0
60.00	340.0
61.00	1619.0
62.00	1555.0
63.10	1345.0
64.00	288.0
64.90	226.0
66.80	126.0
68.00	3076.0
69.10	3305.0
70.00	340.0
72.00	140.0
73.00	1531.0
74.00	5777.0
75.10	16464.0
76.10	1599.0
76.90	249.0
78.00	102.0
79.00	1325.0
80.00	524.0
80.90	1347.0
82.00	368.0
85.70	102.0
87.00	1401.0
88.00	1314.0
90.80	125.0
92.00	918.0
93.00	1545.0
94.00	3879.0
95.00	31448.0
96.10	2299.0
97.00	116.0
103.80	179.0
105.80	174.0
115.80	158.0
116.90	308.0
117.90	251.0
118.80	242.0
127.90	193.0
129.80	160.0
134.70	109.0
140.90	467.0
143.00	538.0
144.80	163.0
147.80	121.0
154.90	111.0
172.10	380.0
174.00	30264.0
175.00	2299.0
176.00	29456.0
177.00	1966.0

Instrument :
MSVOA_V
ClientSampleId :
BFB259

m/z	Abundance
36.10	287.0
37.00	1535.0
38.00	1282.0
39.10	562.0
44.00	312.0
45.00	286.0
47.00	257.0
48.10	199.0
49.00	1207.0
50.10	6055.0
51.00	1811.0
56.00	558.0
57.00	924.0
60.00	352.0
61.00	1588.0
62.00	1677.0
63.00	1371.0
64.00	254.0
65.00	237.0
66.90	116.0
68.00	3082.0
69.10	3404.0
70.00	363.0
72.00	144.0
73.00	1593.0
74.00	5993.0
75.10	16840.0
76.10	1526.0
76.90	271.0
79.00	1399.0
80.00	552.0
81.00	1431.0
81.90	374.0
87.00	1369.0
88.00	1299.0
90.90	138.0
92.00	1028.0
93.00	1578.0
94.00	4111.0
95.00	32848.0
96.10	2346.0
97.00	118.0
103.90	160.0
105.80	207.0
115.80	131.0
116.80	309.0
117.90	264.0
118.80	207.0
127.80	203.0
129.80	151.0
134.80	110.0
140.90	473.0
143.00	625.0
144.80	183.0
147.80	159.0
154.90	140.0
172.00	395.0
174.00	32248.0
175.00	2536.0
176.00	31032.0
177.00	2029.0

Instrument :
MSVOA_V
ClientSampleId :
BFB259

m/z	Abundance
36.10	275.0
37.00	1376.0
38.00	1094.0
39.00	540.0
44.10	339.0
45.00	201.0
47.00	286.0
48.00	156.0
49.00	1050.0
50.10	5704.0
51.10	1765.0
56.00	453.0
57.00	882.0
60.00	312.0
61.00	1447.0
62.00	1691.0
63.00	1349.0
64.00	217.0
65.10	252.0
67.00	101.0
68.00	2914.0
69.10	3172.0
70.00	361.0
71.90	173.0
73.00	1535.0
74.10	5685.0
75.10	15643.0
76.00	1379.0
77.00	217.0
78.10	170.0
79.00	1307.0
80.00	493.0
81.00	1390.0
81.90	336.0
87.00	1317.0
88.00	1067.0
90.90	165.0
92.00	1030.0
93.00	1522.0
94.00	3964.0
95.00	31128.0
96.10	2034.0
104.00	163.0
105.80	201.0
115.70	106.0
116.80	263.0
117.90	190.0
118.90	210.0
127.80	211.0
129.80	118.0
140.90	459.0
142.20	113.0
143.00	590.0
144.90	178.0
147.80	150.0
154.90	136.0
172.00	339.0
174.00	30880.0
175.00	2513.0
176.00	29600.0
177.00	1969.0

Instrument :
MSVOA_V
ClientSampleId :
BFB259