
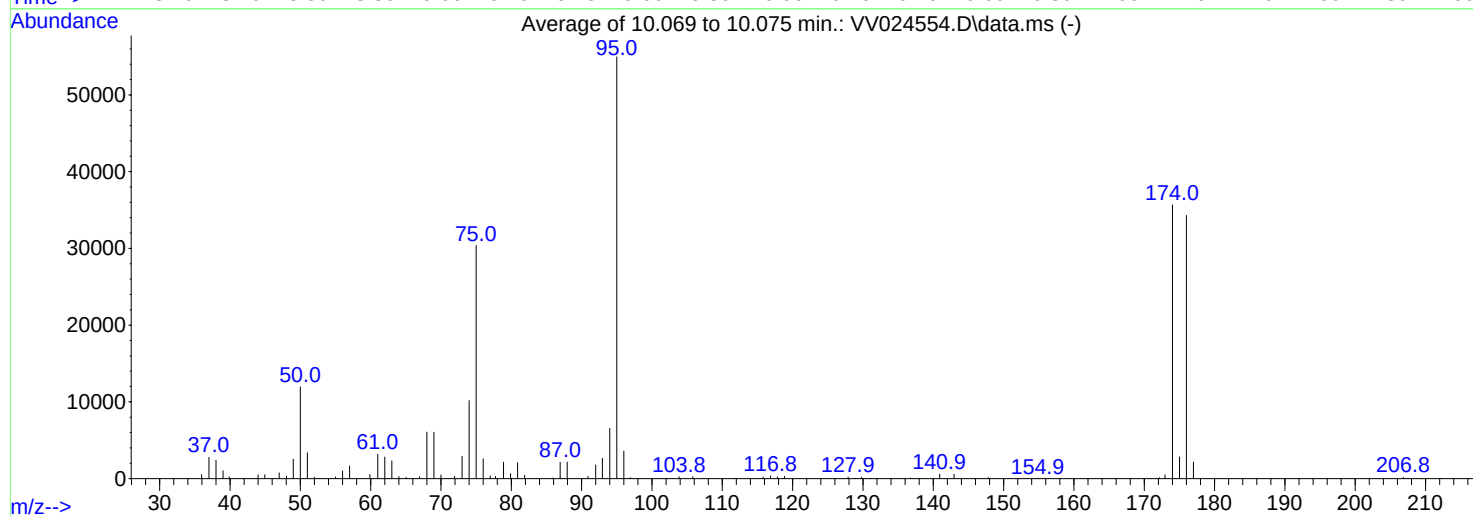


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020422\
 Data File : VV024554.D
 Acq On : 04 Feb 2022 08:49
 Operator : SY/MD
 Sample : BFB263
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB263

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM020222WMA.M
 Title : VOC Analysis
 Last Update : Sat Feb 05 00:18:38 2022

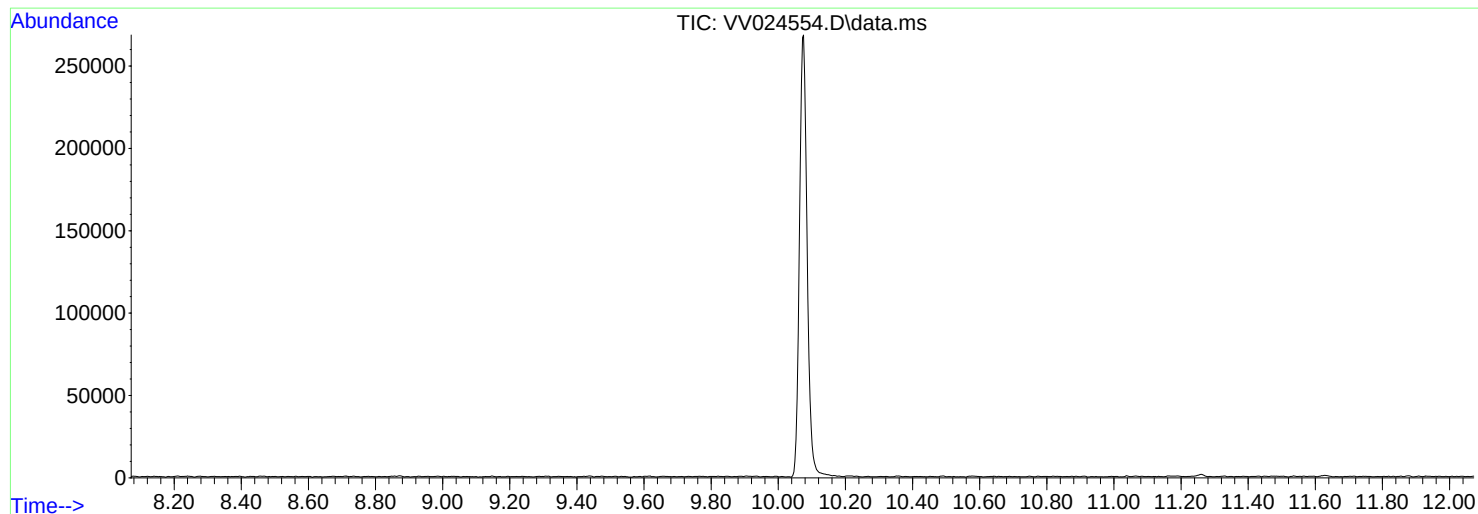

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2798

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.8	11977	PASS
75	95	30	80	55.3	30384	PASS
95	95	100	100	100.0	54957	PASS
96	95	5	9	6.5	3579	PASS
173	174	0.00	2	1.4	493	PASS
174	95	50	120	64.9	35672	PASS
175	174	5	9	8.0	2838	PASS
176	174	95	105	96.1	34288	PASS
177	176	5	10	6.3	2165	PASS

Scan 2798 (10.037 min): VV024554.D\data.ms
BFB263

m/z	Abundance
44.00	392.0
207.10	144.0

Instrument :
MSVOA_V
ClientSampleId :
BFB263

m/z	Abundance
36.00	470.0
37.00	2658.0
38.00	2326.0
39.00	941.0
39.90	234.0
44.00	903.0
45.00	488.0
47.00	746.0
48.00	339.0
49.00	2379.0
50.00	11440.0
51.00	3150.0
52.00	179.0
55.00	226.0
56.00	962.0
57.00	1569.0
59.90	592.0
61.00	2919.0
62.00	2694.0
63.00	2160.0
64.00	256.0
65.10	138.0
67.00	221.0
68.00	5621.0
69.00	5611.0
70.00	462.0
71.90	302.0
73.00	2716.0
74.00	9495.0
75.00	28368.0
76.00	2486.0
77.00	358.0
77.70	245.0
78.90	1966.0
79.90	585.0
80.90	1951.0
81.90	385.0
87.00	2057.0
88.00	1944.0
90.90	352.0
92.00	1825.0
92.90	2407.0
94.00	6139.0
95.00	51296.0
96.00	3405.0
96.90	108.0
103.80	223.0
105.80	257.0
115.80	235.0
116.90	311.0
117.90	202.0
118.90	269.0
127.90	167.0
128.90	111.0
129.80	169.0
140.90	545.0
142.90	515.0
147.80	107.0
171.80	113.0
172.10	117.0
173.00	445.0
174.00	31848.0
175.00	2614.0
176.00	30728.0
177.00	1998.0
206.90	149.0

Instrument :
MSVOA_V
ClientSampleId :
BFB263

m/z	Abundance
36.00	545.0
37.00	2886.0
38.00	2482.0
39.00	1077.0
39.90	227.0
44.00	918.0
44.90	504.0
47.00	786.0
48.10	339.0
49.00	2589.0
50.00	12434.0
51.00	3467.0
52.00	198.0
55.00	212.0
56.00	1014.0
57.00	1707.0
59.90	555.0
61.00	3300.0
62.00	2902.0
63.00	2397.0
64.00	278.0
65.00	180.0
66.90	254.0
68.00	6263.0
69.00	6255.0
70.00	476.0
71.90	303.0
73.00	3054.0
74.00	10581.0
75.00	31464.0
76.00	2687.0
77.00	375.0
77.80	309.0
78.90	2243.0
79.90	650.0
80.90	2147.0
81.90	448.0
85.90	117.0
87.00	2177.0
87.90	2234.0
90.90	309.0
92.00	1838.0
93.00	2778.0
94.00	6749.0
95.00	57000.0
96.00	3668.0
96.90	139.0
103.90	268.0
105.80	252.0
115.80	230.0
116.90	357.0
117.80	238.0
118.90	294.0
127.90	212.0
129.80	192.0
136.80	106.0
140.90	618.0
142.90	576.0
147.80	124.0
172.20	139.0
172.90	506.0
174.00	36712.0
175.00	2961.0
176.00	35592.0
177.00	2259.0
206.80	175.0

Instrument :
MSVOA_V
ClientSampleId :
BFB263

m/z	Abundance
35.90	563.0
37.00	2784.0
38.00	2434.0
39.00	1049.0
39.90	184.0
43.00	110.0
44.00	853.0
44.90	527.0
47.00	700.0
48.10	327.0
49.00	2614.0
50.00	12056.0
51.00	3493.0
52.00	187.0
55.00	169.0
56.00	1034.0
57.00	1675.0
58.00	107.0
59.90	498.0
61.00	3303.0
62.00	2879.0
63.00	2371.0
64.00	260.0
65.00	169.0
66.90	273.0
68.00	6289.0
69.00	6242.0
70.00	502.0
71.90	282.0
73.00	2947.0
74.00	10435.0
75.00	31320.0
76.00	2579.0
77.00	341.0
77.80	308.0
78.90	2237.0
79.90	679.0
80.90	2182.0
81.90	479.0
85.90	125.0
86.90	2182.0
87.90	2245.0
90.90	239.0
92.00	1672.0
93.00	2789.0
94.00	6784.0
95.00	56576.0
96.00	3664.0
96.90	153.0
103.90	288.0
105.80	267.0
115.80	187.0
116.80	404.0
117.80	268.0
118.80	314.0
127.90	240.0
129.80	183.0
131.10	104.0
136.80	125.0
140.90	633.0
143.00	576.0
145.80	101.0
147.80	136.0
154.90	111.0
172.20	147.0
172.90	527.0
174.00	38456.0
175.00	2939.0
176.00	36544.0
177.00	2237.0
206.90	179.0

Instrument :
MSVOA_V
ClientSampleId :
BFB263