

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042622\
 Data File : VW025730.D
 Acq On : 26 Apr 2022 13:57
 Operator : SY/MD
 Sample : N2492-23
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6W9

Quant Time: Apr 27 05:36:03 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Apr 27 05:32:04 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	208576	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	213691	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	94805	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.310	65	82699	4.265	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	85.200%
7) Chloroethane-d5	1.571	69	80744	3.914	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	78.200%
11) 1,1-Dichloroethene-d2	2.111	63	126909	3.267	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	65.400%
20) 2-Butanone-d5	3.899	46	125496	53.204	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	106.400%
24) Chloroform-d	4.352	84	142448	4.861	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.200%
26) 1,2-Dichloroethane-d4	5.034	65	67069	5.312	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	106.200%
32) Benzene-d6	5.053	84	282860	4.575	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.400%
36) 1,2-Dichloropropane-d6	6.069	67	84762	4.916	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	98.400%
41) Toluene-d8	7.317	98	241392	4.207	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	84.200%
43) trans-1,3-Dichloroprop...	7.622	79	24673	4.257	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	85.200%
46) 2-Hexanone-d5	8.088	63	97913	48.135	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	96.280%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	48308	4.434	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	88.600%
66) 1,2-Dichlorobenzene-d4	11.622	152	80294	5.052	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	101.000%
Target Compounds						Qvalue
47) Tetrachloroethene	7.976	164	334500	25.492	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042622\
Data File : VV025730.D
Acq On : 26 Apr 2022 13:57
Operator : SY/MD
Sample : N2492-23
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6W9


Quant Time: Apr 27 05:36:03 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Apr 27 05:32:04 2022
Response via : Initial Calibration

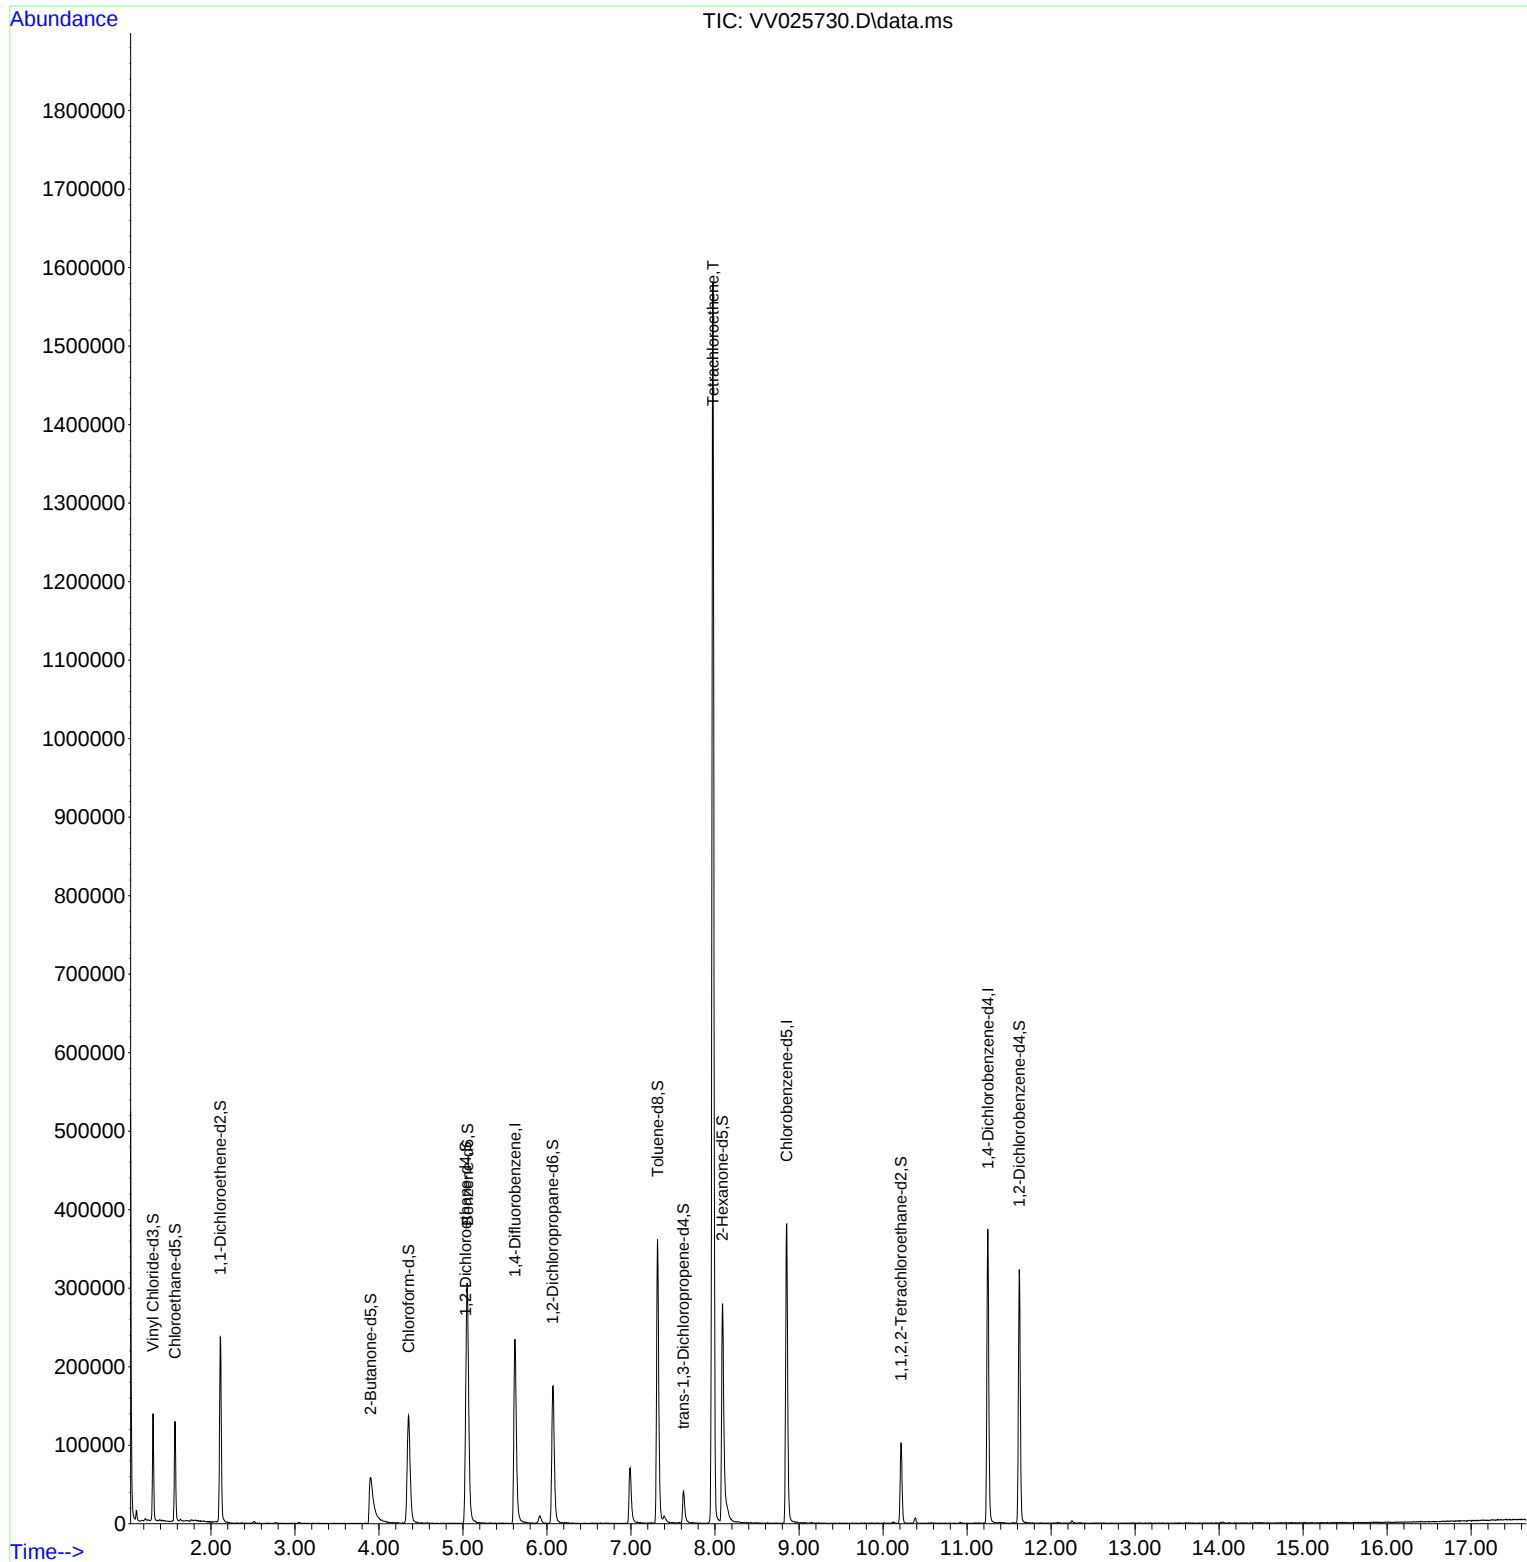

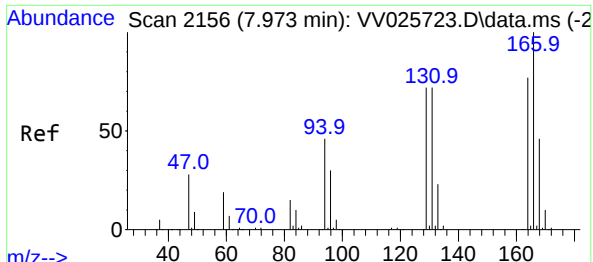

#47
Tetrachloroethene
Concen: 25.492 ug/L
RT: 7.976 min Scan# 21
Delta R.T. 0.003 min
Lab File: VV025730.D
Acq: 26 Apr 2022 13:57

Instrument :
MSVOA_V
ClientSampleId :
EW6W9

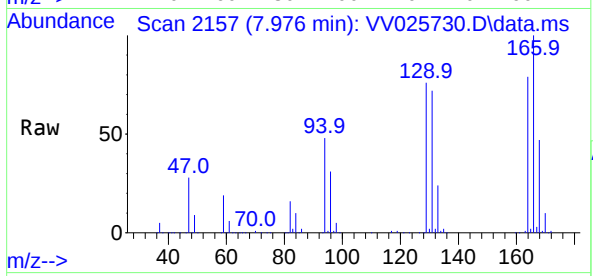

Tgt Ion:164 Resp: 334500

Ion	Ratio	Lower	Upper
164	100		
129	96.9	66.8	124.2
131	92.1	66.4	123.4
166	127.2	91.7	170.3

