

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042622\
 Data File : VV025724.D
 Acq On : 26 Apr 2022 11:31
 Operator : SY/MD
 Sample : VV0426WBL01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK352

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV025724.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	76	84	96	rVV	126578	133998	17.80%	2.191%
2	1.568	156	164	174	rVV	163377	187047	24.85%	3.059%
3	2.108	321	332	348	rVB	242651	352359	46.81%	5.763%
4	2.506	447	456	472	rVB	11206	19197	2.55%	0.314%
5	3.047	612	624	637	rVB7	3867	8986	1.19%	0.147%
6	3.883	872	884	928	rBV	74315	238020	31.62%	3.893%
7	4.346	1010	1028	1054	rBV	134095	336151	44.66%	5.498%
8	5.043	1225	1245	1278	rBV2	300412	752700	100.00%	12.310%
9	5.612	1405	1422	1456	rBV	237808	491218	65.26%	8.034%
10	5.905	1502	1513	1531	rBV6	9166	21413	2.84%	0.350%
11	6.066	1549	1563	1588	rBV	171882	356323	47.34%	5.827%
12	6.985	1837	1849	1871	rBV2	70330	135262	17.97%	2.212%
13	7.313	1936	1951	1970	rBV	356545	621814	82.61%	10.169%
14	7.397	1970	1977	1988	rVB3	5582	11418	1.52%	0.187%
15	7.622	2036	2047	2062	rBV	41163	75012	9.97%	1.227%
16	8.085	2181	2191	2235	rBV	275067	539814	71.72%	8.828%
17	8.850	2416	2429	2449	rBV	377747	623437	82.83%	10.196%
18	10.214	2842	2853	2871	rBV	97050	155638	20.68%	2.545%
19	11.246	3163	3174	3193	rBV	366211	567442	75.39%	9.280%
20	11.622	3279	3291	3311	rBV	301889	478935	63.63%	7.833%
21	13.506	3869	3877	3888	rBV4	5585	8349	1.11%	0.137%




Sum of corrected areas: 6114533

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042622\
Data File : VV025724.D
Acq On : 26 Apr 2022 11:31
Operator : SY/MD
Sample : VV0426WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK352

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

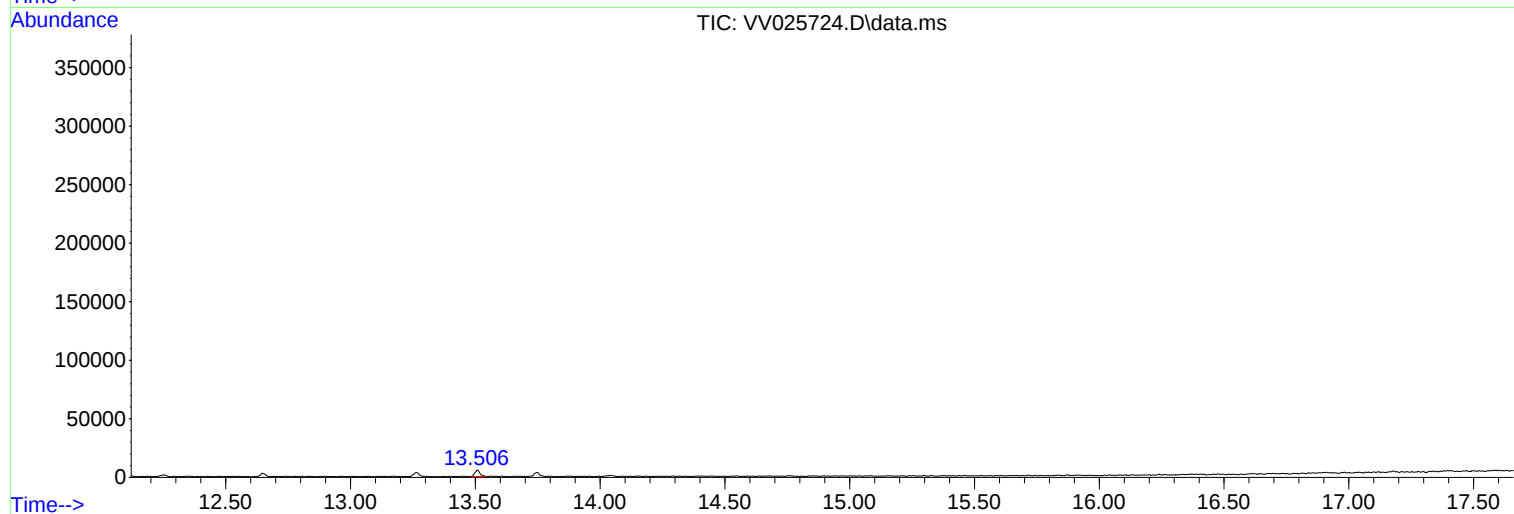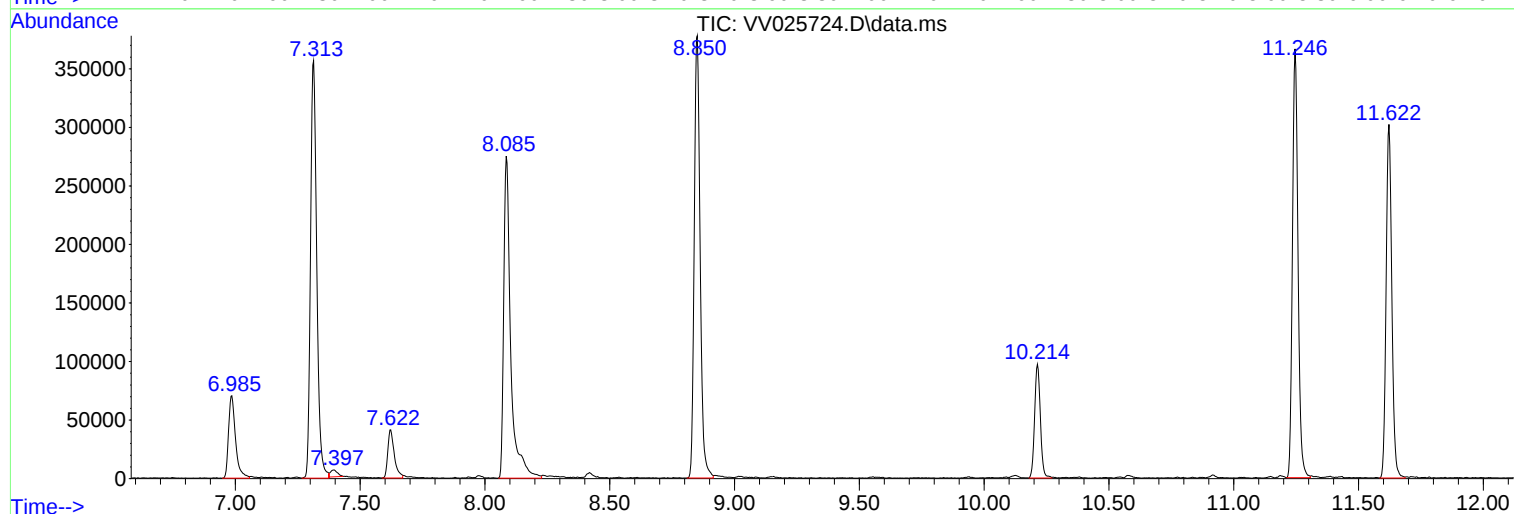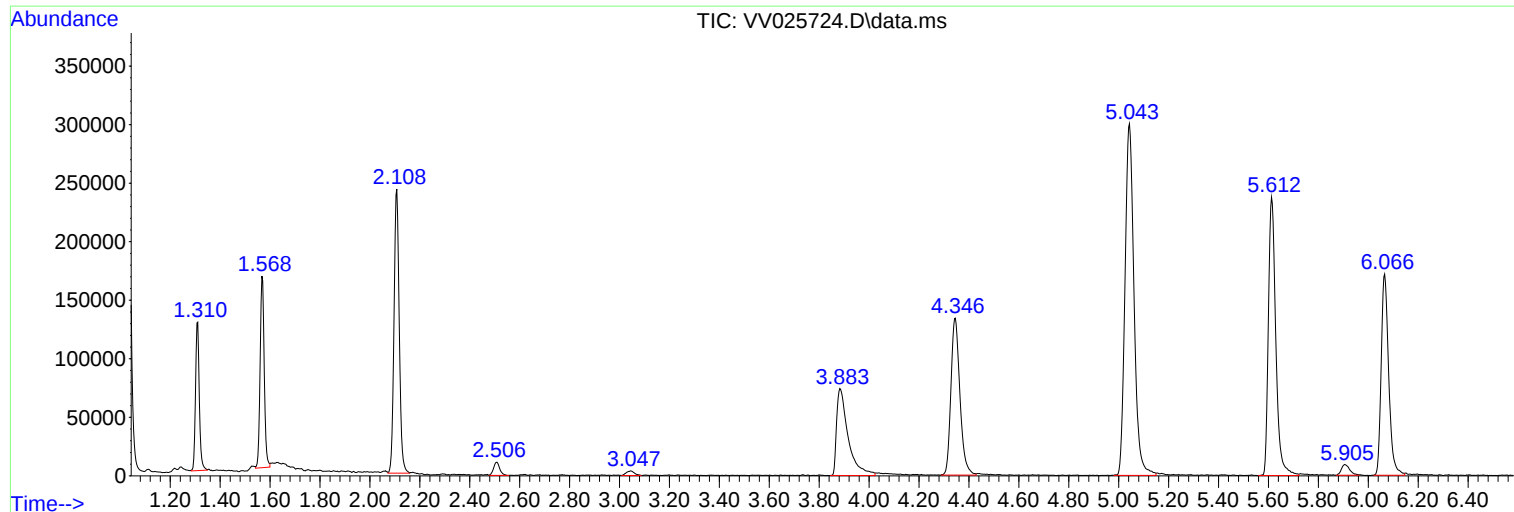

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042622\
Data File : VV025724.D
Acq On : 26 Apr 2022 11:31
Operator : SY/MD
Sample : VV0426WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK352

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042622\
Data File : VV025724.D
Acq On : 26 Apr 2022 11:31
Operator : SY/MD
Sample : VV0426WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK352

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------