

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042622\
 Data File : VV025725.D
 Acq On : 26 Apr 2022 12:00
 Operator : SY/MD
 Sample : N2471-03
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025725.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	76	84	101	rVB	131049	136558	18.33%	2.268%
2	1.571	157	165	178	rBV	126866	144716	19.42%	2.403%
3	2.108	322	332	354	rVB	237398	351139	47.13%	5.831%
4	2.510	448	457	478	rVB2	8573	15646	2.10%	0.260%
5	3.892	874	887	922	rBV	64592	227544	30.54%	3.779%
6	4.346	1011	1028	1054	rBV	132831	333719	44.79%	5.542%
7	5.047	1230	1246	1275	rBV2	299750	745076	100.00%	12.373%
8	5.616	1411	1423	1446	rBV	237908	481249	64.59%	7.992%
9	5.908	1504	1514	1531	rBV4	9905	22162	2.97%	0.368%
10	6.066	1550	1563	1597	rBV	170753	354848	47.63%	5.893%
11	6.985	1838	1849	1877	rBV	71656	137326	18.43%	2.280%
12	7.313	1939	1951	1971	rBV	347656	616844	82.79%	10.243%
13	7.397	1973	1977	1992	rVB3	6142	11656	1.56%	0.194%
14	7.622	2038	2047	2070	rBV	41264	76476	10.26%	1.270%
15	8.088	2182	2192	2230	rBV	259855	525978	70.59%	8.734%
16	8.850	2418	2429	2450	rBV	380343	624491	83.82%	10.370%
17	10.214	2842	2853	2871	rBV	96558	154044	20.67%	2.558%
18	11.246	3163	3174	3193	rBV	366168	576730	77.41%	9.577%
19	11.622	3278	3291	3308	rBV	305392	485667	65.18%	8.065%




Sum of corrected areas: 6021869

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042622\
Data File : VV025725.D
Acq On : 26 Apr 2022 12:00
Operator : SY/MD
Sample : N2471-03
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

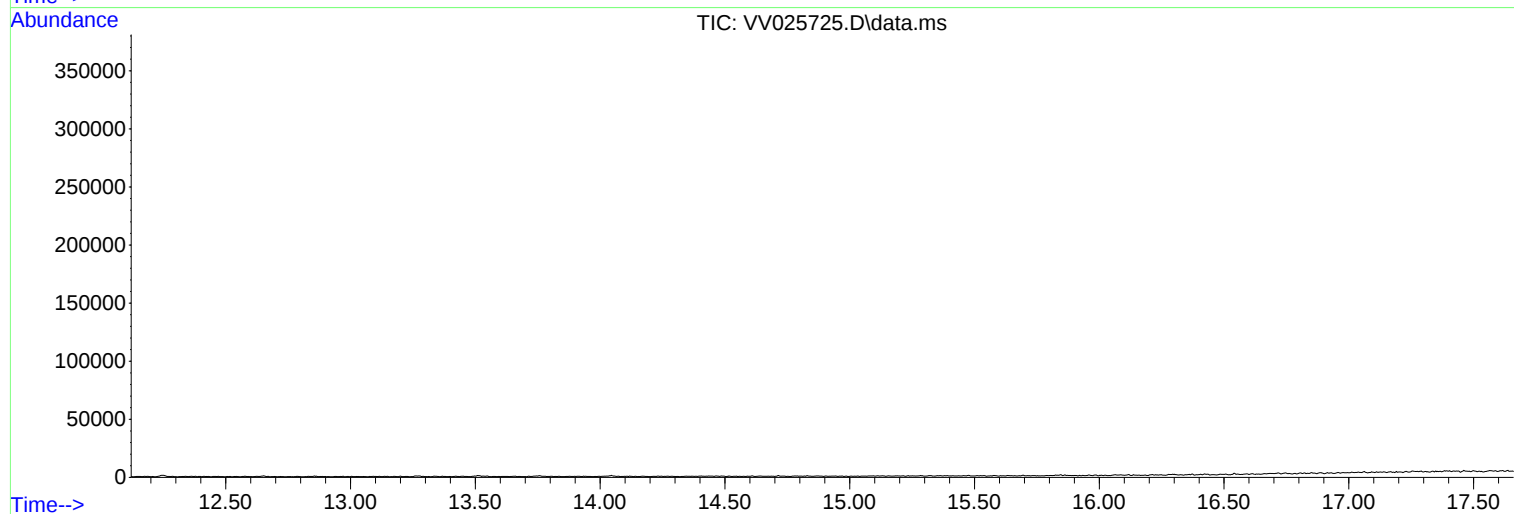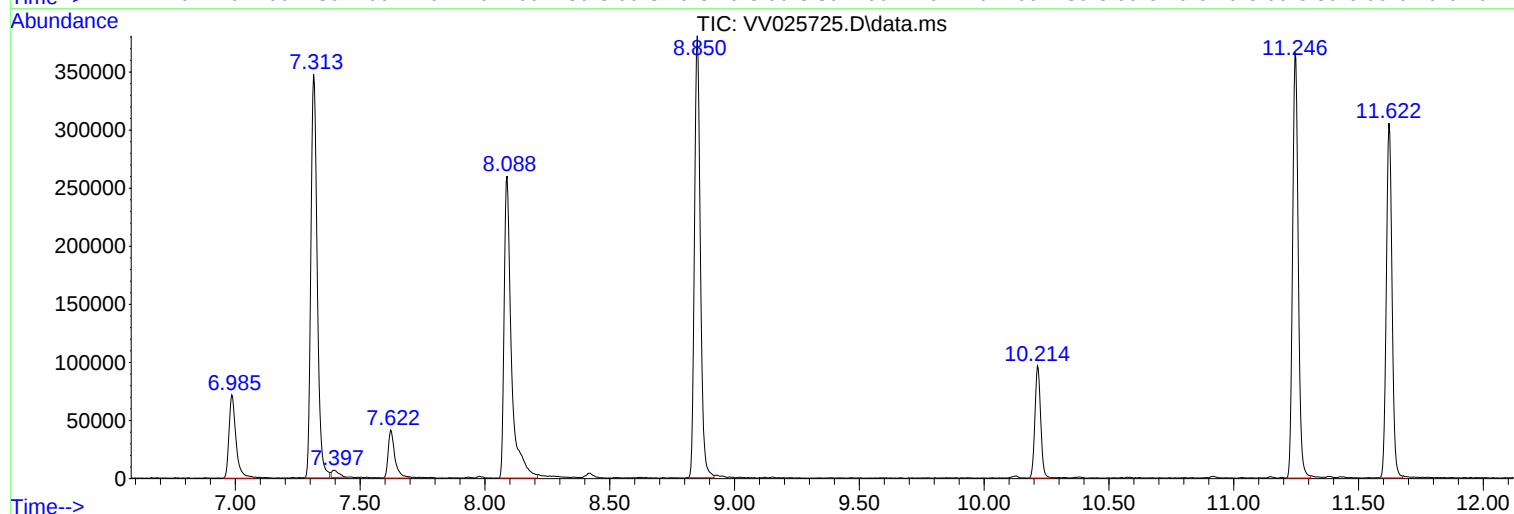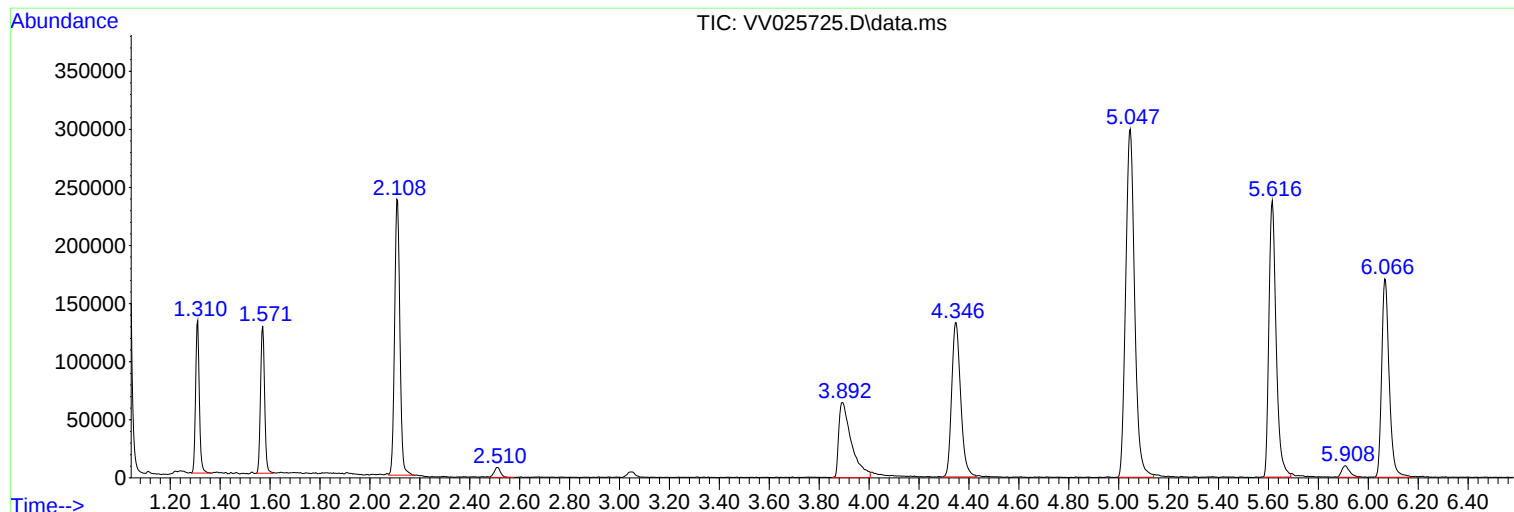

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042622\
Data File : VV025725.D
Acq On : 26 Apr 2022 12:00
Operator : SY/MD
Sample : N2471-03
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042622\
Data File : VV025725.D
Acq On : 26 Apr 2022 12:00
Operator : SY/MD
Sample : N2471-03
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc