

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042622\
 Data File : VV025726.D
 Acq On : 26 Apr 2022 12:23
 Operator : SY/MD
 Sample : N2517-05
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025726.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	75	84	96	rBV	106932	110137	17.92%	2.182%
2	1.571	157	165	177	rBV	105349	118967	19.36%	2.357%
3	2.111	322	333	353	rVB	200121	289130	47.05%	5.729%
4	2.510	448	457	472	rVB3	4829	8722	1.42%	0.173%
5	3.899	879	889	922	rBV	50964	177462	28.88%	3.516%
6	4.352	1011	1030	1057	rBV	110466	277954	45.23%	5.508%
7	5.050	1225	1247	1274	rBV2	248835	614483	100.00%	12.176%
8	5.619	1409	1424	1451	rBV	211493	432136	70.33%	8.563%
9	5.915	1503	1516	1530	rBV5	7110	16250	2.64%	0.322%
10	6.072	1552	1565	1588	rBV	139500	290455	47.27%	5.755%
11	6.989	1838	1850	1877	rBV	59280	113001	18.39%	2.239%
12	7.317	1939	1952	1973	rBV	286653	501952	81.69%	9.946%
13	7.400	1974	1978	1994	rVB10	4183	7785	1.27%	0.154%
14	7.625	2039	2048	2067	rBV2	31649	59320	9.65%	1.175%
15	8.088	2181	2192	2227	rBV	208375	425138	69.19%	8.424%
16	8.850	2416	2429	2454	rBV	341780	562592	91.56%	11.148%
17	10.214	2841	2853	2868	rBV	82663	131183	21.35%	2.599%
18	11.249	3164	3175	3192	rBV	328858	511431	83.23%	10.134%
19	11.622	3280	3291	3307	rBV	257573	398516	64.85%	7.897%




Sum of corrected areas: 5046614

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042622\
Data File : VV025726.D
Acq On : 26 Apr 2022 12:23
Operator : SY/MD
Sample : N2517-05
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

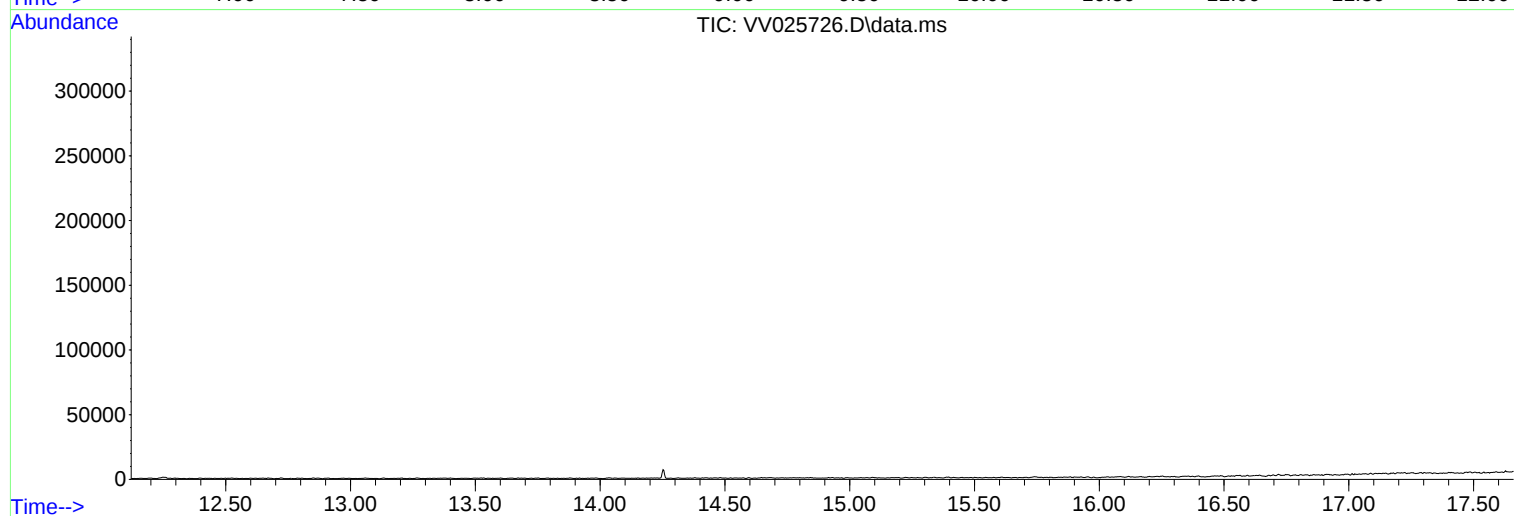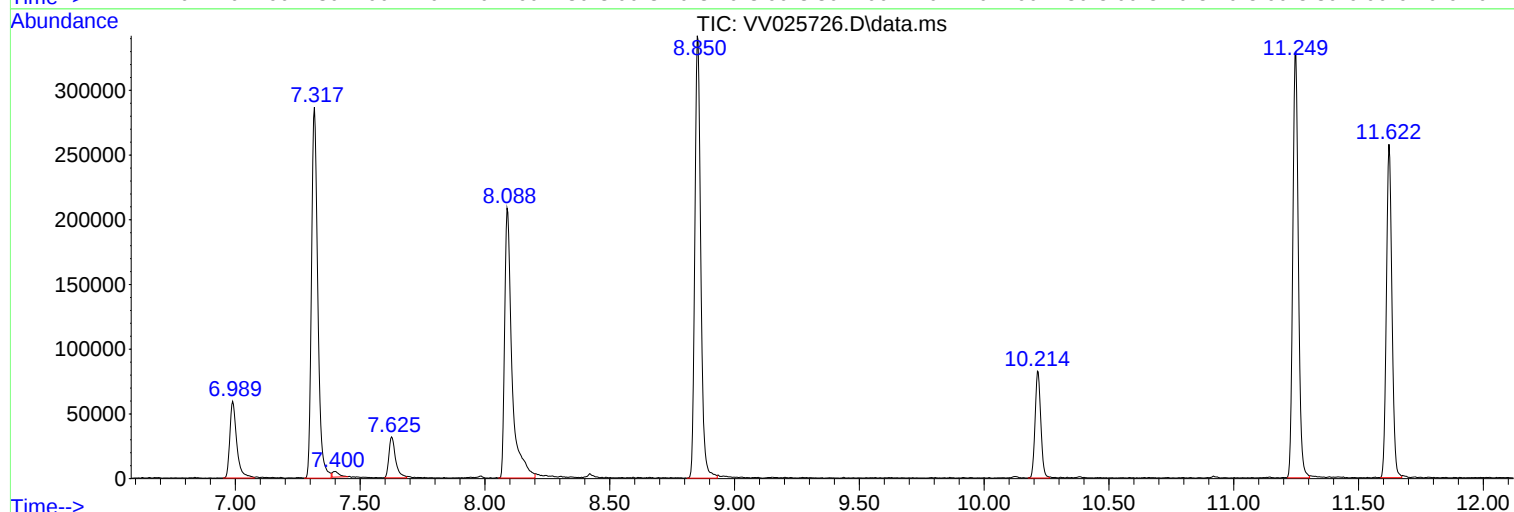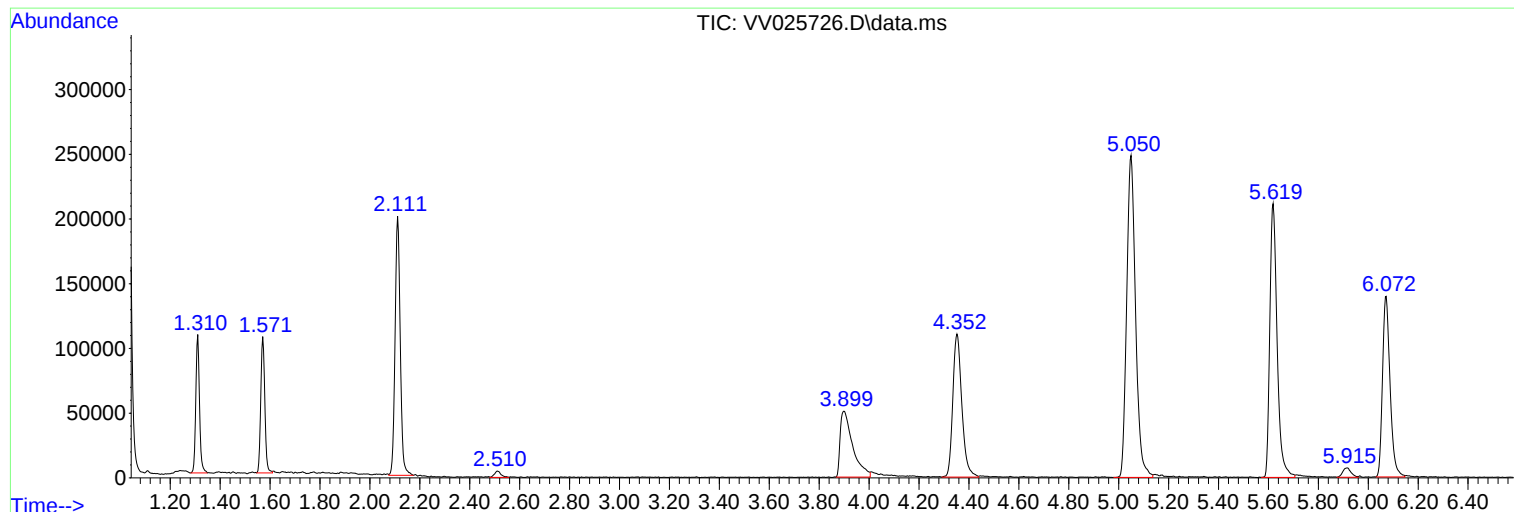

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042622\
Data File : VV025726.D
Acq On : 26 Apr 2022 12:23
Operator : SY/MD
Sample : N2517-05
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042622\
Data File : VV025726.D
Acq On : 26 Apr 2022 12:23
Operator : SY/MD
Sample : N2517-05
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc