

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042622\
 Data File : VV025727.D
 Acq On : 26 Apr 2022 12:47
 Operator : SY/MD
 Sample : N2492-21
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6W7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025727.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.111	18	22	34	rVB3	6885	7607	1.22%	0.134%
2	1.310	76	84	96	rVB	110622	113868	18.19%	2.013%
3	1.571	157	165	178	rVB	107689	119741	19.13%	2.117%
4	2.111	322	333	356	rVB	195726	288484	46.09%	5.101%
5	3.895	878	888	923	rBV	53281	175991	28.12%	3.112%
6	4.352	1014	1030	1061	rBV	113313	285852	45.67%	5.054%
7	5.050	1230	1247	1273	rBV2	251271	625920	100.00%	11.067%
8	5.619	1412	1424	1450	rBV	204211	415942	66.45%	7.354%
9	5.915	1506	1516	1530	rBV10	7068	16063	2.57%	0.284%
10	6.069	1551	1564	1589	rBV	145353	303605	48.51%	5.368%
11	6.989	1839	1850	1872	rBV	60435	113911	18.20%	2.014%
12	7.317	1941	1952	1970	rBV	294609	516123	82.46%	9.125%
13	7.625	2037	2048	2066	rBV2	34552	61699	9.86%	1.091%
14	7.976	2136	2157	2178	rBV	336735	571631	91.33%	10.107%
15	8.088	2183	2192	2226	rBV	223232	439327	70.19%	7.768%
16	8.853	2417	2430	2453	rBV	333137	547819	87.52%	9.686%
17	10.217	2843	2854	2877	rVB	84190	134897	21.55%	2.385%
18	10.381	2896	2905	2922	rVB3	8379	13260	2.12%	0.234%
19	11.249	3163	3175	3197	rBV	313922	495226	79.12%	8.756%
20	11.622	3280	3291	3311	rBV	255913	408925	65.33%	7.230%




Sum of corrected areas: 5655891

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042622\
Data File : VV025727.D
Acq On : 26 Apr 2022 12:47
Operator : SY/MD
Sample : N2492-21
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6W7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

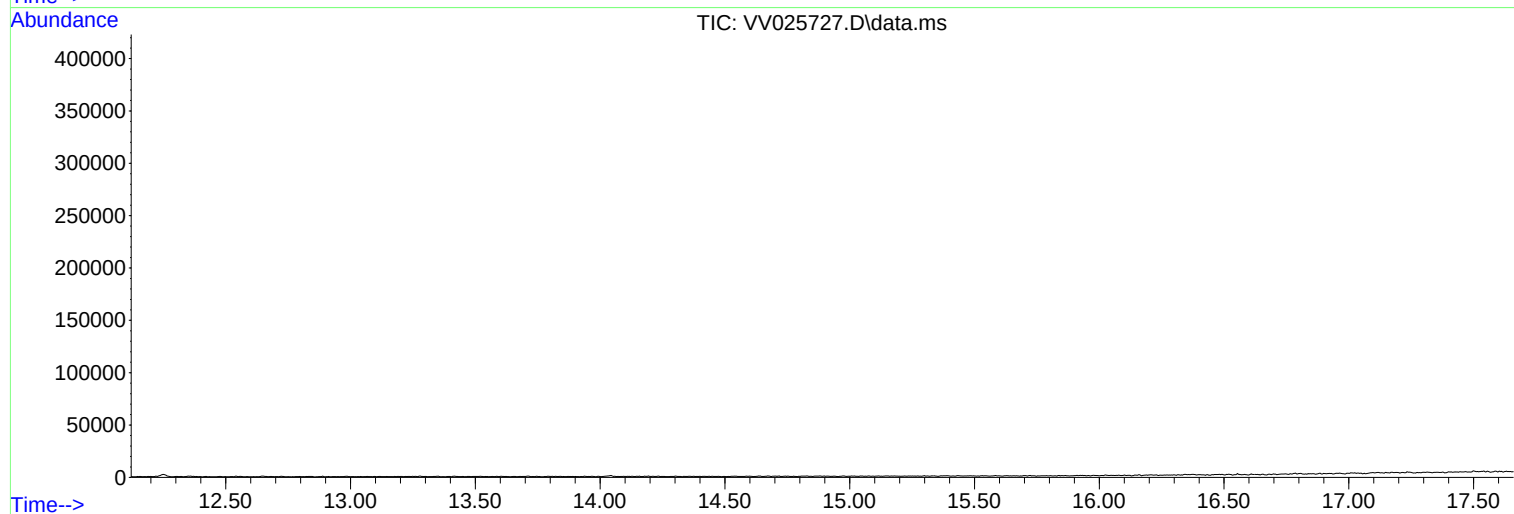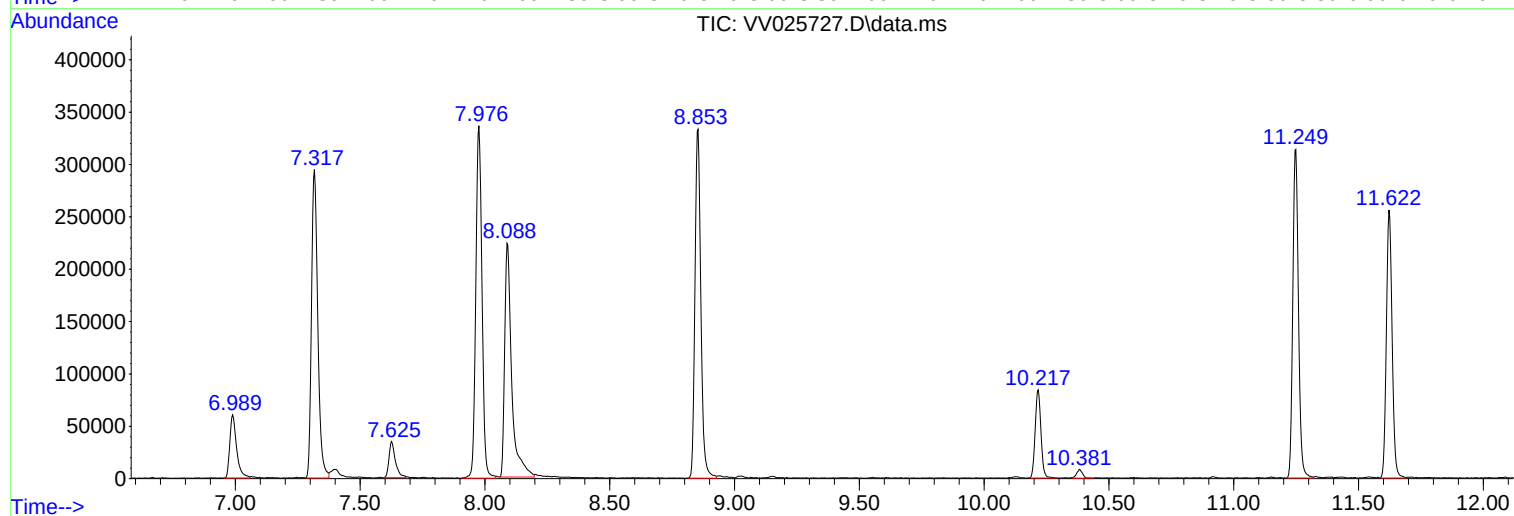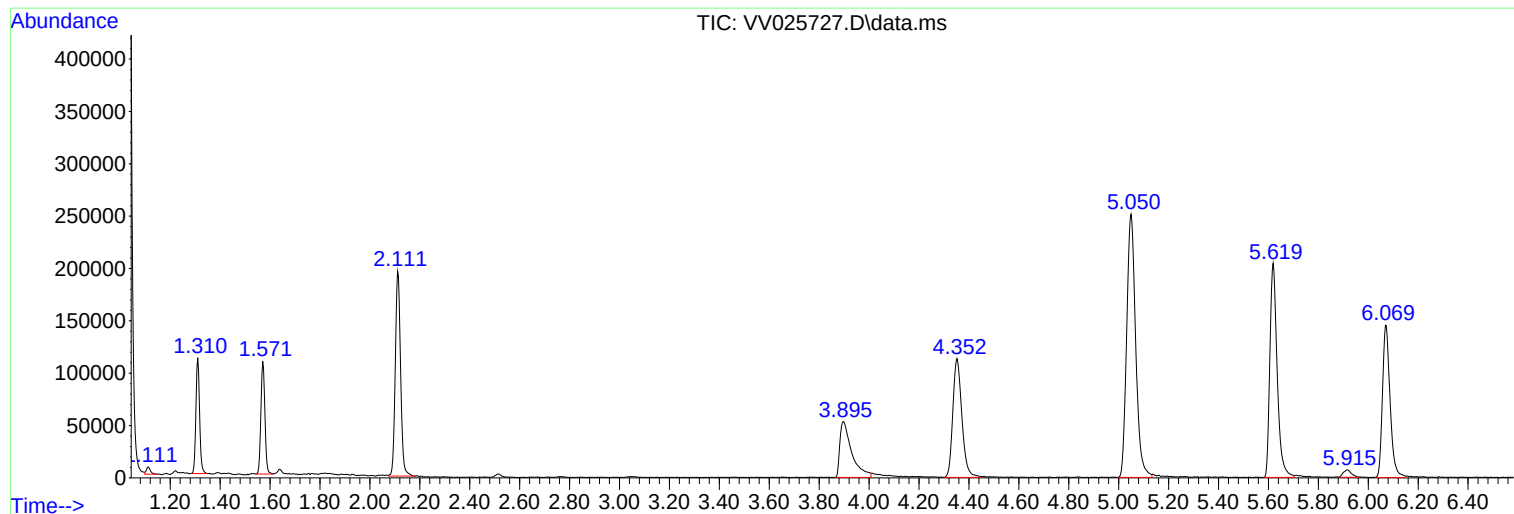

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042622\
Data File : VV025727.D
Acq On : 26 Apr 2022 12:47
Operator : SY/MD
Sample : N2492-21
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6W7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042622\
Data File : VV025727.D
Acq On : 26 Apr 2022 12:47
Operator : SY/MD
Sample : N2492-21
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6W7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc