

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042622\
 Data File : VV025728.D
 Acq On : 26 Apr 2022 13:10
 Operator : SY/MD
 Sample : N2492-16DL 100X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6W4DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025728.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	75	84	99	rVB	123643	128884	17.73%	2.048%
2	1.571	157	165	175	rBV	120381	136712	18.81%	2.172%
3	2.111	320	333	353	rBV	220089	322221	44.34%	5.120%
4	2.513	450	458	472	rVB3	5464	9442	1.30%	0.150%
5	3.902	878	890	937	rBV	61834	233088	32.07%	3.704%
6	4.352	1009	1030	1062	rBV	132139	332060	45.69%	5.277%
7	5.050	1231	1247	1276	rBV2	288113	726779	100.00%	11.549%
8	5.619	1412	1424	1447	rBV	238387	490775	67.53%	7.799%
9	5.915	1506	1516	1534	rBV7	11700	27844	3.83%	0.442%
10	6.069	1550	1564	1593	rBV	170447	354100	48.72%	5.627%
11	6.989	1839	1850	1873	rBV2	69326	134232	18.47%	2.133%
12	7.317	1936	1952	1971	rBV	331771	596814	82.12%	9.484%
13	7.625	2038	2048	2073	rBV	39377	73597	10.13%	1.170%
14	7.976	2133	2157	2176	rBV	193831	338107	46.52%	5.373%
15	8.088	2182	2192	2228	rBV	257580	519788	71.52%	8.260%
16	8.850	2415	2429	2451	rBV	385750	637484	87.71%	10.130%
17	10.214	2843	2853	2869	rBV2	98678	154479	21.26%	2.455%
18	10.381	2896	2905	2917	rVB3	6682	11523	1.59%	0.183%
19	11.246	3162	3174	3193	rBV	379630	591285	81.36%	9.396%
20	11.622	3279	3291	3313	rBV	293911	473720	65.18%	7.528%




Sum of corrected areas: 6292934

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042622\
Data File : VV025728.D
Acq On : 26 Apr 2022 13:10
Operator : SY/MD
Sample : N2492-16DL 100X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6W4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

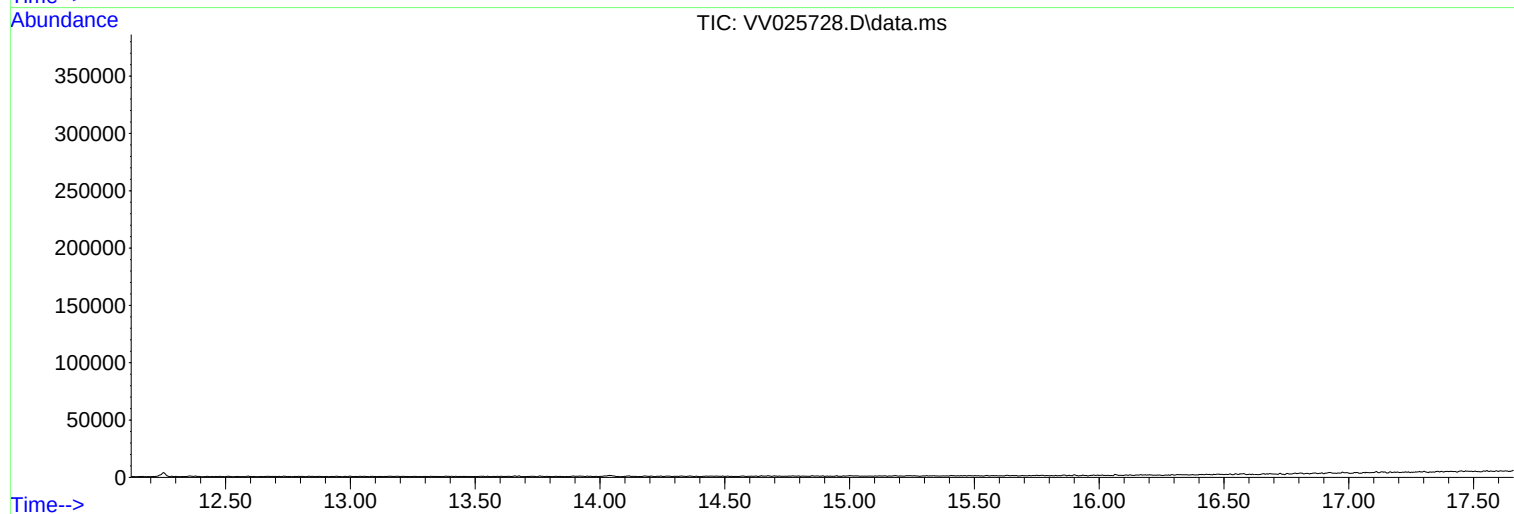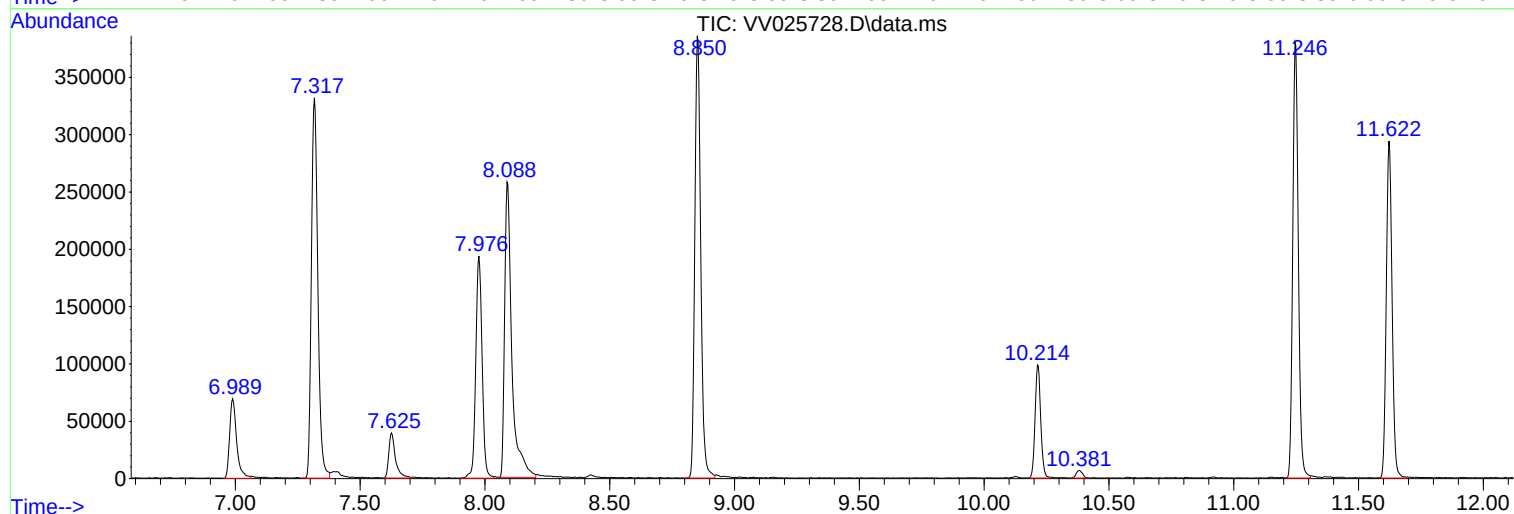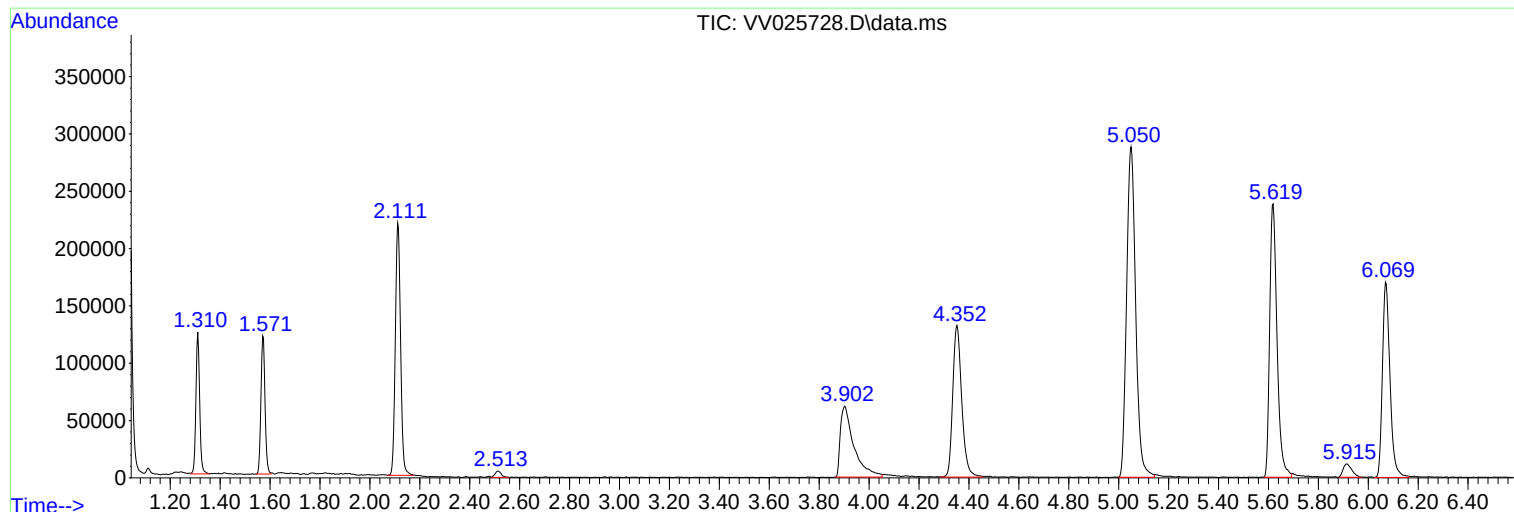

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042622\
Data File : VV025728.D
Acq On : 26 Apr 2022 13:10
Operator : SY/MD
Sample : N2492-16DL 100X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6W4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042622\
Data File : VV025728.D
Acq On : 26 Apr 2022 13:10
Operator : SY/MD
Sample : N2492-16DL 100X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6W4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------