
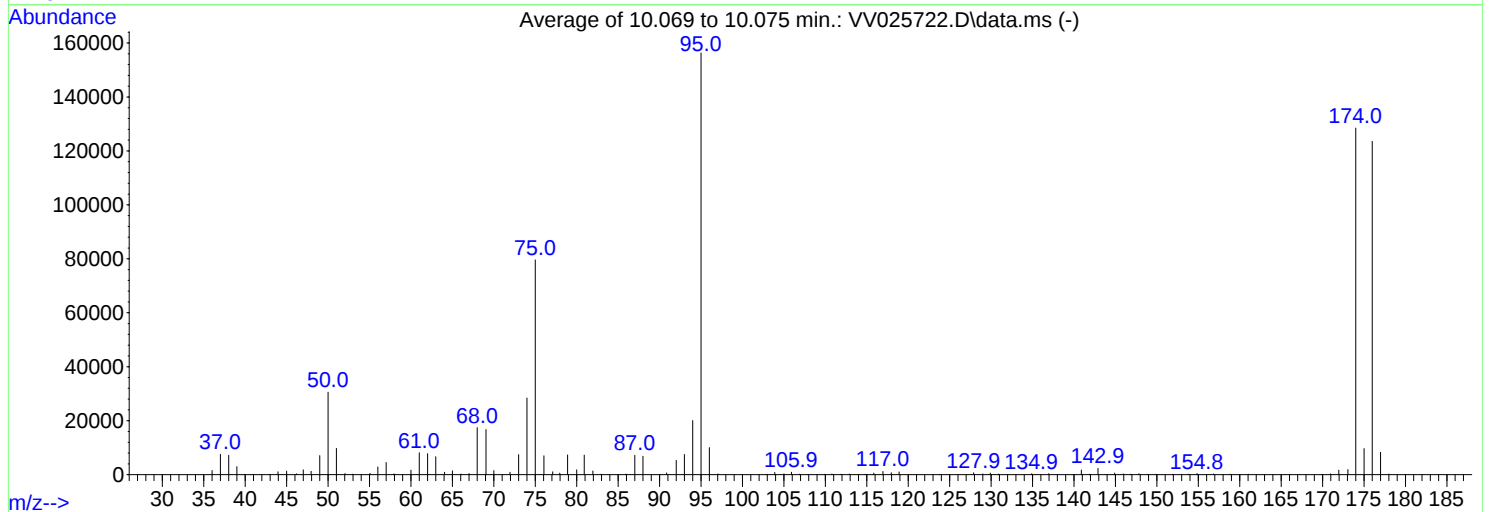


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042622\
 Data File : VV025722.D
 Acq On : 26 Apr 2022 09:39
 Operator : SY/MD
 Sample : BFB310
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB310

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Wed Apr 27 05:32:04 2022

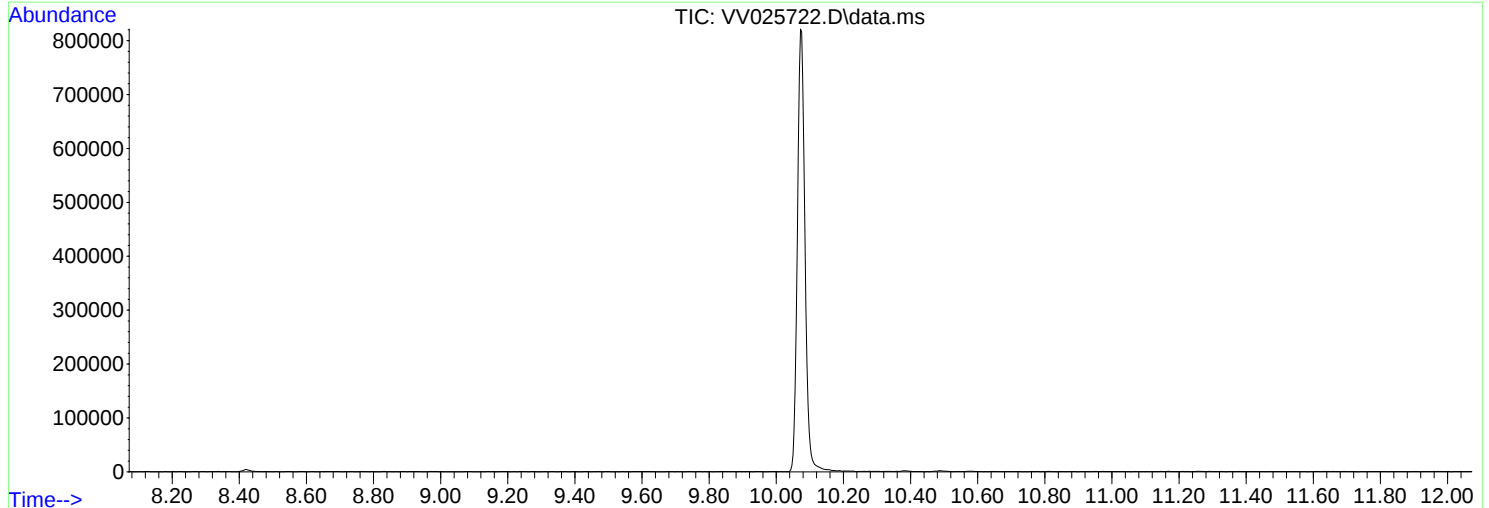

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.5	30523	PASS
75	95	30	80	50.9	79605	PASS
95	95	100	100	100.0	156352	PASS
96	95	5	9	6.4	10055	PASS
173	174	0.00	2	1.5	1928	PASS
174	95	50	120	82.2	128475	PASS
175	174	5	9	7.5	9649	PASS
176	174	95	105	96.2	123573	PASS
177	176	5	10	6.7	8290	PASS

m/z	Abundance
39.80	181.0
43.90	268.0

Instrument :
MSVOA_V
ClientSampleId :
BFB310

m/z	Abundance
36.00	1447.0
37.00	7243.0
38.00	6846.0
39.00	2751.0
40.00	288.0
42.90	107.0
44.00	1312.0
45.00	1196.0
46.20	284.0
47.00	1760.0
47.90	1208.0
49.00	6650.0
50.00	28712.0
51.00	9249.0
52.10	465.0
53.00	197.0
54.10	118.0
55.10	454.0
56.00	2713.0
57.00	4334.0
57.90	288.0
60.00	1564.0
61.00	7993.0
62.00	7300.0
63.00	6456.0
64.00	1003.0
65.00	1373.0
66.00	179.0
67.00	417.0
68.00	17136.0
69.10	16208.0
70.00	1251.0
72.00	858.0
73.00	7108.0
74.00	27296.0
75.00	75560.0
76.10	6756.0
77.10	1092.0
78.00	605.0
78.90	7049.0
80.00	1746.0
80.90	6901.0
82.00	1363.0
83.00	169.0
86.00	224.0
87.00	6724.0
88.00	6369.0
90.90	708.0
92.00	4917.0
93.00	7168.0
94.00	18888.0
95.00	147328.0
96.00	9481.0
97.10	248.0
102.80	103.0
103.90	795.0
105.00	243.0
105.90	813.0
106.90	202.0
107.90	114.0
110.00	184.0
110.80	169.0
111.90	106.0
112.90	229.0
114.80	198.0
115.80	550.0
117.00	1185.0
117.90	650.0
118.90	903.0
127.90	686.0
129.00	237.0
129.90	575.0
130.90	247.0
134.90	324.0
137.00	369.0
139.90	178.0
140.90	1557.0
141.90	186.0
142.90	2165.0
143.90	140.0
144.90	625.0
146.00	290.0
146.90	143.0
147.90	382.0
149.80	186.0
153.00	156.0
153.80	123.0
154.80	369.0
156.80	279.0
158.90	190.0
161.00	168.0
170.00	141.0

Instrument :
MSVOA_V
ClientSampleId :
BFB310

171.00	318.0
171.90	1509.0
173.10	1728.0
174.00	118608.0
175.00	8873.0
176.00	111984.0
177.00	7714.0
178.00	221.0

Instrument :
MSVOA_V
ClientSampleId :
BFB310

m/z	Abundance
36.00	1654.0
37.00	7861.0
38.00	7539.0
39.00	3035.0
40.00	309.0
40.70	132.0
42.90	132.0
44.00	1387.0
45.00	1313.0
46.20	309.0
47.00	1888.0
47.90	1278.0
49.00	7408.0
50.00	31552.0
51.00	10170.0
52.10	445.0
52.90	209.0
54.00	125.0
55.10	500.0
56.00	2939.0
57.00	4714.0
57.90	320.0
60.00	1763.0
61.00	8316.0
62.00	7914.0
63.00	6874.0
64.00	963.0
65.00	1424.0
66.10	244.0
67.00	452.0
68.00	18056.0
69.00	17248.0
70.00	1510.0
72.00	915.0
73.00	7699.0
74.00	29296.0
75.00	82080.0
76.10	7283.0
77.10	1126.0
78.00	607.0
78.90	7668.0
80.00	1826.0
80.90	7492.0
82.00	1443.0
83.00	177.0
86.00	301.0
87.00	7466.0
88.00	6953.0
90.90	670.0
92.00	5483.0
93.00	7694.0
94.00	20688.0
95.00	161984.0
96.00	10429.0
97.10	303.0
103.90	811.0
105.00	285.0
105.90	959.0
106.90	218.0
107.90	158.0
110.00	163.0
110.80	248.0
111.90	162.0
112.90	267.0
114.80	201.0
115.90	626.0
116.90	1244.0
118.00	767.0
118.90	1022.0
123.80	125.0
127.90	757.0
129.00	284.0
129.90	629.0
130.90	239.0
134.90	373.0
137.00	364.0
139.90	163.0
140.90	1772.0
141.90	192.0
142.90	2394.0
143.80	126.0
144.90	644.0
145.90	332.0
146.90	190.0
147.80	410.0
148.90	120.0
149.90	227.0
151.90	101.0
153.00	202.0
153.80	184.0
154.90	431.0
156.90	310.0

Instrument :
MSVOA_V
ClientSampleId :
BFB310

158.90	192.0
161.10	174.0
169.90	142.0
171.00	345.0
172.00	1742.0
173.10	1992.0
174.00	132992.0
175.00	9952.0
176.00	127928.0
177.00	8572.0
178.00	237.0

Instrument :
MSVOA_V
ClientSampleId :
BFB310

m/z	Abundance
36.00	1562.0
37.00	7539.0
38.00	7186.0
39.00	3116.0
40.00	280.0
42.90	148.0
44.00	1325.0
45.00	1335.0
46.20	256.0
47.00	1714.0
48.00	1287.0
49.00	7136.0
50.00	31304.0
51.00	9858.0
52.00	414.0
52.90	181.0
54.00	126.0
55.00	496.0
56.00	2879.0
57.00	4567.0
58.00	291.0
60.00	1705.0
61.00	8074.0
62.00	8083.0
63.00	6653.0
64.10	814.0
65.00	1414.0
66.10	267.0
67.00	406.0
68.00	17192.0
69.00	16768.0
70.00	1636.0
71.90	889.0
73.00	7486.0
74.00	28568.0
75.00	81176.0
76.00	7015.0
77.10	977.0
77.90	608.0
78.90	7216.0
80.00	1835.0
80.90	7233.0
81.90	1374.0
82.90	202.0
85.90	265.0
87.00	7336.0
88.00	7143.0
90.80	626.0
92.00	5465.0
93.00	7585.0
94.00	20560.0
95.00	159744.0
96.00	10255.0
97.00	300.0
103.90	826.0
105.00	317.0
105.90	971.0
106.90	185.0
107.90	124.0
109.90	125.0
110.80	281.0
111.90	223.0
112.90	238.0
115.00	210.0
115.90	689.0
116.90	1204.0
118.00	794.0
118.90	1078.0
123.70	157.0
127.90	741.0
129.00	301.0
129.90	627.0
130.90	216.0
134.90	340.0
136.90	319.0
140.90	1792.0
141.90	204.0
142.90	2425.0
143.80	100.0
144.90	579.0
145.90	332.0
146.80	170.0
147.80	379.0
148.90	143.0
150.00	210.0
151.90	102.0
153.00	174.0
153.80	179.0
154.90	459.0
156.90	330.0
158.80	185.0
161.10	166.0

Instrument :
MSVOA_V
ClientSampleId :
BFB310

169.80	126.0
170.80	326.0
172.00	1690.0
173.00	2063.0
174.00	133824.0
175.00	10122.0
176.00	130808.0
177.00	8584.0
178.00	254.0

Instrument :
MSVOA_V
ClientSampleId :
BFB310