

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060222\
 Data File : VV025981.D
 Acq On : 02 Jun 2022 13:57
 Operator : SY/MD
 Sample : N3173-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXEK3

Quant Time: Jun 03 00:07:08 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jun 03 00:06:32 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	350335	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	349278	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	161784	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	170199	37.643	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	75.280%		
7) Chloroethane-d5	1.568	69	150885	38.000	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	76.000%		
11) 1,1-Dichloroethene-d2	2.108	63	251135	31.758	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	63.520%		
21) 2-Butanone-d5	3.892	46	110677	57.111	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	57.110%		
24) Chloroform-d	4.346	84	284970	45.124	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	90.240%		
26) 1,2-Dichloroethane-d4	5.031	65	171291	44.879	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	89.760%		
32) Benzene-d6	5.047	84	570570	46.859	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	93.720%		
36) 1,2-Dichloropropane-d6	6.066	67	181459	48.521	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	97.040%		
41) Toluene-d8	7.314	98	501997	44.746	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	89.500%		
43) trans-1,3-Dichloroprop...	7.619	79	69950	41.900	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	83.800%		
47) 2-Hexanone-d5	8.088	63	110220	80.387	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	80.390%		
56) 1,1,2,2-Tetrachloroeth...	10.214	84	230734	46.264	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	92.520%		
66) 1,2-Dichlorobenzene-d4	11.622	152	186594	52.579	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	105.160%		
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	6.986	75	4457	1.058	ug/L	# 69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060222\
Data File : VV025981.D
Acq On : 02 Jun 2022 13:57
Operator : SY/MD
Sample : N3173-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXEK3

Quant Time: Jun 03 00:07:08 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jun 03 00:06:32 2022
Response via : Initial Calibration

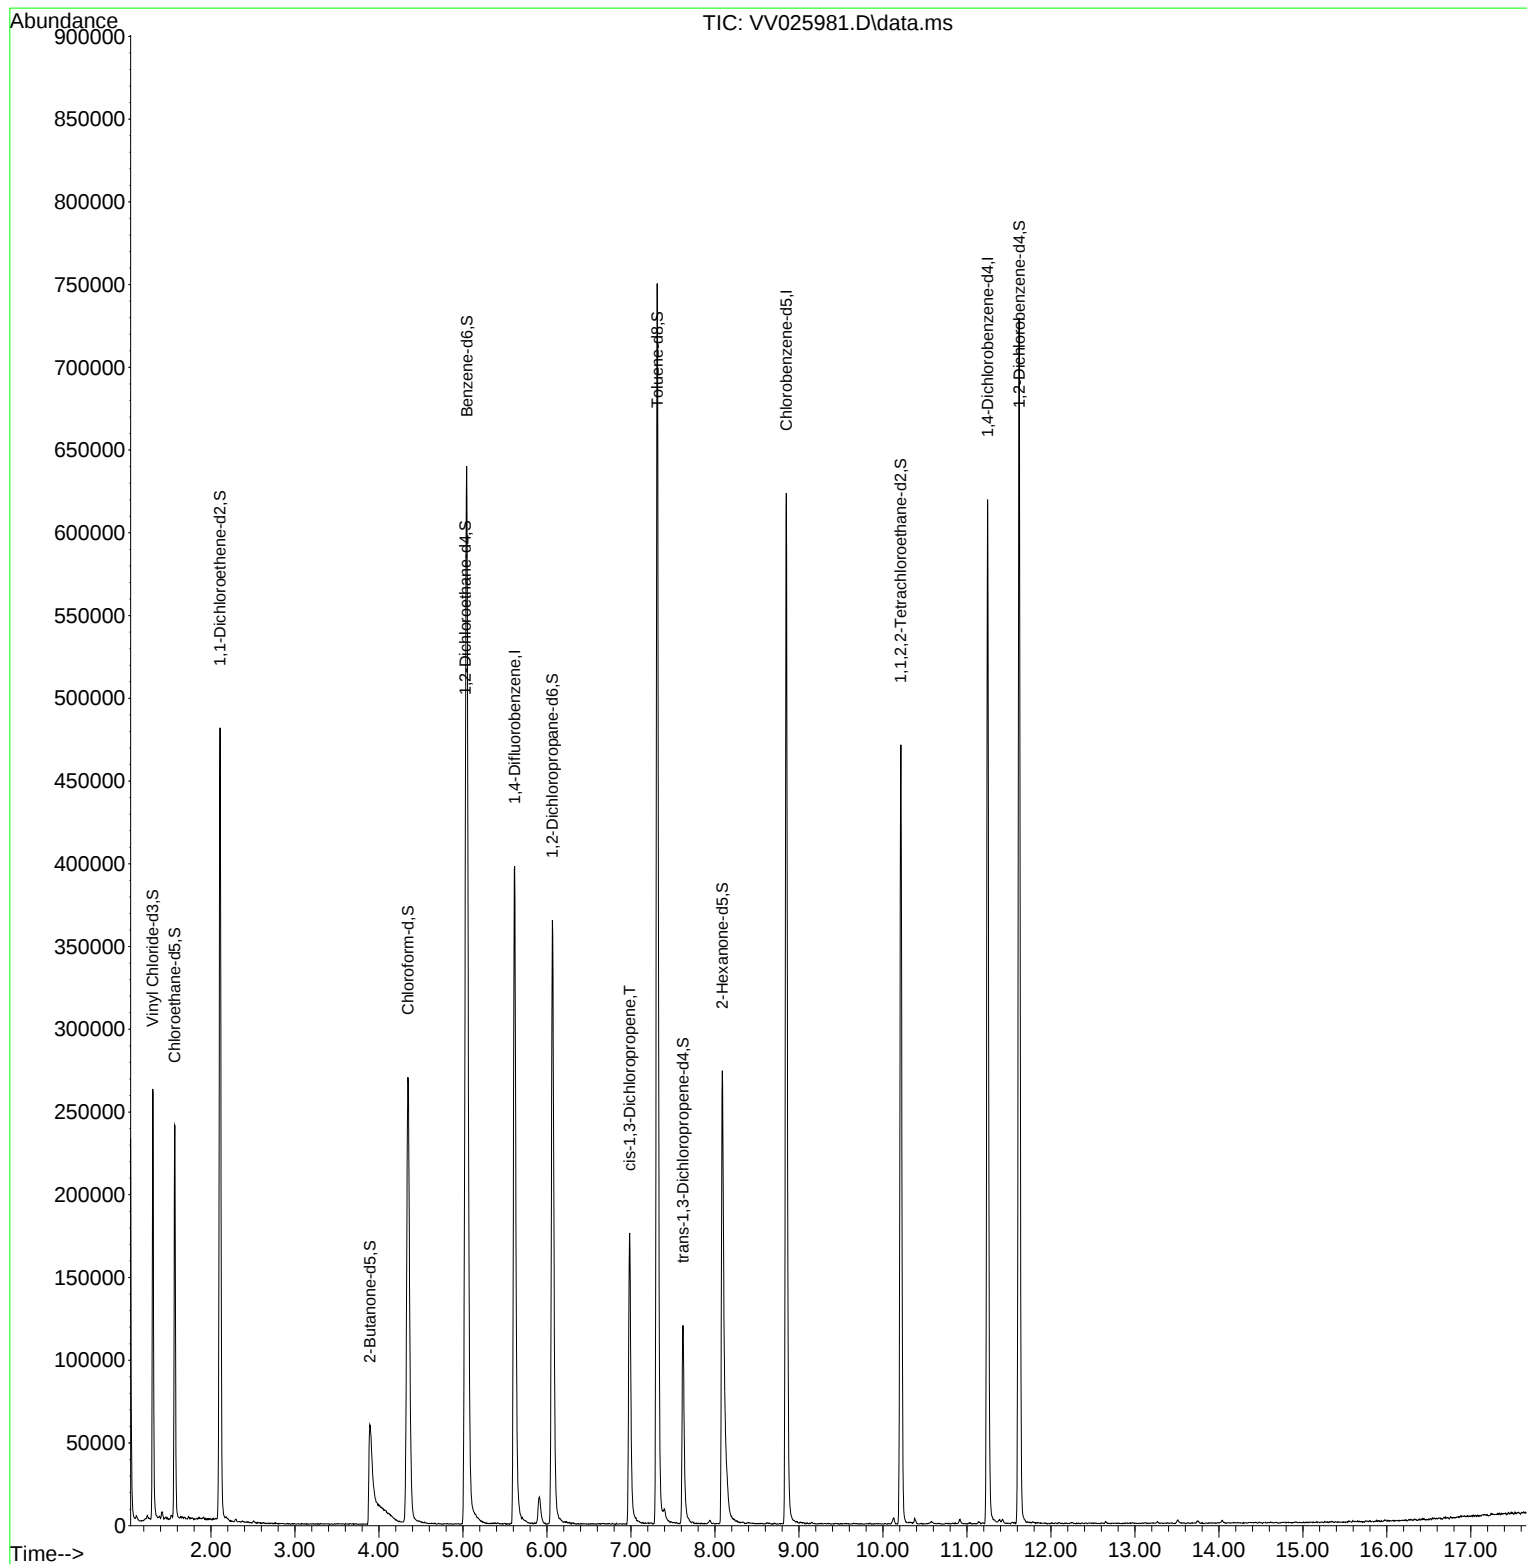

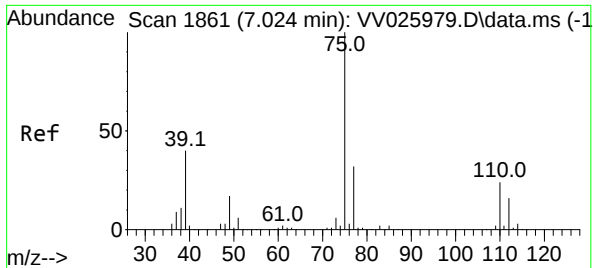

#39
 cis-1,3-Dichloropropene
 Concen: 1.058 ug/L
 RT: 6.986 min Scan# 11
 Delta R.T. -0.039 min
 Lab File: VV025981.D
 Acq: 02 Jun 2022 13:57

Instrument :
 MSVOA_V
 ClientSampleId :
 EXEK3

Tgt Ion: 75 Resp: 4457
 Ion Ratio Lower Upper
 75 100
 77 49.0 22.4 41.6#

