




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV060222\  
 Data File : VV025982.D  
 Acq On : 02 Jun 2022 14:21  
 Operator : SY/MD  
 Sample : N3173-02  
 Misc : 5.0mL/MSVOA\_V/WATER  
 ALS Vial : 5 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 EXEK5

Manual IntegrationsAPPROVED

Quant Time: Jun 03 00:07:21 2022  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVLM051022WMA.M  
 Quant Title : VOC Analysis  
 QLast Update : Fri Jun 03 00:06:32 2022  
 Response via : Initial Calibration

Reviewed By :John Carlone 06/06/2022  
 Supervised By :Mahesh Dadoda 06/06/2022

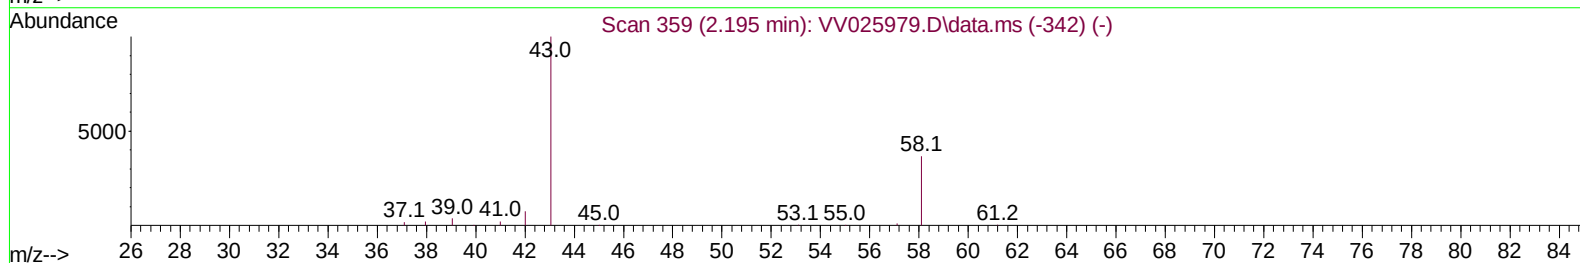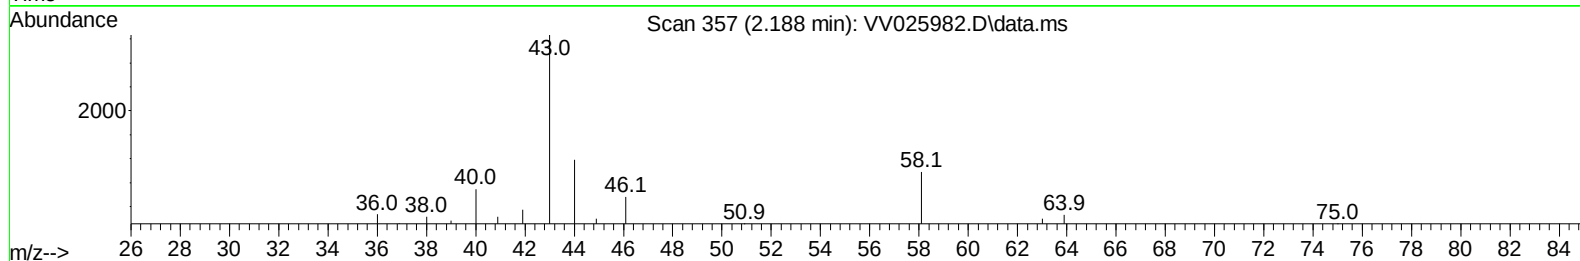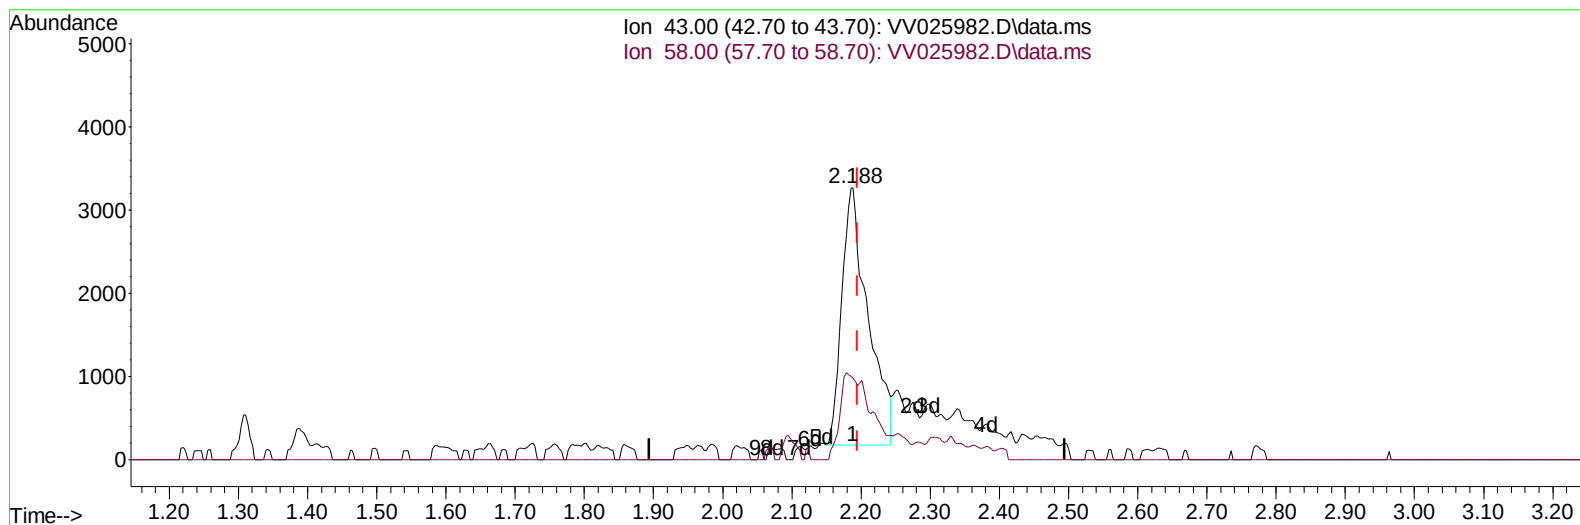

TIC: VV025982.D\data.ms

(13) Acetone (T)

2.188min (-0.006) 6.85 ug/L

response 8163

| Ion   | Exp%   | Act%   |
|-------|--------|--------|
| 43.00 | 100.00 | 100.00 |
| 58.00 | 32.50  | 21.22  |
| 0.00  | 0.00   | 0.00   |
| 0.00  | 0.00   | 0.00   |




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV060222\  
 Data File : VV025982.D  
 Acq On : 02 Jun 2022 14:21  
 Operator : SY/MD  
 Sample : N3173-02  
 Misc : 5.0mL/MSVOA\_V/WATER  
 ALS Vial : 5 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 EXEK5

Manual IntegrationsAPPROVED

Quant Time: Jun 03 00:07:21 2022  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVLM051022WMA.M  
 Quant Title : VOC Analysis  
 QLast Update : Fri Jun 03 00:06:32 2022  
 Response via : Initial Calibration

Reviewed By :John Carlone 06/06/2022  
 Supervised By :Mahesh Dadoda 06/06/2022

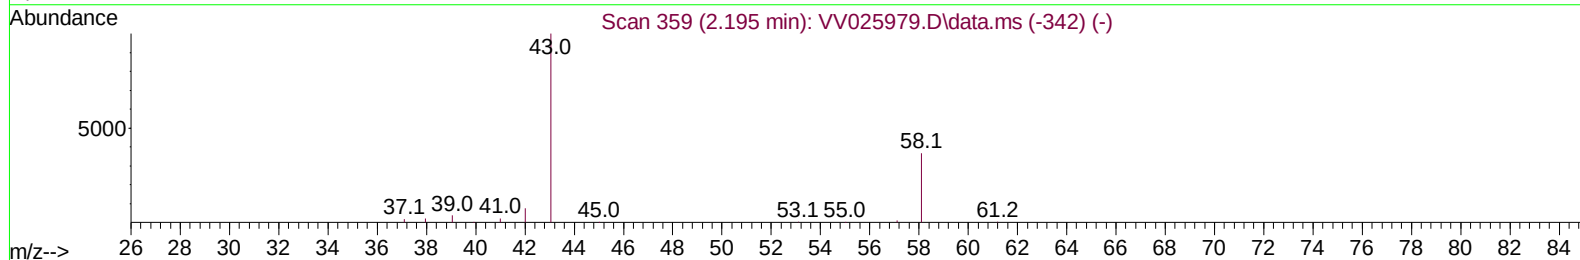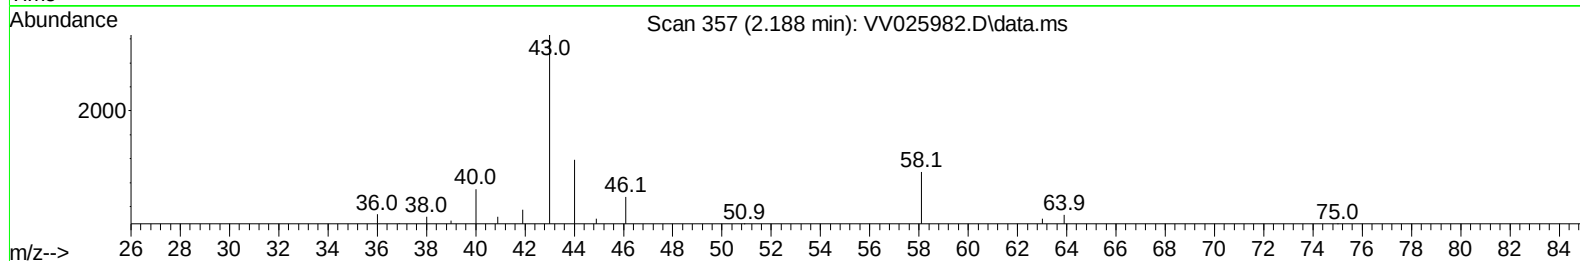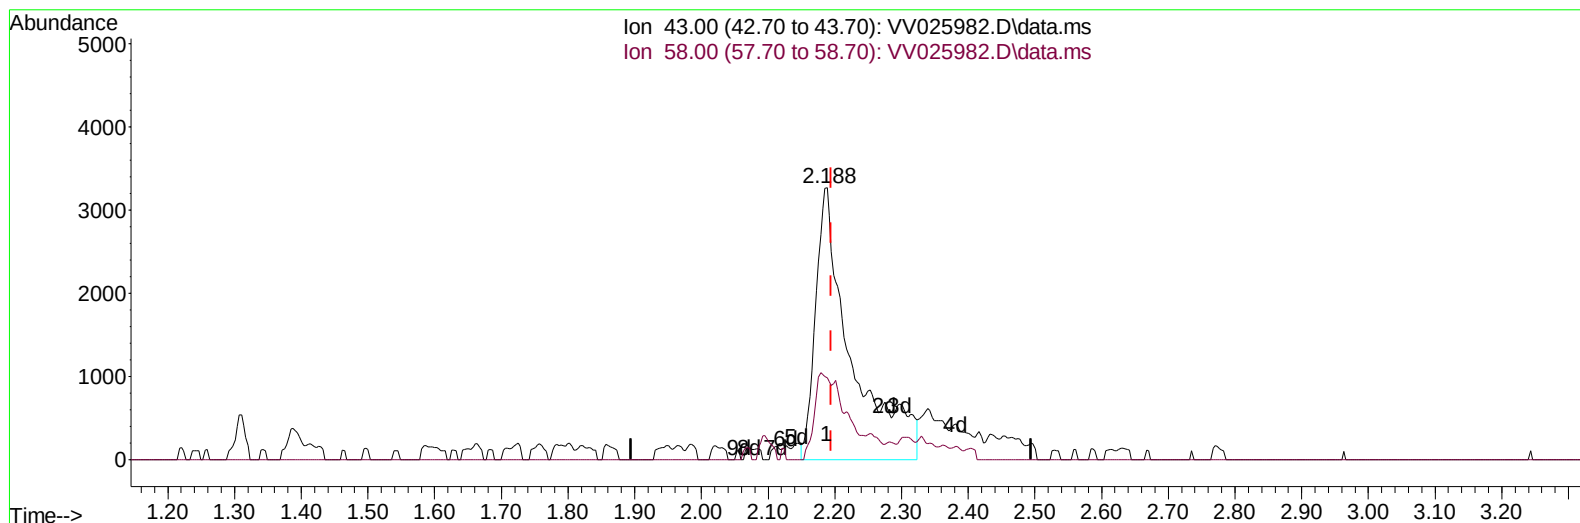

TIC: VV025982.D\data.ms

(13) Acetone (T)

2.188min (-0.006) 10.17 ug/L m

response 12118

| Ion   | Exp%   | Act%   |
|-------|--------|--------|
| 43.00 | 100.00 | 100.00 |
| 58.00 | 32.50  | 14.29  |
| 0.00  | 0.00   | 0.00   |
| 0.00  | 0.00   | 0.00   |

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV060222\  
 Data File : VV025982.D  
 Acq On : 02 Jun 2022 14:21  
 Operator : SY/MD  
 Sample : N3173-02  
 Misc : 5.0mL/MSVOA\_V/WATER  
 ALS Vial : 5 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 EXEK5

Manual IntegrationsAPPROVED

Quant Time: Jun 03 00:07:21 2022  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVLM051022WMA.M  
 Quant Title : VOC Analysis  
 QLast Update : Fri Jun 03 00:06:32 2022  
 Response via : Initial Calibration

Reviewed By :John Carlone 06/06/2022  
 Supervised By :Mahesh Dadoda 06/06/2022

| Compound                      | R.T.     | Q     | Ion | Response | Conc   | Units    | Dev(Min) |
|-------------------------------|----------|-------|-----|----------|--------|----------|----------|
| -----                         |          |       |     |          |        |          |          |
| Internal Standards            |          |       |     |          |        |          |          |
| 1) 1,4-Difluorobenzene        | 5.616    | 114   |     | 315554   | 50.000 | ug/L     | 0.00     |
| 28) Chlorobenzene-d5          | 8.850    | 117   |     | 314508   | 50.000 | ug/L     | 0.00     |
| 58) 1,4-Dichlorobenzene-d4    | 11.249   | 152   |     | 140418   | 50.000 | ug/L     | 0.00     |
| System Monitoring Compounds   |          |       |     |          |        |          |          |
| 4) Vinyl Chloride-d3          | 1.307    | 65    |     | 148018   | 36.346 | ug/L     | 0.00     |
| Spiked Amount 50.000          | Range 60 | - 135 |     | Recovery | =      | 72.700%  |          |
| 7) Chloroethane-d5            | 1.571    | 69    |     | 128157   | 35.834 | ug/L     | 0.00     |
| Spiked Amount 50.000          | Range 70 | - 130 |     | Recovery | =      | 71.660%  |          |
| 11) 1,1-Dichloroethene-d2     | 2.108    | 63    |     | 216663   | 30.419 | ug/L     | 0.00     |
| Spiked Amount 50.000          | Range 60 | - 125 |     | Recovery | =      | 60.840%  |          |
| 21) 2-Butanone-d5             | 3.896    | 46    |     | 120369   | 68.958 | ug/L     | 0.00     |
| Spiked Amount 100.000         | Range 40 | - 130 |     | Recovery | =      | 68.960%  |          |
| 24) Chloroform-d              | 4.349    | 84    |     | 249137   | 43.799 | ug/L     | 0.00     |
| Spiked Amount 50.000          | Range 70 | - 125 |     | Recovery | =      | 87.600%  |          |
| 26) 1,2-Dichloroethane-d4     | 5.031    | 65    |     | 147594   | 42.933 | ug/L     | 0.00     |
| Spiked Amount 50.000          | Range 70 | - 125 |     | Recovery | =      | 85.860%  |          |
| 32) Benzene-d6                | 5.050    | 84    |     | 498107   | 45.430 | ug/L     | 0.00     |
| Spiked Amount 50.000          | Range 70 | - 125 |     | Recovery | =      | 90.860%  |          |
| 36) 1,2-Dichloropropane-d6    | 6.069    | 67    |     | 158414   | 47.042 | ug/L     | 0.00     |
| Spiked Amount 50.000          | Range 70 | - 120 |     | Recovery | =      | 94.080%  |          |
| 41) Toluene-d8                | 7.317    | 98    |     | 428011   | 42.369 | ug/L     | 0.00     |
| Spiked Amount 50.000          | Range 80 | - 120 |     | Recovery | =      | 84.740%  |          |
| 43) trans-1,3-Dichloroprop... | 7.622    | 79    |     | 62214    | 41.386 | ug/L     | 0.00     |
| Spiked Amount 50.000          | Range 60 | - 125 |     | Recovery | =      | 82.780%  |          |
| 47) 2-Hexanone-d5             | 8.088    | 63    |     | 106997   | 86.664 | ug/L     | 0.00     |
| Spiked Amount 100.000         | Range 45 | - 130 |     | Recovery | =      | 86.660%  |          |
| 56) 1,1,2,2-Tetrachloroeth... | 10.214   | 84    |     | 206436   | 45.968 | ug/L     | 0.00     |
| Spiked Amount 50.000          | Range 65 | - 120 |     | Recovery | =      | 91.940%  |          |
| 66) 1,2-Dichlorobenzene-d4    | 11.622   | 152   |     | 157111   | 51.007 | ug/L     | 0.00     |
| Spiked Amount 50.000          | Range 80 | - 120 |     | Recovery | =      | 102.020% |          |

|                  |       |    |        |        |      |  |        |
|------------------|-------|----|--------|--------|------|--|--------|
| Target Compounds |       |    |        |        |      |  | Qvalue |
| 13) Acetone      | 2.188 | 43 | 12118m | 10.173 | ug/L |  |        |

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV060222\  
Data File : VV025982.D  
Acq On : 02 Jun 2022 14:21  
Operator : SY/MD  
Sample : N3173-02  
Misc : 5.0mL/MSVOA\_V/WATER  
ALS Vial : 5 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
EXEK5

Manual IntegrationsAPPROVED

Quant Time: Jun 03 00:07:21 2022  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVLM051022WMA.M  
Quant Title : VOC Analysis  
QLast Update : Fri Jun 03 00:06:32 2022  
Response via : Initial Calibration

Reviewed By :John Carlone 06/06/2022  
Supervised By :Mahesh Dadoda 06/06/2022

