




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060222\
Data File : VV025984.D
Acq On : 02 Jun 2022 15:09
Operator : SY/MD
Sample : N3171-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBTZ0

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 06/06/2022
Supervised By :Mahesh Dadoda 06/06/2022

Quant Time: Jun 03 00:07:47 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jun 03 00:06:32 2022
Response via : Initial Calibration

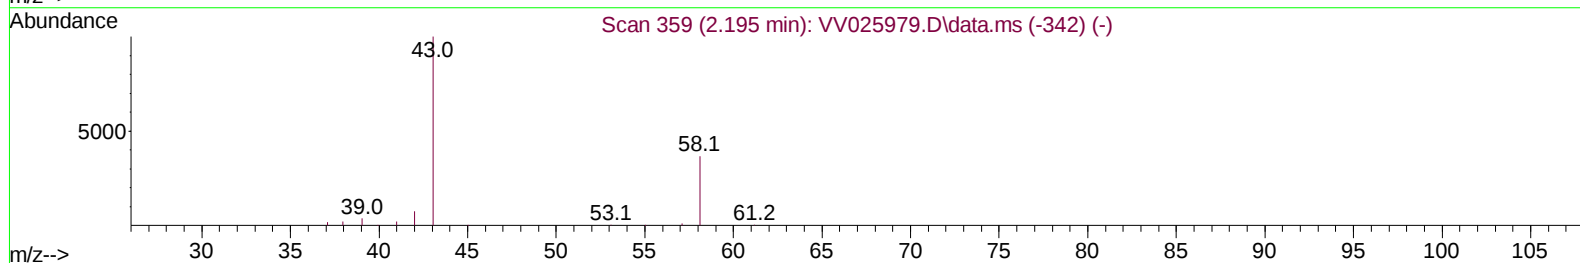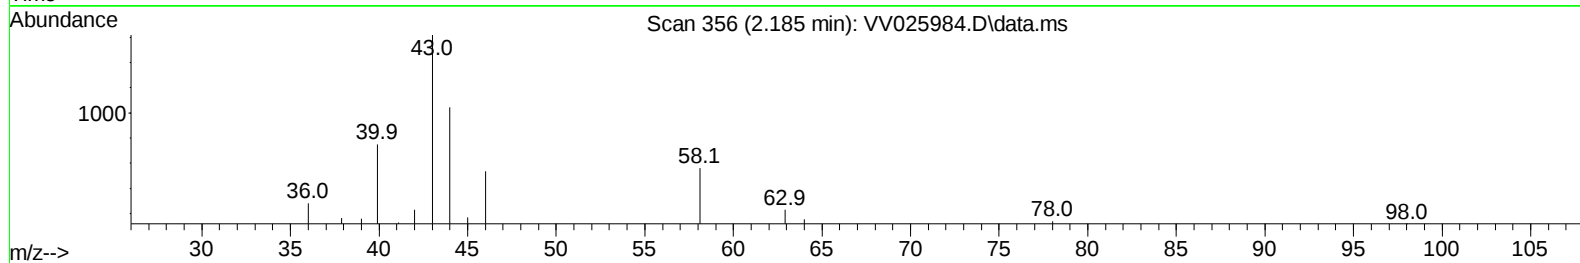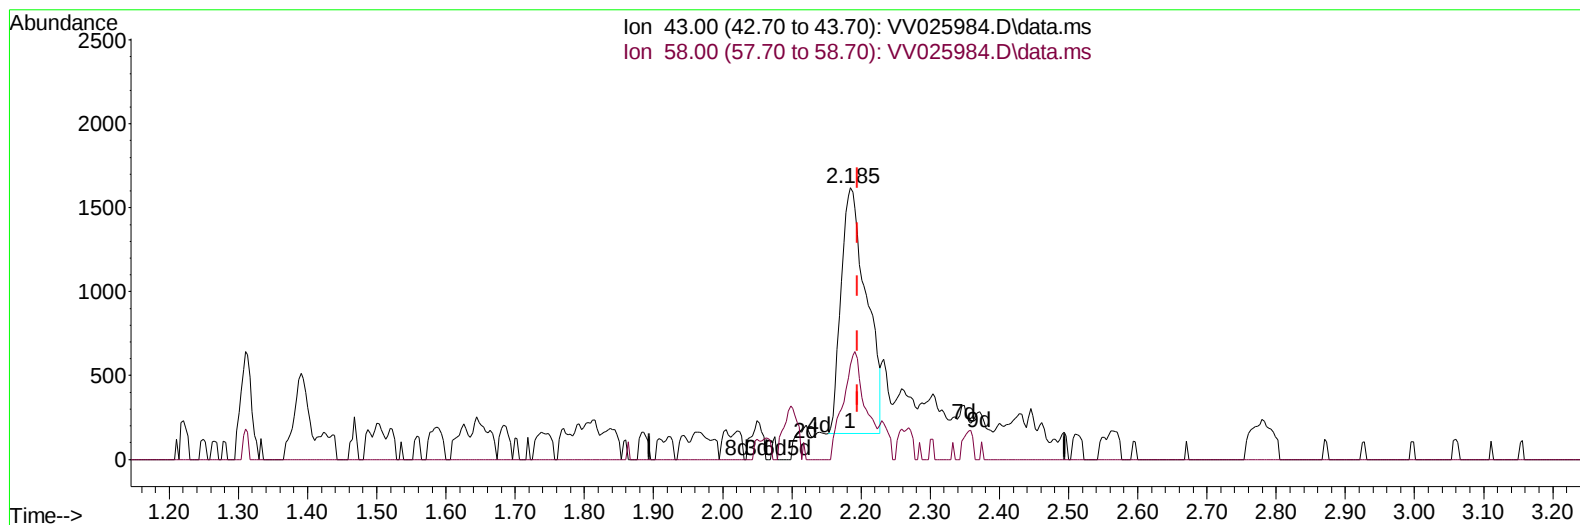

TIC: VV025984.D\data.ms

(13) Acetone (T)

2.185min (-0.010) 3.32 ug/L

response 3683

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.50	38.77
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060222\
 Data File : VV025984.D
 Acq On : 02 Jun 2022 15:09
 Operator : SY/MD
 Sample : N3171-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBTZ0

Manual IntegrationsAPPROVED

Quant Time: Jun 03 00:07:47 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jun 03 00:06:32 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 06/06/2022
 Supervised By :Mahesh Dadoda 06/06/2022

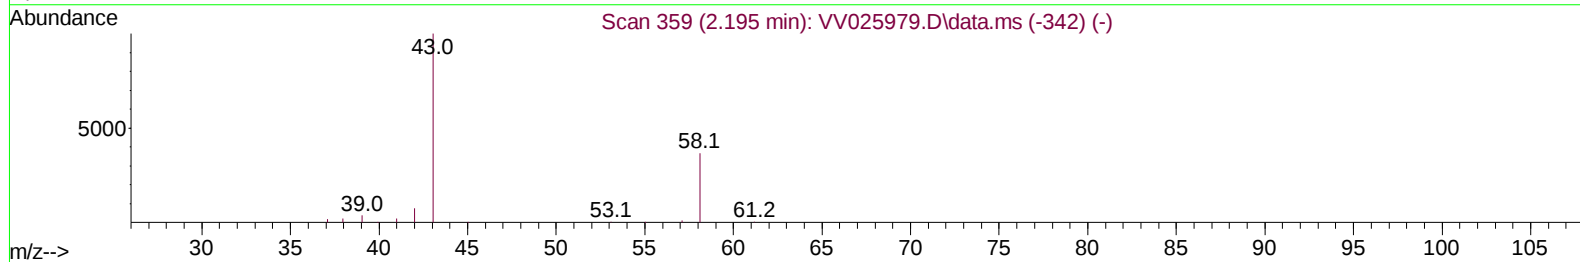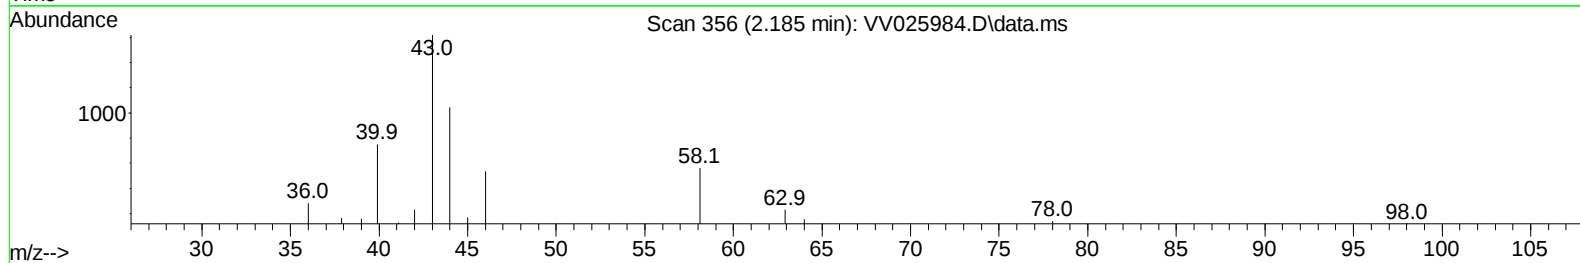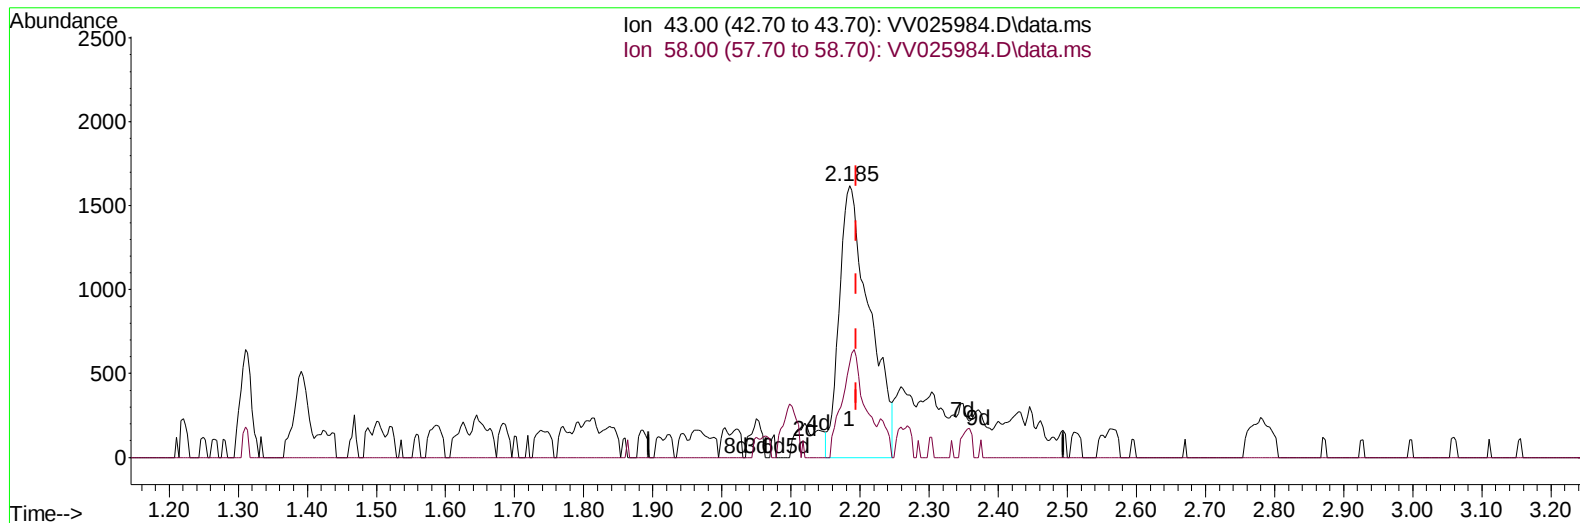

TIC: VV025984.D\data.ms

(13) Acetone (T)

2.185min (-0.010) 4.45 ug/L m

response 4933

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.50	28.95
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060222\
 Data File : VV025984.D
 Acq On : 02 Jun 2022 15:09
 Operator : SY/MD
 Sample : N3171-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBTZ0

Manual IntegrationsAPPROVED

Quant Time: Jun 03 00:07:47 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jun 03 00:06:32 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 06/06/2022
 Supervised By :Mahesh Dadoda 06/06/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	293666	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	294312	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	130974	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.310	65	154158	40.675	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	81.340%	
7) Chloroethane-d5	1.571	69	136407	40.983	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	81.960%	
11) 1,1-Dichloroethene-d2	2.111	63	224712	33.900	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	67.800%	
21) 2-Butanone-d5	3.899	46	113686	69.984	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	69.980%	
24) Chloroform-d	4.352	84	258369	48.807	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	97.620%	
26) 1,2-Dichloroethane-d4	5.034	65	153491	47.976	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	95.960%	
32) Benzene-d6	5.050	84	514226	50.119	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	100.240%	
36) 1,2-Dichloropropane-d6	6.072	67	163571	51.906	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	103.820%	
41) Toluene-d8	7.316	98	441021	46.652	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	93.300%	
43) trans-1,3-Dichloroprop...	7.622	79	64088	45.559	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	91.120%	
47) 2-Hexanone-d5	8.091	63	108372	93.801	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	93.800%	
56) 1,1,2,2-Tetrachloroeth...	10.213	84	215821	51.356	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	102.720%	
66) 1,2-Dichlorobenzene-d4	11.622	152	167018	58.133	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	116.260%	
Target Compounds						
13) Acetone	2.185	43	4933m	4.450	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060222\
Data File : VV025984.D
Acq On : 02 Jun 2022 15:09
Operator : SY/MD
Sample : N3171-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBTZ0

Manual IntegrationsAPPROVED

Quant Time: Jun 03 00:07:47 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jun 03 00:06:32 2022
Response via : Initial Calibration

Reviewed By :John Carlone 06/06/2022
Supervised By :Mahesh Dadoda 06/06/2022

