




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060222\
 Data File : VV025985.D
 Acq On : 02 Jun 2022 15:36
 Operator : SY/MD
 Sample : N3171-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBTZ3

Manual IntegrationsAPPROVED

Quant Time: Jun 03 00:08:00 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jun 03 00:06:32 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 06/06/2022
 Supervised By :Mahesh Dadoda 06/06/2022

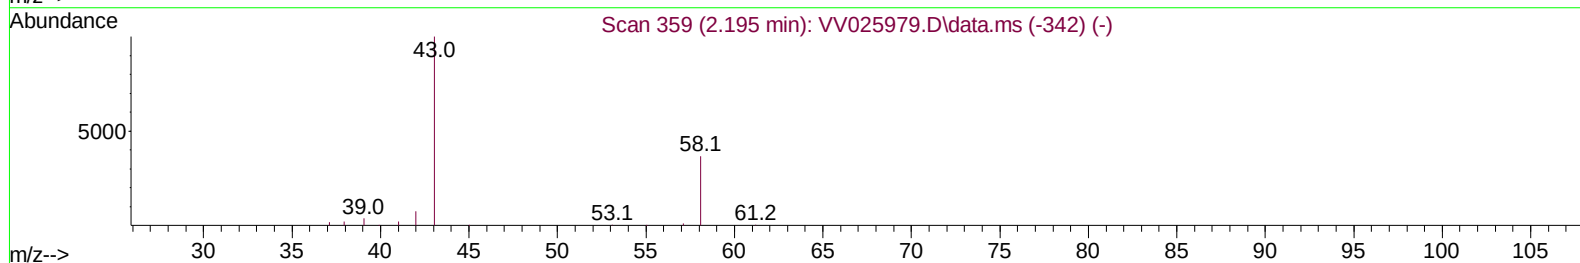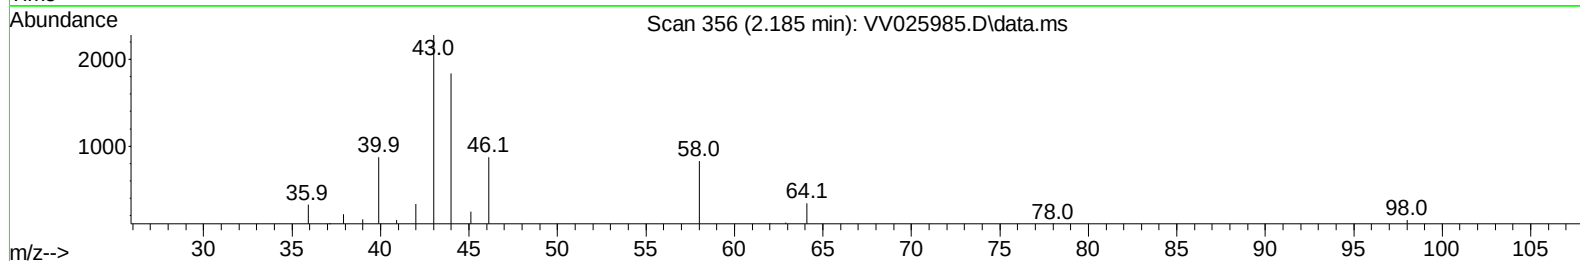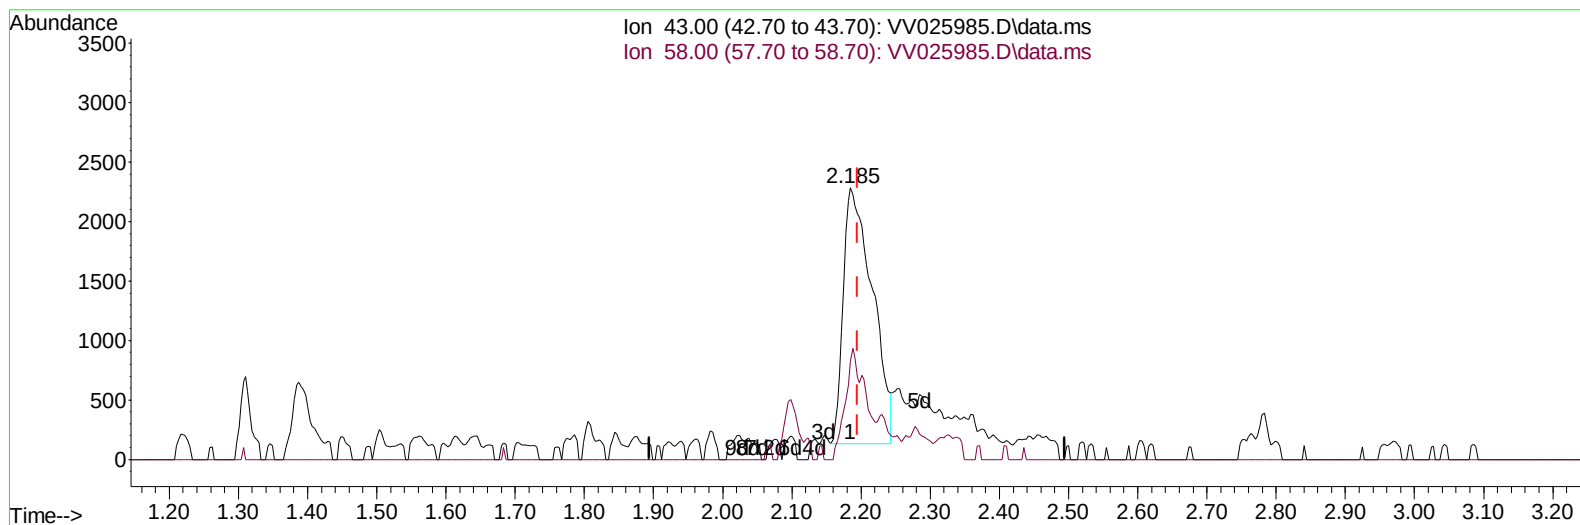

TIC: VV025985.D\data.ms

(13) Acetone (T)

2.185min (-0.010) 5.07 ug/L

response 6259

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.50	19.46
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060222\
 Data File : VV025985.D
 Acq On : 02 Jun 2022 15:36
 Operator : SY/MD
 Sample : N3171-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBT23

Manual IntegrationsAPPROVED

Quant Time: Jun 03 00:08:00 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jun 03 00:06:32 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 06/06/2022
 Supervised By :Mahesh Dadoda 06/06/2022

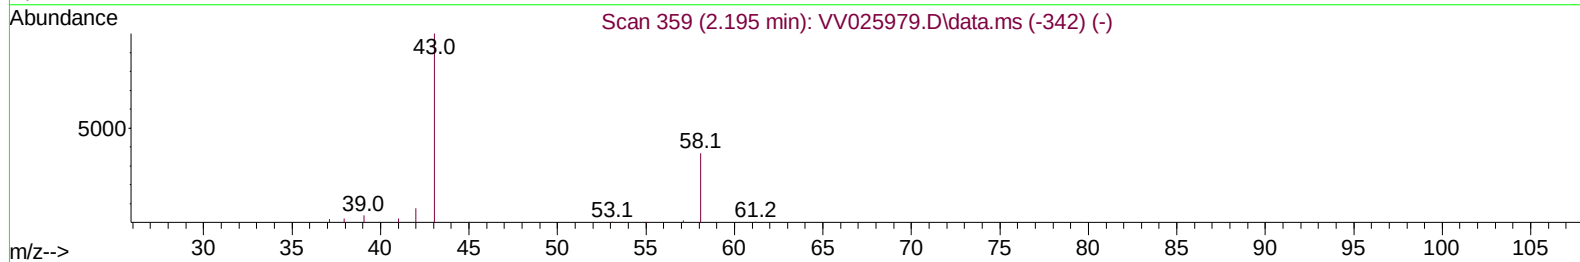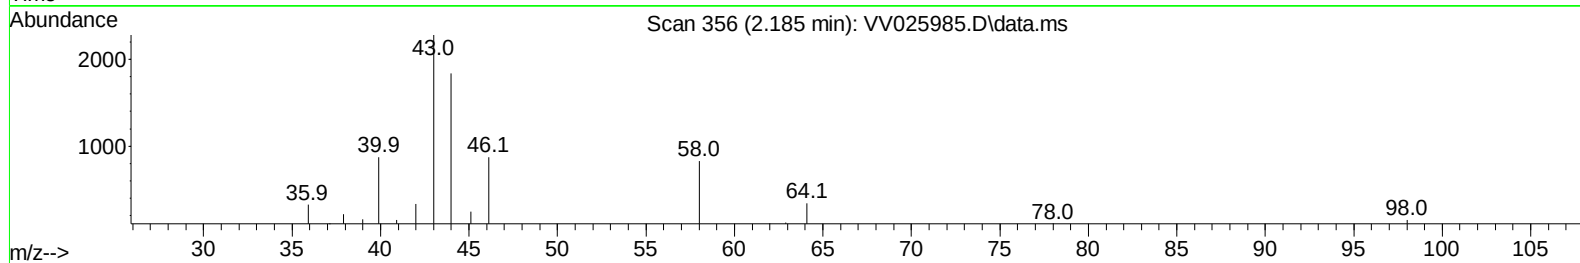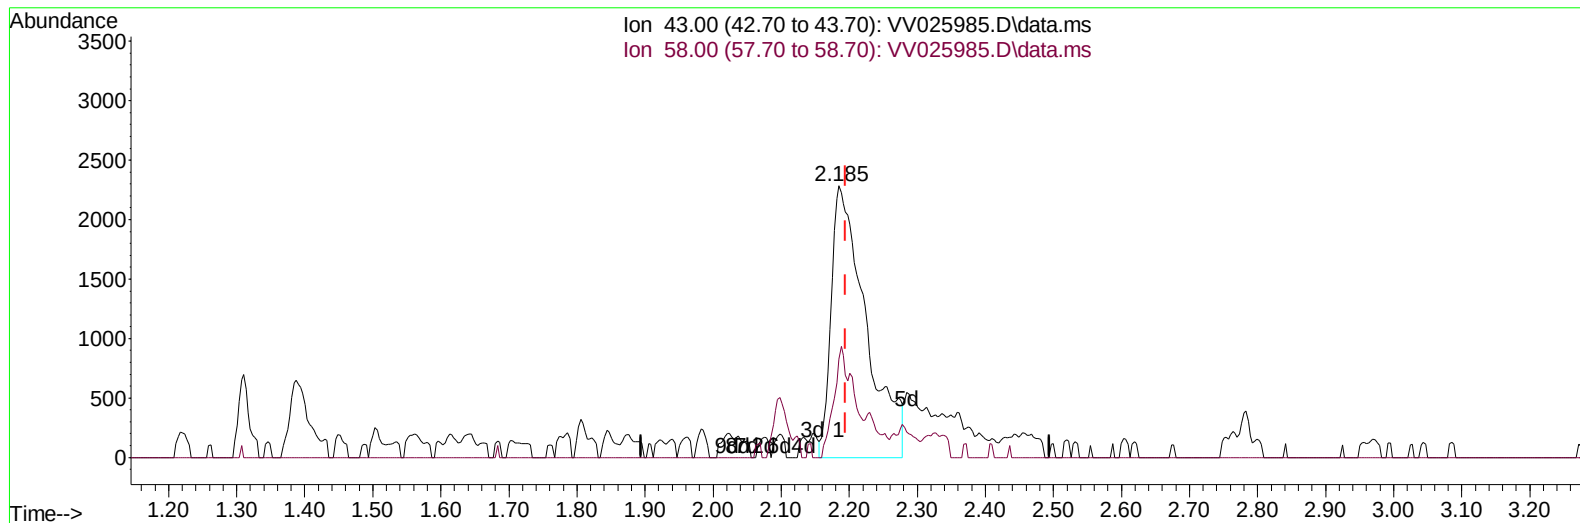

TIC: VV025985.D\data.ms

(13) Acetone (T)

2.185min (-0.010) 6.51 ug/L m

response 8045

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.50	15.14
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060222\
 Data File : VV025985.D
 Acq On : 02 Jun 2022 15:36
 Operator : SY/MD
 Sample : N3171-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBTZ3

Manual IntegrationsAPPROVED

Quant Time: Jun 03 00:08:00 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jun 03 00:06:32 2022
 Response via : Initial Calibration

Reviewed By : John Carlone 06/06/2022
 Supervised By : Mahesh Dadoda 06/06/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.616	114		327218	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117		332014	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152		154570	50.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.310	65		147664	34.966	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135		Recovery	=	69.940%	
7) Chloroethane-d5	1.571	69		130365	35.152	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130		Recovery	=	70.300%	
11) 1,1-Dichloroethene-d2	2.108	63		219162	29.673	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125		Recovery	=	59.340%#	
21) 2-Butanone-d5	3.902	46		128378	70.925	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130		Recovery	=	70.930%	
24) Chloroform-d	4.349	84		250449	42.460	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125		Recovery	=	84.920%	
26) 1,2-Dichloroethane-d4	5.030	65		151792	42.580	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125		Recovery	=	85.160%	
32) Benzene-d6	5.050	84		498228	43.045	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125		Recovery	=	86.100%	
36) 1,2-Dichloropropane-d6	6.069	67		159120	44.760	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120		Recovery	=	89.520%	
41) Toluene-d8	7.317	98		427310	40.069	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120		Recovery	=	80.140%	
43) trans-1,3-Dichloroprop...	7.622	79		62627	39.465	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125		Recovery	=	78.920%	
47) 2-Hexanone-d5	8.091	63		107194	82.245	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130		Recovery	=	82.250%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84		209834	44.261	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120		Recovery	=	88.520%	
66) 1,2-Dichlorobenzene-d4	11.622	152		176313	52.000	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120		Recovery	=	104.000%	
Target Compounds							
13) Acetone	2.185	43		8045m	6.513	ug/L	
52) Ethylbenzene	9.014	91		22558	1.823	ug/L	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060222\
Data File : VV025985.D
Acq On : 02 Jun 2022 15:36
Operator : SY/MD
Sample : N3171-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBTZ3

Manual IntegrationsAPPROVED

Quant Time: Jun 03 00:08:00 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jun 03 00:06:32 2022
Response via : Initial Calibration

Reviewed By :John Carlone 06/06/2022
Supervised By :Mahesh Dadoda 06/06/2022

