




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060222\
Data File : VV025986.D
Acq On : 02 Jun 2022 16:00
Operator : SY/MD
Sample : N3171-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBTZ4

Manual IntegrationsAPPROVED

Quant Time: Jun 03 00:08:12 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jun 03 00:06:32 2022
Response via : Initial Calibration

Reviewed By :John Carlone 06/06/2022
Supervised By :Mahesh Dadoda 06/06/2022

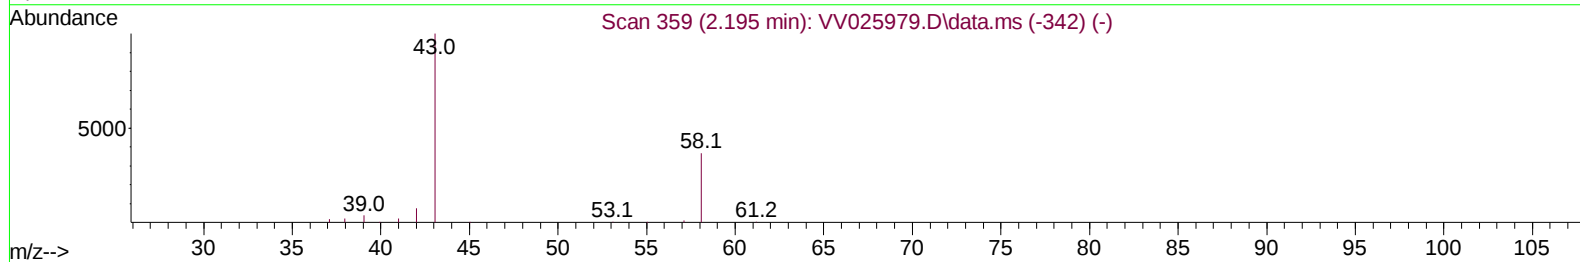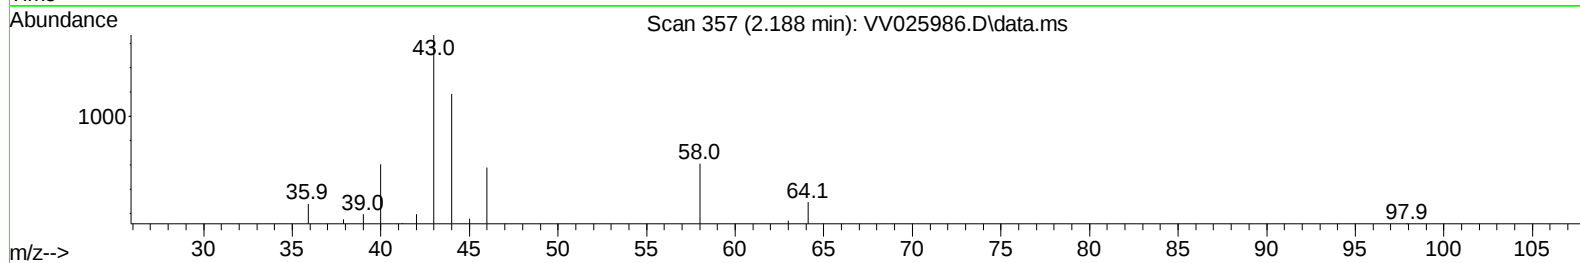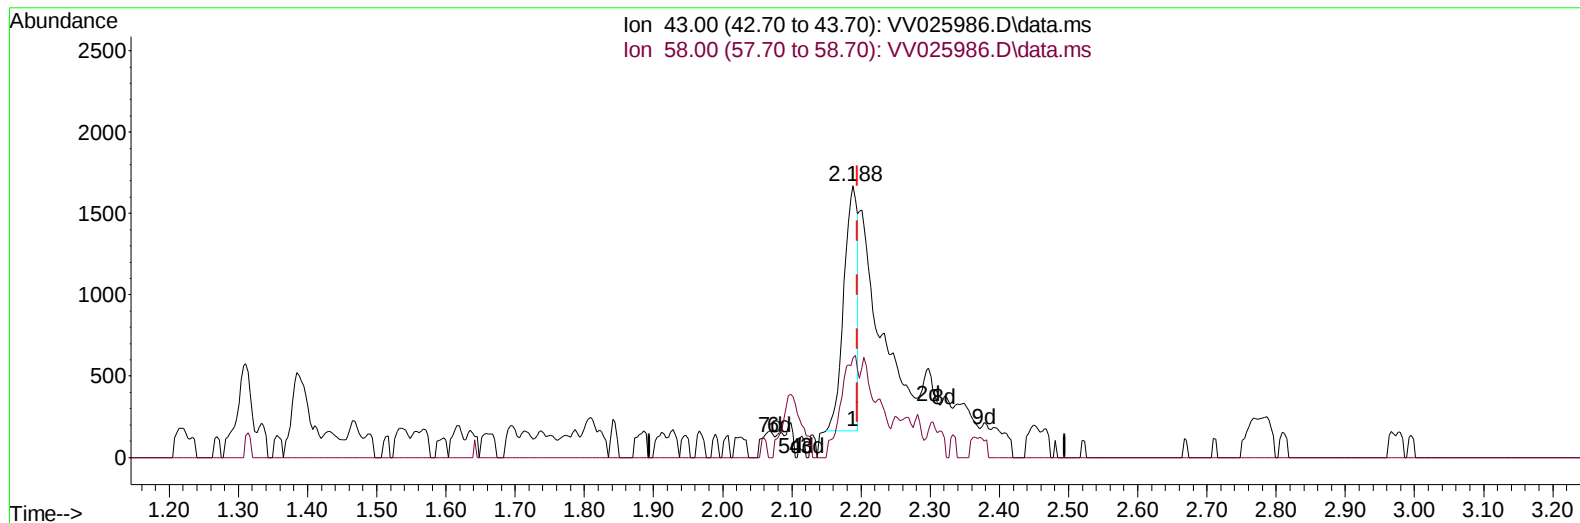

TIC: VV025986.D\data.ms

(13) Acetone (T)

2.188min (-0.006) 1.72 ug/L

response 2049

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.50	22.25
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060222\
 Data File : VV025986.D
 Acq On : 02 Jun 2022 16:00
 Operator : SY/MD
 Sample : N3171-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBTZ4

Manual IntegrationsAPPROVED

Quant Time: Jun 03 00:08:12 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jun 03 00:06:32 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 06/06/2022
 Supervised By :Mahesh Dadoda 06/06/2022

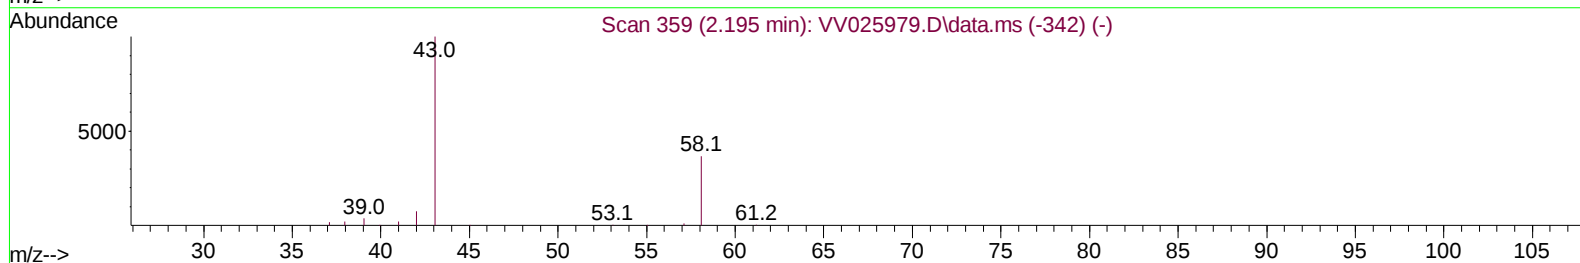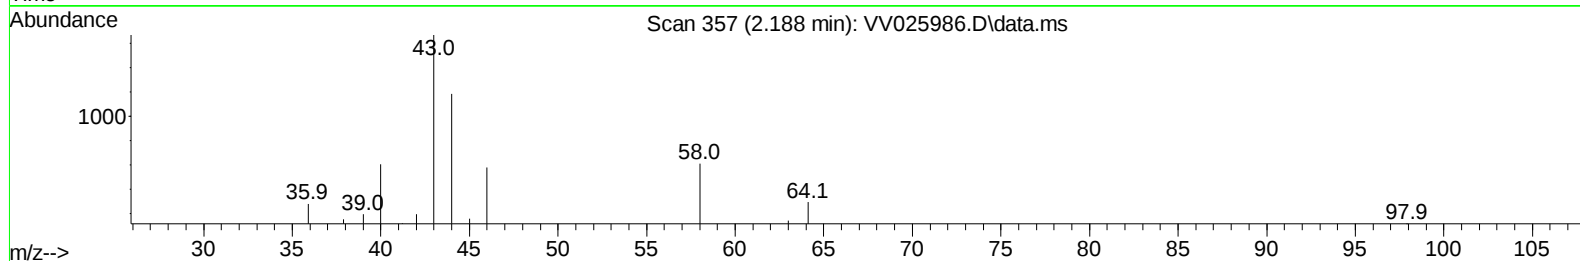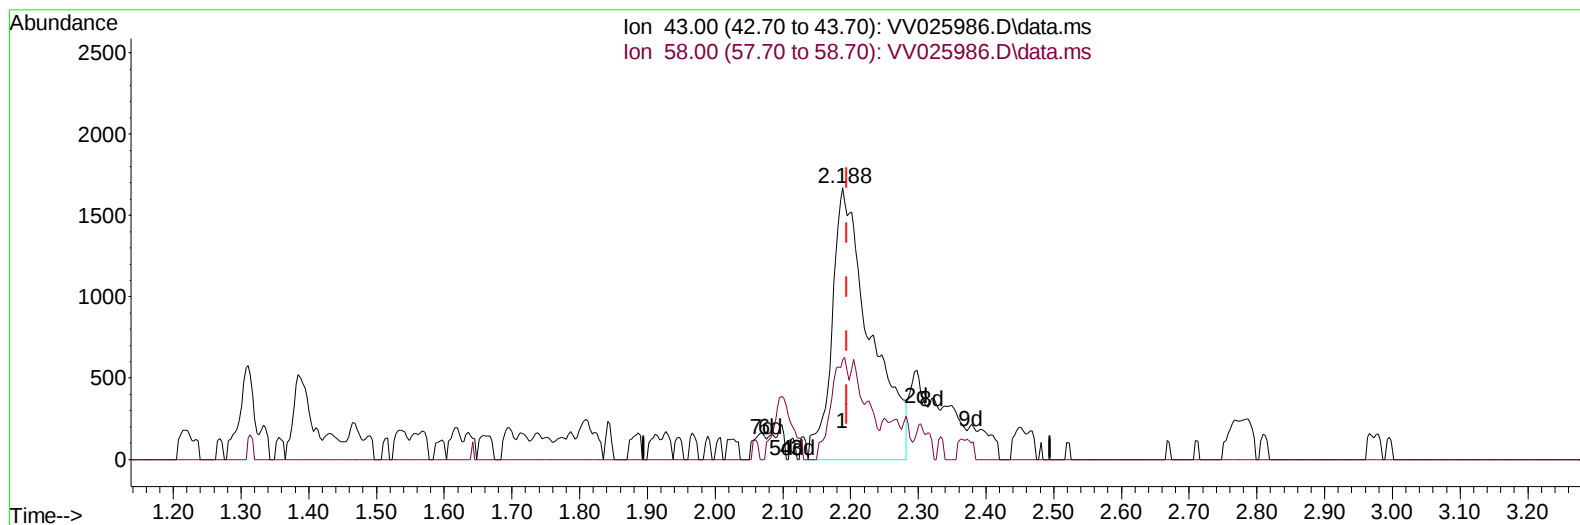

TIC: VV025986.D\data.ms

(13) Acetone (T)

2.188min (-0.006) 5.47 ug/L m

response 6510

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.50	7.00
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060222\
 Data File : VV025986.D
 Acq On : 02 Jun 2022 16:00
 Operator : SY/MD
 Sample : N3171-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBTZ4

Manual IntegrationsAPPROVED

Quant Time: Jun 03 00:08:12 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jun 03 00:06:32 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 06/06/2022
 Supervised By :Mahesh Dadoda 06/06/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	315523	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	317067	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	148459	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	145669	35.772	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	71.540%	
7) Chloroethane-d5	1.571	69	127091	35.539	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	71.080%	
11) 1,1-Dichloroethene-d2	2.108	63	212616	29.853	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	59.700%#	
21) 2-Butanone-d5	3.902	46	125609	71.967	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	71.970%	
24) Chloroform-d	4.352	84	246647	43.365	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	86.740%	
26) 1,2-Dichloroethane-d4	5.034	65	146191	42.529	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	85.060%	
32) Benzene-d6	5.050	84	491459	44.462	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	88.920%	
36) 1,2-Dichloropropane-d6	6.069	67	158574	46.709	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	93.420%	
41) Toluene-d8	7.317	98	418278	41.071	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	82.140%	
43) trans-1,3-Dichloroprop...	7.622	79	59541	39.289	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	78.580%	
47) 2-Hexanone-d5	8.092	63	106491	85.558	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	85.560%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	205683	45.431	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	90.860%	
66) 1,2-Dichlorobenzene-d4	11.622	152	172397	52.938	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	105.880%	
Target Compounds						
					Qvalue	
13) Acetone	2.188	43	6510m	5.466	ug/L	
33) Benzene	5.108	78	7651	0.717	ug/L	100
52) Ethylbenzene	9.018	91	24079	2.038	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060222\
Data File : VV025986.D
Acq On : 02 Jun 2022 16:00
Operator : SY/MD
Sample : N3171-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBTZ4

Manual IntegrationsAPPROVED

Quant Time: Jun 03 00:08:12 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jun 03 00:06:32 2022
Response via : Initial Calibration

Reviewed By :John Carlone 06/06/2022
Supervised By :Mahesh Dadoda 06/06/2022

