




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060222\
Data File : VV025987.D
Acq On : 02 Jun 2022 16:22
Operator : SY/MD
Sample : N3171-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBTZ6

Manual IntegrationsAPPROVED

Quant Time: Jun 03 00:08:27 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jun 03 00:06:32 2022
Response via : Initial Calibration

Reviewed By :John Carlone 06/06/2022
Supervised By :Mahesh Dadoda 06/06/2022

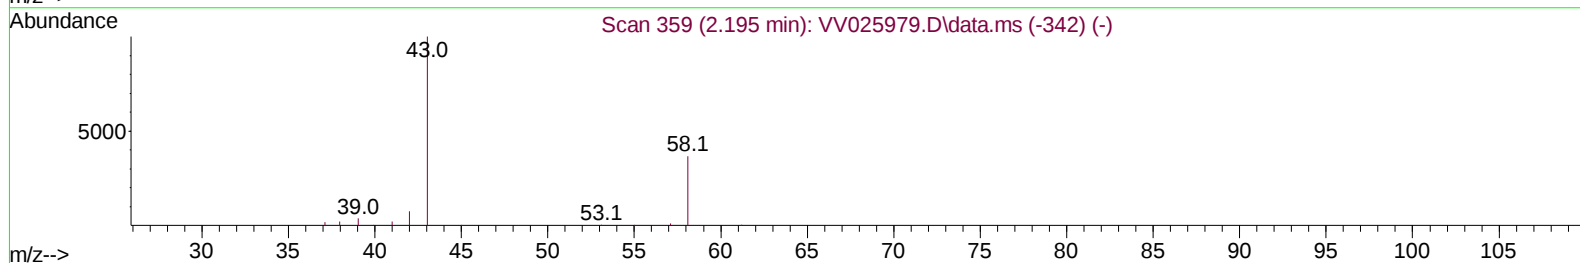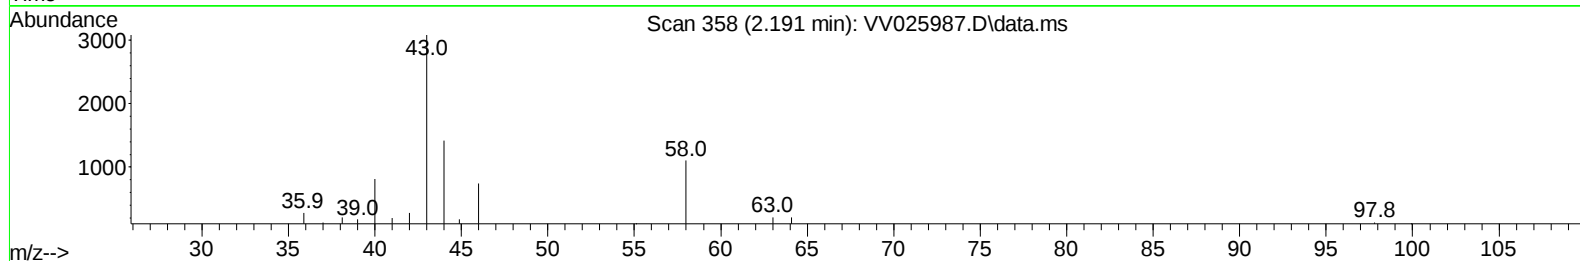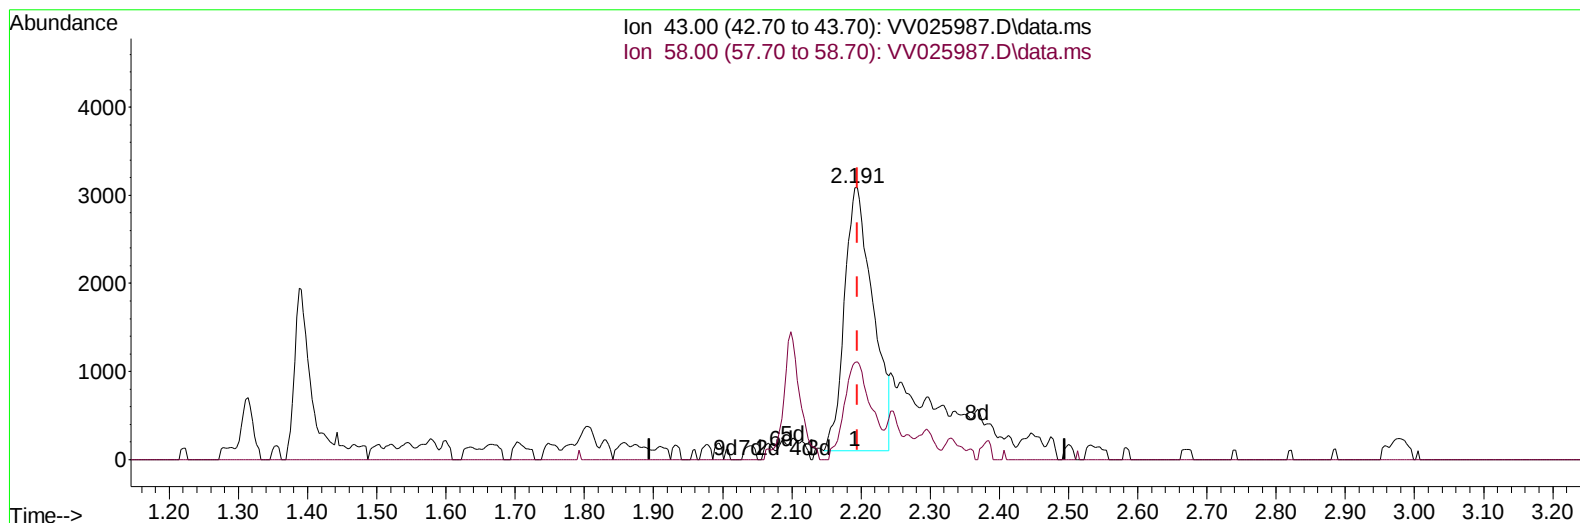

TIC: VV025987.D\data.ms

(13) Acetone (T)

2.191min (-0.003) 7.17 ug/L

response 8558

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.50	35.00
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060222\
 Data File : VV025987.D
 Acq On : 02 Jun 2022 16:22
 Operator : SY/MD
 Sample : N3171-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBTZ6

Manual IntegrationsAPPROVED

Quant Time: Jun 03 00:08:27 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jun 03 00:06:32 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 06/06/2022
 Supervised By :Mahesh Dadoda 06/06/2022

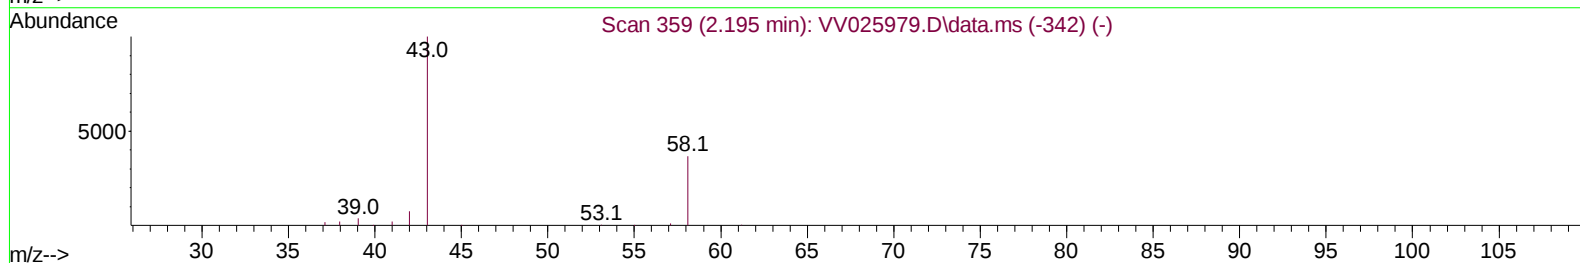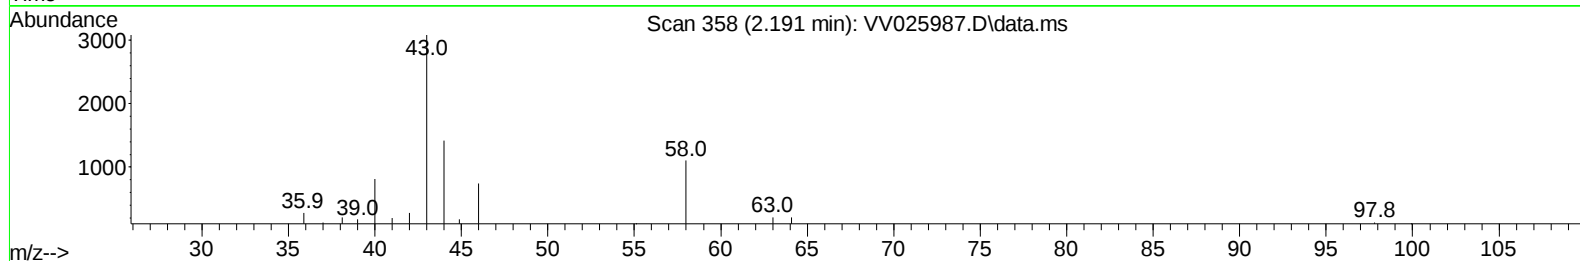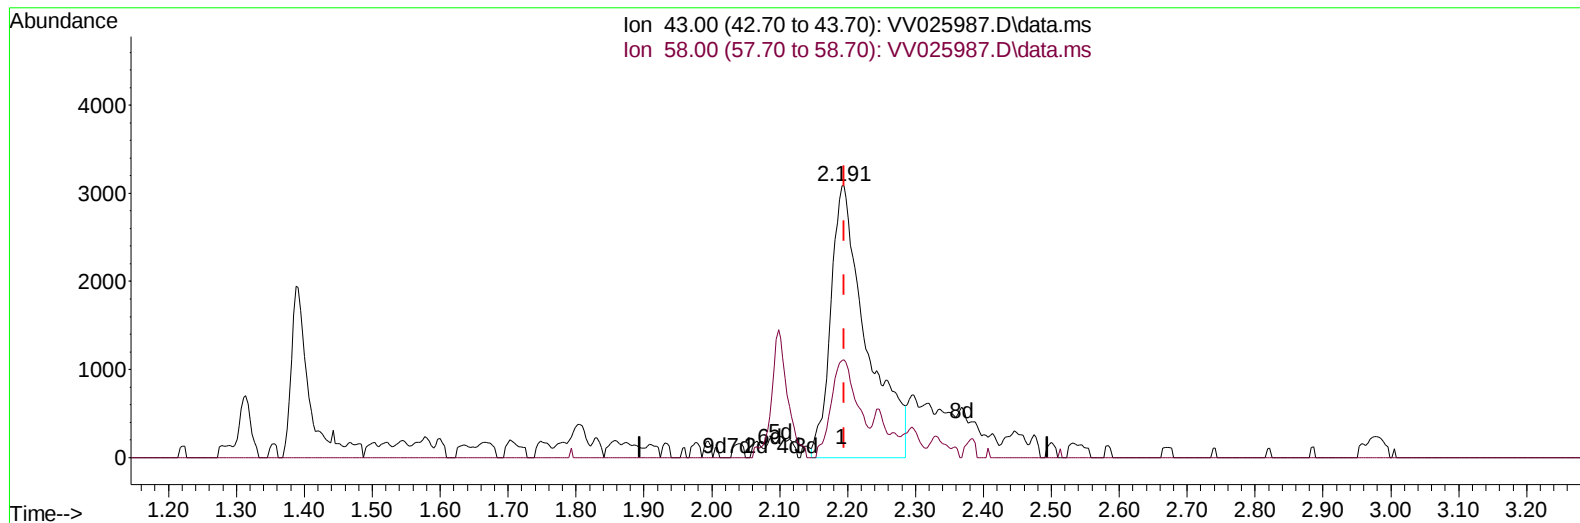

TIC: VV025987.D\data.ms

(13) Acetone (T)

2.191min (-0.003) 9.40 ug/L m

response 11219

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.50	26.70
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060222\
 Data File : VV025987.D
 Acq On : 02 Jun 2022 16:22
 Operator : SY/MD
 Sample : N3171-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBTZ6

Manual IntegrationsAPPROVED

Quant Time: Jun 03 00:43:43 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jun 03 00:06:32 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 06/06/2022
 Supervised By :Mahesh Dadoda 06/06/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.619	114		316099	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117		313570	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152		142744	50.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.310	65		152706	37.432	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135		Recovery	=	74.860%	
7) Chloroethane-d5	1.571	69		130941	36.549	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130		Recovery	=	73.100%	
11) 1,1-Dichloroethene-d2	2.111	63		221344	31.022	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125		Recovery	=	62.040%	
21) 2-Butanone-d5	3.902	46		137587	78.687	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130		Recovery	=	78.690%	
24) Chloroform-d	4.352	84		254680	44.696	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125		Recovery	=	89.400%	
26) 1,2-Dichloroethane-d4	5.037	65		157021	45.596	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125		Recovery	=	91.200%	
32) Benzene-d6	5.053	84		511809	46.819	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125		Recovery	=	93.640%	
36) 1,2-Dichloropropane-d6	6.072	67		163551	48.712	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120		Recovery	=	97.420%	
41) Toluene-d8	7.317	98		444171	44.100	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120		Recovery	=	88.200%	
43) trans-1,3-Dichloroprop...	7.622	79		65020	43.382	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125		Recovery	=	86.760%	
47) 2-Hexanone-d5	8.092	63		118297	96.103	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130		Recovery	=	96.100%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84		219248	48.967	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120		Recovery	=	97.940%	
66) 1,2-Dichlorobenzene-d4	11.622	152		163621	52.255	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120		Recovery	=	104.520%	
Target Compounds							
13) Acetone	2.191	43		11219m	9.402	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060222\
Data File : VV025987.D
Acq On : 02 Jun 2022 16:22
Operator : SY/MD
Sample : N3171-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 3

Instrument :
MSVOA_V
ClientSampleId :
DBTZ6

Manual IntegrationsAPPROVED

Quant Time: Jun 03 00:43:43 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jun 03 00:06:32 2022
Response via : Initial Calibration

Reviewed By :John Carlone 06/06/2022
Supervised By :Mahesh Dadoda 06/06/2022

