

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060222\
 Data File : VV025982.D
 Acq On : 02 Jun 2022 14:21
 Operator : SY/MD
 Sample : N3173-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXEK5

Manual Integrations
 APPROVED

Reviewed By : John Carlone 06/06/2022
 Supervised By : Mahesh Dadoda 06/06/2022

Quant Time: Jun 03 00:07:21 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jun 03 00:06:32 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	315554	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	314508	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	140418	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	148018	36.346	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	72.700%		
7) Chloroethane-d5	1.571	69	128157	35.834	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	71.660%		
11) 1,1-Dichloroethene-d2	2.108	63	216663	30.419	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	60.840%		
21) 2-Butanone-d5	3.896	46	120369	68.958	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	68.960%		
24) Chloroform-d	4.349	84	249137	43.799	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	87.600%		
26) 1,2-Dichloroethane-d4	5.031	65	147594	42.933	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	85.860%		
32) Benzene-d6	5.050	84	498107	45.430	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	90.860%		
36) 1,2-Dichloropropane-d6	6.069	67	158414	47.042	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	94.080%		
41) Toluene-d8	7.317	98	428011	42.369	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	84.740%		
43) trans-1,3-Dichloroprop...	7.622	79	62214	41.386	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	82.780%		
47) 2-Hexanone-d5	8.088	63	106997	86.664	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	86.660%		
56) 1,1,2,2-Tetrachloroeth...	10.214	84	206436	45.968	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	91.940%		
66) 1,2-Dichlorobenzene-d4	11.622	152	157111	51.007	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	102.020%		
Target Compounds					Qvalue	
13) Acetone	2.188	43	12118m	10.173	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060222\
Data File : VV025982.D
Acq On : 02 Jun 2022 14:21
Operator : SY/MD
Sample : N3173-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
EXEK5

Manual Integrations
APPROVED

Reviewed By : John Carlone 06/06/2022
Supervised By : Mahesh Dadoda 06/06/2022


Quant Time: Jun 03 00:07:21 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jun 03 00:06:32 2022
Response via : Initial Calibration

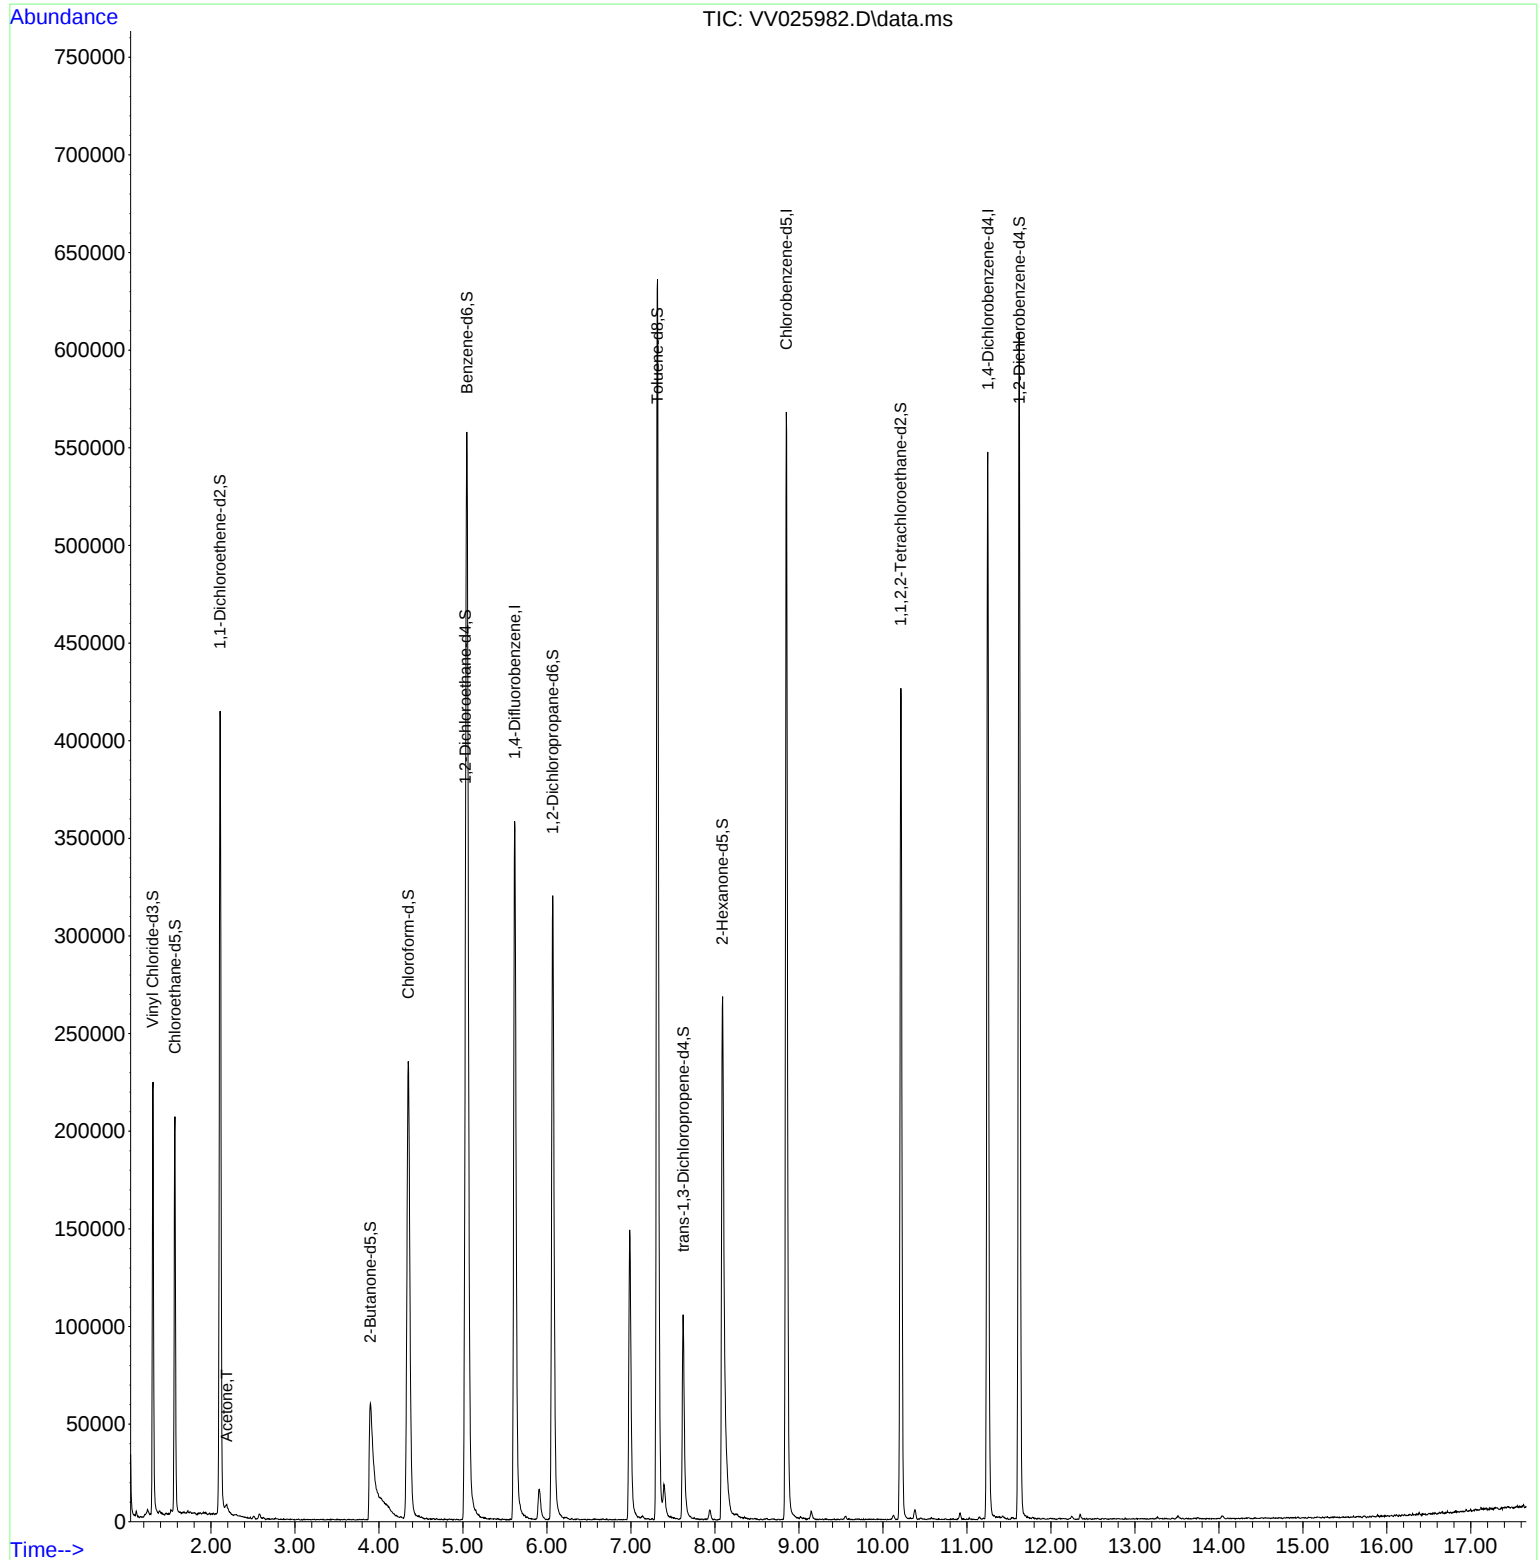

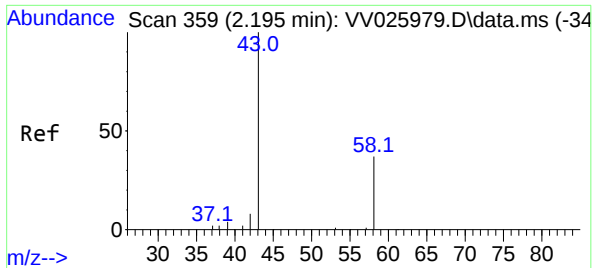

#13
 Acetone
 Concen: 10.173 ug/L m
 RT: 2.188 min Scan# 3
 Delta R.T. -0.006 min
 Lab File: VV025982.D
 Acq: 02 Jun 2022 14:21

Instrument :
 MSVOA_V
 ClientSampleId :
 EXEK5

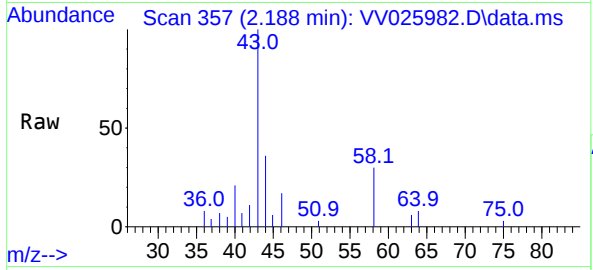

Tgt Ion: 43 Resp: 12118

Ion	Ratio	Lower	Upper
43	100		
58	14.3	0.0	65.0

Manual Integrations
 APPROVED

Reviewed By :John Carlone 06/06/2022
 Supervised By :Mahesh Dadoda 06/06/2022

