

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060222\
 Data File : VV025980.D
 Acq On : 02 Jun 2022 13:28
 Operator : SY/MD
 Sample : VV0602WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK218

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M

Title : VOC Analysis

Signal : TIC: VV025980.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	99	rVB	229501	240568	16.16%	2.277%
2	1.568	157	164	179	rVB	212727	238856	16.05%	2.261%
3	2.108	322	332	352	rVB	429647	613706	41.23%	5.810%
4	2.503	449	455	457	rBV3	3921	3775	0.25%	0.036%
5	2.709	514	519	523	rBV3	652	547	0.04%	0.005%
6	2.744	523	530	531	rBV4	425	444	0.03%	0.004%
7	2.828	553	556	557	rBV	228	149	0.01%	0.001%
8	2.870	567	569	573	rBV	323	210	0.01%	0.002%
9	3.008	609	612	616	rBV2	263	254	0.02%	0.002%
10	3.111	641	644	646	rBV2	343	205	0.01%	0.002%
11	3.124	646	648	650	rBV	361	178	0.01%	0.002%
12	3.169	660	662	664	rVB	339	140	0.01%	0.001%
13	3.211	667	675	677	rBV4	382	385	0.03%	0.004%
14	3.439	740	746	747	rBV2	255	221	0.01%	0.002%
15	3.449	747	749	753	rVV	177	145	0.01%	0.001%
16	3.545	776	779	783	rBV2	290	191	0.01%	0.002%
17	3.596	791	795	798	rVB	330	249	0.02%	0.002%
18	3.677	817	820	823	rVB	322	180	0.01%	0.002%
19	3.693	823	825	828	rBV2	271	162	0.01%	0.002%
20	3.725	832	835	838	rVB2	289	180	0.01%	0.002%
21	3.854	871	875	879	rBV2	218	219	0.01%	0.002%
22	3.902	879	890	910	rBV	55942	196016	13.17%	1.856%
23	4.346	1013	1028	1054	rBV	239934	593058	39.84%	5.614%
24	4.580	1097	1101	1102	rBV4	446	303	0.02%	0.003%
25	4.683	1131	1133	1137	rVB2	339	205	0.01%	0.002%
26	4.757	1153	1156	1158	rBV2	413	204	0.01%	0.002%
27	4.789	1164	1166	1171	rVB2	505	273	0.02%	0.003%
28	4.818	1171	1175	1176	rBV2	222	149	0.01%	0.001%
29	4.860	1182	1188	1190	rBV	401	301	0.02%	0.003%
30	4.879	1191	1194	1197	rBV2	411	254	0.02%	0.002%
31	4.924	1205	1208	1210	rBV3	382	214	0.01%	0.002%
32	5.043	1229	1245	1287	rBV2	580125	1488515	100.00%	14.092%
33	5.323	1329	1332	1334	rBV	300	160	0.01%	0.002%
34	5.410	1356	1359	1360	rBV2	285	159	0.01%	0.002%
35	5.500	1384	1387	1390	rBV3	408	261	0.02%	0.002%
36	5.564	1404	1407	1411	rBV3	465	341	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060222\
 Data File : VV025980.D
 Acq On : 02 Jun 2022 13:28
 Operator : SY/MD
 Sample : VV0602WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK218

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Title : VOC Analysis

37	5.616	1411	1423	1453	rBV	347539	717519	48.20%	6.793%
38	5.802	1479	1481	1485	rVB3	760	354	0.02%	0.003%
39	5.908	1503	1514	1528	rBV3	13966	29901	2.01%	0.283%
40	6.066	1550	1563	1604	rBV	328843	680191	45.70%	6.439%
41	6.288	1630	1632	1640	rVB3	667	590	0.04%	0.006%
42	6.326	1640	1644	1647	rVB2	301	240	0.02%	0.002%
43	6.349	1647	1651	1652	rBV2	314	220	0.01%	0.002%
44	6.358	1652	1654	1659	rVB3	620	425	0.03%	0.004%
45	6.413	1667	1671	1673	rBV	310	239	0.02%	0.002%
46	6.513	1700	1702	1706	rBV	308	178	0.01%	0.002%
47	6.532	1706	1708	1710	rBV2	422	205	0.01%	0.002%
48	6.625	1734	1737	1742	rBV2	386	325	0.02%	0.003%
49	6.657	1743	1747	1751	rBV3	425	500	0.03%	0.005%
50	6.773	1780	1783	1787	rVB	453	324	0.02%	0.003%
51	6.802	1787	1792	1797	rVB3	464	505	0.03%	0.005%
52	6.831	1797	1801	1805	rBV2	493	364	0.02%	0.003%
53	6.911	1824	1826	1829	rBV	359	221	0.01%	0.002%
54	6.982	1838	1848	1880	rBV	158322	299598	20.13%	2.836%
55	7.313	1939	1951	1971	rBV	671084	1157890	77.79%	10.962%
56	7.619	2037	2046	2074	rBV	107971	195357	13.12%	1.849%
57	7.828	2108	2111	2112	rBV	361	205	0.01%	0.002%
58	7.918	2135	2139	2143	rBV3	422	403	0.03%	0.004%
59	7.944	2143	2147	2149	rBV	284	194	0.01%	0.002%
60	7.960	2149	2152	2154	rBV	220	164	0.01%	0.002%
61	7.985	2154	2160	2166	rVB5	726	901	0.06%	0.009%
62	8.011	2166	2168	2173	rVB2	273	133	0.01%	0.001%
63	8.088	2181	2192	2230	rBV	274662	587696	39.48%	5.564%
64	8.455	2304	2306	2309	rBV3	637	386	0.03%	0.004%
65	8.603	2350	2352	2353	rBV2	505	162	0.01%	0.002%
66	8.667	2369	2372	2376	rBV2	371	310	0.02%	0.003%
67	8.715	2385	2387	2389	rBV	384	177	0.01%	0.002%
68	8.738	2390	2394	2398	rVB3	563	371	0.02%	0.004%
69	8.770	2400	2404	2408	rBV2	600	403	0.03%	0.004%
70	8.850	2415	2429	2456	rBV	561597	918930	61.73%	8.699%
71	9.271	2557	2560	2561	rBV	335	155	0.01%	0.001%
72	9.342	2579	2582	2586	rBV2	369	267	0.02%	0.003%
73	9.416	2602	2605	2609	rBV2	175	176	0.01%	0.002%
74	9.442	2609	2613	2621	rVV3	416	583	0.04%	0.006%
75	9.545	2643	2645	2648	rBV3	540	354	0.02%	0.003%
76	9.580	2654	2656	2659	rVB3	514	295	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060222\
 Data File : VV025980.D
 Acq On : 02 Jun 2022 13:28
 Operator : SY/MD
 Sample : VV0602WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK218

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Title : VOC Analysis

77	9.596	2659	2661	2665	rBV3	821	530	0.04%	0.005%
78	9.648	2673	2677	2680	rBV	468	369	0.02%	0.003%
79	9.699	2691	2693	2698	rBV2	315	240	0.02%	0.002%
80	9.882	2745	2750	2753	rBV2	519	439	0.03%	0.004%
81	9.937	2764	2767	2772	rBV	451	333	0.02%	0.003%
82	10.030	2793	2796	2799	rBV	322	257	0.02%	0.002%
83	10.066	2804	2807	2809	rBV	256	168	0.01%	0.002%
84	10.127	2820	2826	2831	rVB4	2833	3282	0.22%	0.031%
85	10.214	2841	2853	2876	rBV	435962	687035	46.16%	6.504%
86	10.410	2911	2914	2919	rVB3	468	323	0.02%	0.003%
87	10.484	2933	2937	2940	rBV2	317	233	0.02%	0.002%
88	10.577	2961	2966	2970	rBV3	782	770	0.05%	0.007%
89	10.709	3004	3007	3011	rBV	422	220	0.01%	0.002%
90	10.731	3011	3014	3016	rBV	286	201	0.01%	0.002%
91	10.770	3023	3026	3030	rVB2	473	267	0.02%	0.003%
92	10.860	3052	3054	3063	rVB3	531	370	0.02%	0.004%
93	10.911	3064	3070	3082	rVB7	2074	3930	0.26%	0.037%
94	11.021	3103	3104	3107	rBV2	413	251	0.02%	0.002%
95	11.249	3163	3175	3196	rBV	553870	857465	57.61%	8.118%
96	11.622	3280	3291	3318	rBV	644746	1012117	68.00%	9.582%
97	12.545	3577	3578	3580	rBV	399	179	0.01%	0.002%
98	13.262	3798	3801	3812	rVB8	2149	3280	0.22%	0.031%
99	13.506	3871	3877	3887	rVB2	4665	7007	0.47%	0.066%
100	13.747	3945	3952	3962	rVB5	3295	4996	0.34%	0.047%



Sum of corrected areas: 10563050

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060222\
Data File : VV025980.D
Acq On : 02 Jun 2022 13:28
Operator : SY/MD
Sample : VV0602WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK218

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

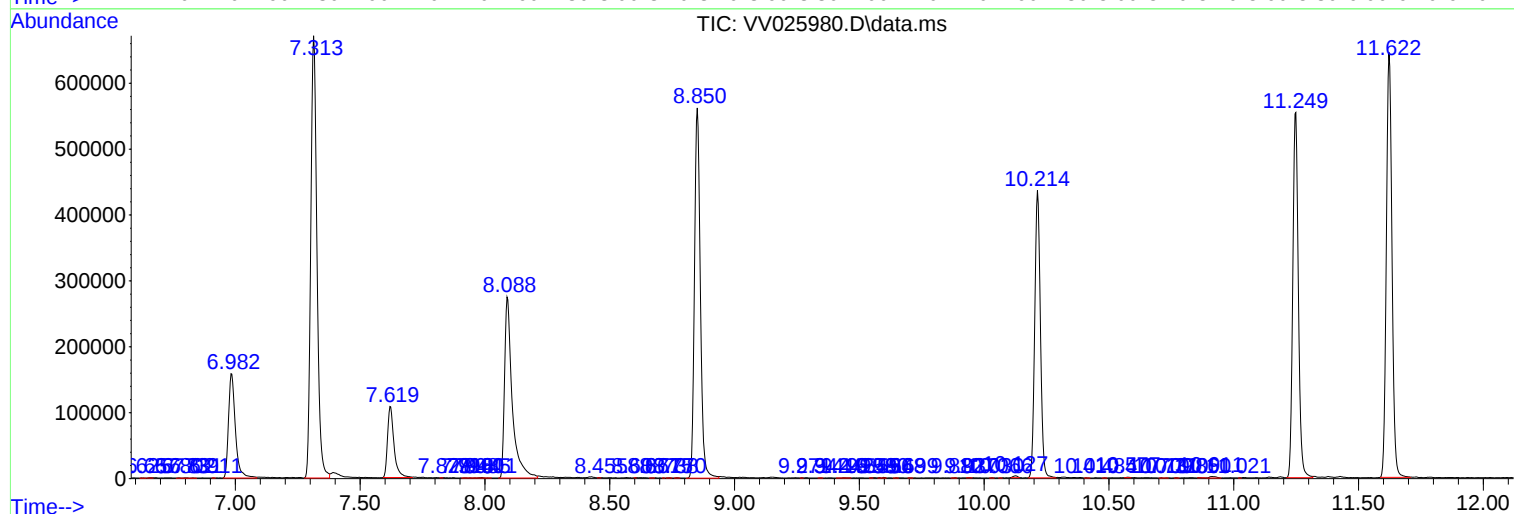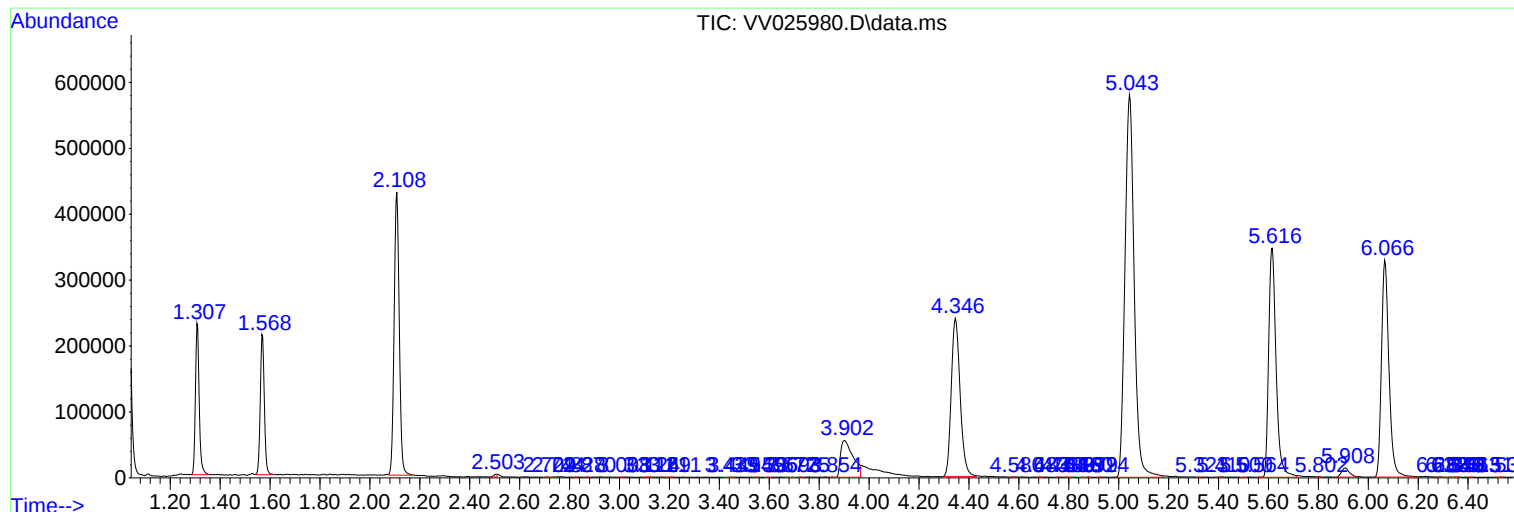

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060222\
Data File : VV025980.D
Acq On : 02 Jun 2022 13:28
Operator : SY/MD
Sample : VV0602WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK218

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060222\
Data File : VV025980.D
Acq On : 02 Jun 2022 13:28
Operator : SY/MD
Sample : VV0602WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK218

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc