

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060222\
 Data File : VV025981.D
 Acq On : 02 Jun 2022 13:57
 Operator : SY/MD
 Sample : N3173-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXEK3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Title : VOC Analysis

Signal : TIC: VV025981.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	102	rBV	259859	274547	16.74%	2.357%
2	1.568	157	164	181	rVB	237584	269490	16.43%	2.313%
3	2.108	322	332	350	rBV	477348	680678	41.51%	5.843%
4	2.754	530	533	536	rBV2	698	463	0.03%	0.004%
5	2.770	536	538	545	rVV4	734	564	0.03%	0.005%
6	2.909	578	581	585	rVB	486	322	0.02%	0.003%
7	2.931	585	588	591	rBV	446	258	0.02%	0.002%
8	2.966	596	599	600	rBV	406	164	0.01%	0.001%
9	2.989	602	606	610	rBV	404	324	0.02%	0.003%
10	3.053	624	626	629	rBV	199	98	0.01%	0.001%
11	3.092	635	638	642	rVB	365	260	0.02%	0.002%
12	3.114	642	645	649	rVB	370	293	0.02%	0.003%
13	3.137	649	652	658	rBV2	372	295	0.02%	0.003%
14	3.204	671	673	675	rBV2	194	103	0.01%	0.001%
15	3.249	685	687	692	rVB	318	157	0.01%	0.001%
16	3.275	692	695	697	rBV	334	175	0.01%	0.002%
17	3.288	697	699	702	rVB	345	174	0.01%	0.001%
18	3.307	702	705	713	rBV3	553	782	0.05%	0.007%
19	3.407	734	736	740	rVB3	344	160	0.01%	0.001%
20	3.433	740	744	746	rBV	304	244	0.01%	0.002%
21	3.474	753	757	759	rBV	283	210	0.01%	0.002%
22	3.500	763	765	769	rVV2	252	164	0.01%	0.001%
23	3.568	782	786	788	rBV3	288	232	0.01%	0.002%
24	3.603	794	797	799	rBV2	582	337	0.02%	0.003%
25	3.619	799	802	806	rVV	327	323	0.02%	0.003%
26	3.642	807	809	811	rVV	255	125	0.01%	0.001%
27	3.654	811	813	820	rVB3	346	343	0.02%	0.003%
28	3.699	826	827	830	rVB	320	101	0.01%	0.001%
29	3.725	832	835	840	rVV3	328	253	0.02%	0.002%
30	3.745	840	841	845	rVB	296	120	0.01%	0.001%
31	3.767	845	848	849	rBV	150	92	0.01%	0.001%
32	3.818	861	864	868	rBV2	224	189	0.01%	0.002%
33	3.892	878	887	916	rBV	60085	208354	12.71%	1.789%
34	4.346	1014	1028	1065	rVB	268125	659137	40.20%	5.658%
35	4.777	1158	1162	1164	rBV2	380	276	0.02%	0.002%
36	4.818	1171	1175	1178	rVB2	413	301	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060222\
 Data File : VV025981.D
 Acq On : 02 Jun 2022 13:57
 Operator : SY/MD
 Sample : N3173-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXEK3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Title : VOC Analysis

37	4.896	1197	1199	1201	rBV	280	150	0.01%	0.001%
38	4.966	1219	1221	1222	rBV2	210	80	0.00%	0.001%
39	5.043	1228	1245	1284	rBV2	639309	1639823	100.00%	14.077%
40	5.330	1330	1334	1336	rBV4	454	325	0.02%	0.003%
41	5.365	1343	1345	1347	rBV4	458	251	0.02%	0.002%
42	5.468	1374	1377	1380	rVB2	462	254	0.02%	0.002%
43	5.490	1380	1384	1386	rBV3	613	520	0.03%	0.004%
44	5.529	1394	1396	1398	rBV	396	230	0.01%	0.002%
45	5.568	1404	1408	1411	rBV2	645	605	0.04%	0.005%
46	5.616	1411	1423	1449	rBV	397294	804409	49.05%	6.905%
47	5.851	1492	1496	1498	rBV2	653	424	0.03%	0.004%
48	5.908	1502	1514	1533	rVV7	16095	37279	2.27%	0.320%
49	5.998	1539	1542	1543	rBV	302	132	0.01%	0.001%
50	6.066	1549	1563	1588	rBV	364766	745907	45.49%	6.403%
51	6.297	1632	1635	1637	rBV2	946	593	0.04%	0.005%
52	6.359	1651	1654	1657	rBV2	310	285	0.02%	0.002%
53	6.407	1667	1669	1671	rVB2	276	87	0.01%	0.001%
54	6.551	1712	1714	1715	rBV	184	86	0.01%	0.001%
55	6.600	1726	1729	1732	rBV2	350	290	0.02%	0.002%
56	6.654	1742	1746	1749	rBV3	552	533	0.03%	0.005%
57	6.732	1767	1770	1771	rBV2	250	135	0.01%	0.001%
58	6.780	1783	1785	1790	rVB2	573	322	0.02%	0.003%
59	6.828	1796	1800	1803	rBV2	611	420	0.03%	0.004%
60	6.908	1821	1825	1829	rVB2	245	209	0.01%	0.002%
61	6.928	1829	1831	1834	rBV2	261	166	0.01%	0.001%
62	6.986	1838	1849	1871	rBV	176023	326354	19.90%	2.802%
63	7.314	1938	1951	1972	rBV	749501	1297876	79.15%	11.141%
64	7.619	2036	2046	2077	rBV	119563	214964	13.11%	1.845%
65	7.838	2111	2114	2118	rBV4	497	398	0.02%	0.003%
66	7.873	2124	2125	2128	rBV2	297	151	0.01%	0.001%
67	8.088	2182	2192	2225	rBV	273581	613679	37.42%	5.268%
68	8.612	2352	2355	2356	rBV	532	279	0.02%	0.002%
69	8.706	2381	2384	2388	rBV2	613	510	0.03%	0.004%
70	8.850	2417	2429	2455	rBV	622966	1021143	62.27%	8.766%
71	9.079	2498	2500	2504	rBV2	381	191	0.01%	0.002%
72	9.098	2504	2506	2510	rBV3	606	406	0.02%	0.003%
73	9.130	2515	2516	2518	rBV	371	140	0.01%	0.001%
74	9.227	2544	2546	2549	rVB3	314	167	0.01%	0.001%
75	9.246	2550	2552	2554	rBV3	315	189	0.01%	0.002%
76	9.429	2605	2609	2612	rBV	613	548	0.03%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060222\
 Data File : VV025981.D
 Acq On : 02 Jun 2022 13:57
 Operator : SY/MD
 Sample : N3173-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXEK3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Title : VOC Analysis

77	9.497	2626	2630	2631	rBV	428	251	0.02%	0.002%
78	9.526	2637	2639	2640	rBV	232	123	0.01%	0.001%
79	9.555	2642	2648	2652	rVV4	426	473	0.03%	0.004%
80	9.648	2673	2677	2681	rBV2	434	393	0.02%	0.003%
81	9.731	2698	2703	2706	rBV	388	286	0.02%	0.002%
82	9.786	2717	2720	2721	rBV	255	140	0.01%	0.001%
83	9.841	2734	2737	2744	rVB2	615	618	0.04%	0.005%
84	9.870	2744	2746	2750	rVB2	270	141	0.01%	0.001%
85	9.895	2750	2754	2755	rBV2	321	173	0.01%	0.001%
86	10.059	2801	2805	2808	rBV	451	374	0.02%	0.003%
87	10.127	2814	2826	2834	rBV4	3803	6349	0.39%	0.055%
88	10.214	2841	2853	2876	rBV	471013	746759	45.54%	6.410%
89	10.484	2933	2937	2940	rBV2	381	313	0.02%	0.003%
90	10.789	3030	3032	3036	rVB	508	287	0.02%	0.002%
91	10.860	3052	3054	3058	rVB	685	306	0.02%	0.003%
92	11.059	3114	3116	3119	rBV	301	147	0.01%	0.001%
93	11.182	3152	3154	3156	rBV3	570	312	0.02%	0.003%
94	11.246	3163	3174	3195	rBV	618860	946198	57.70%	8.122%
95	11.622	3278	3291	3317	rBV	728625	1133092	69.10%	9.727%
96	12.053	3421	3425	3431	rBV3	588	658	0.04%	0.006%
97	12.095	3435	3438	3440	rBV3	665	528	0.03%	0.005%
98	12.304	3501	3503	3504	rBV	355	120	0.01%	0.001%
99	12.593	3590	3593	3594	rBV2	414	258	0.02%	0.002%
100	14.294	4120	4122	4125	rBV2	560	333	0.02%	0.003%


Sum of corrected areas: 11649250

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060222\
Data File : VV025981.D
Acq On : 02 Jun 2022 13:57
Operator : SY/MD
Sample : N3173-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXEK3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

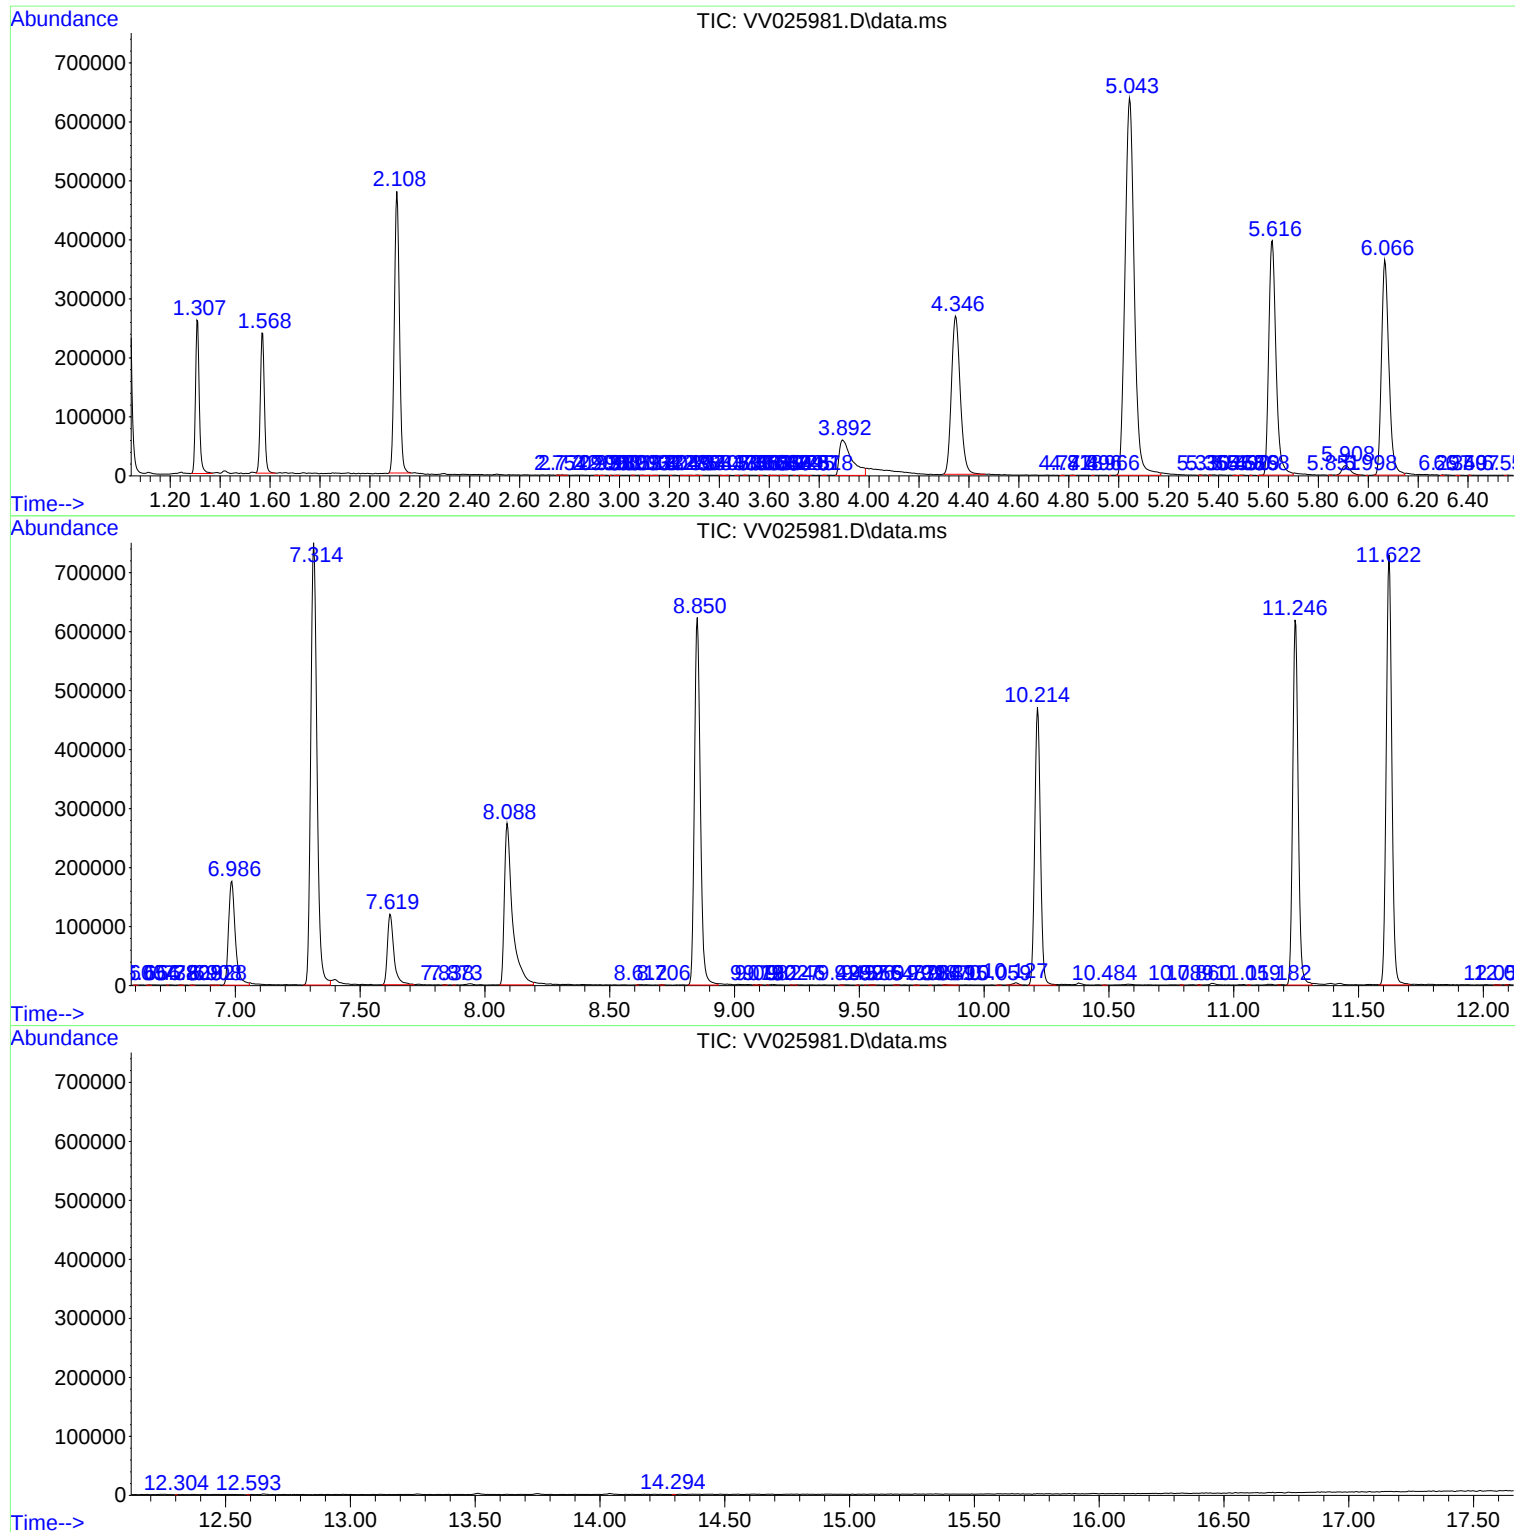

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060222\
Data File : VV025981.D
Acq On : 02 Jun 2022 13:57
Operator : SY/MD
Sample : N3173-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXEK3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060222\
Data File : VV025981.D
Acq On : 02 Jun 2022 13:57
Operator : SY/MD
Sample : N3173-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXEK3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc