

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060222\
 Data File : VV025982.D
 Acq On : 02 Jun 2022 14:21
 Operator : SY/MD
 Sample : N3173-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXEK5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Title : VOC Analysis

Signal : TIC: VV025982.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.311	76	84	104	rBV	221327	238279	16.74%	2.314%
2	1.571	157	165	181	rVB	202783	227287	15.96%	2.207%
3	2.108	323	332	349	rBV	409253	583987	41.02%	5.671%
4	2.754	531	533	534	rBV	370	132	0.01%	0.001%
5	2.857	563	565	567	rBV	271	143	0.01%	0.001%
6	2.883	570	573	575	rBV	250	148	0.01%	0.001%
7	2.995	607	608	610	rBV	202	65	0.00%	0.001%
8	3.082	633	635	638	rVB3	426	238	0.02%	0.002%
9	3.111	638	644	647	rBV3	510	551	0.04%	0.005%
10	3.259	686	690	691	rBV2	188	141	0.01%	0.001%
11	3.384	725	729	731	rBV2	362	263	0.02%	0.003%
12	3.397	731	733	734	rBV	192	65	0.00%	0.001%
13	3.426	740	742	744	rVB2	373	112	0.01%	0.001%
14	3.442	744	747	748	rBV	310	146	0.01%	0.001%
15	3.497	763	764	767	rBV2	328	155	0.01%	0.002%
16	3.510	767	768	772	rVB2	277	106	0.01%	0.001%
17	3.552	777	781	786	rBV2	310	362	0.03%	0.004%
18	3.577	786	789	790	rBV	217	102	0.01%	0.001%
19	3.626	800	804	805	rBV2	320	200	0.01%	0.002%
20	3.651	811	812	817	rVB	250	126	0.01%	0.001%
21	3.690	822	824	833	rVB2	388	384	0.03%	0.004%
22	3.815	860	863	868	rVB2	391	320	0.02%	0.003%
23	3.899	879	889	922	rBV	59623	230139	16.17%	2.235%
24	4.349	1015	1029	1058	rVB	232649	571576	40.15%	5.550%
25	4.597	1104	1106	1111	rBV4	451	359	0.03%	0.003%
26	4.651	1116	1123	1127	rBV5	487	641	0.05%	0.006%
27	4.777	1160	1162	1164	rBV	538	206	0.01%	0.002%
28	4.841	1176	1182	1185	rBV3	364	391	0.03%	0.004%
29	4.892	1195	1198	1200	rBV2	529	381	0.03%	0.004%
30	4.928	1206	1209	1213	rVB	329	203	0.01%	0.002%
31	4.982	1223	1226	1228	rBV2	287	174	0.01%	0.002%
32	5.047	1229	1246	1277	rBV2	557069	1423661	100.00%	13.824%
33	5.471	1374	1378	1381	rBV2	569	501	0.04%	0.005%
34	5.535	1394	1398	1399	rBV	298	171	0.01%	0.002%
35	5.545	1399	1401	1404	rVB2	350	142	0.01%	0.001%
36	5.561	1404	1406	1407	rBV	500	208	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW060222\
 Data File : VW025982.D
 Acq On : 02 Jun 2022 14:21
 Operator : SY/MD
 Sample : N3173-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXEK5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Title : VOC Analysis

37	5.616	1411	1423	1452	rBV	357598	727929	51.13%	7.068%
38	5.908	1505	1514	1531	rBV3	14890	31546	2.22%	0.306%
39	6.018	1545	1548	1549	rBV2	440	192	0.01%	0.002%
40	6.069	1551	1564	1590	rBV	319296	651727	45.78%	6.328%
41	6.359	1650	1654	1656	rBV4	415	369	0.03%	0.004%
42	6.410	1666	1670	1671	rBV2	275	182	0.01%	0.002%
43	6.487	1692	1694	1697	rBV2	374	251	0.02%	0.002%
44	6.551	1709	1714	1715	rBV2	489	340	0.02%	0.003%
45	6.645	1739	1743	1746	rBV2	355	293	0.02%	0.003%
46	6.661	1746	1748	1751	rBV2	432	308	0.02%	0.003%
47	6.712	1760	1764	1766	rVB3	593	419	0.03%	0.004%
48	6.751	1772	1776	1778	rBV3	369	324	0.02%	0.003%
49	6.812	1792	1795	1797	rBV	380	198	0.01%	0.002%
50	6.908	1823	1825	1826	rBV	211	90	0.01%	0.001%
51	6.986	1838	1849	1870	rBV	148527	277840	19.52%	2.698%
52	7.317	1939	1952	1969	rBV	635197	1103969	77.54%	10.720%
53	7.622	2037	2047	2072	rBV	104476	184496	12.96%	1.791%
54	7.870	2122	2124	2125	rBV	406	199	0.01%	0.002%
55	7.940	2137	2146	2158	rVB3	5037	8838	0.62%	0.086%
56	7.989	2158	2161	2163	rBV	454	320	0.02%	0.003%
57	8.050	2171	2180	2182	rBV2	474	554	0.04%	0.005%
58	8.092	2183	2193	2229	rBV	267787	605186	42.51%	5.876%
59	8.423	2294	2296	2299	rBV3	575	398	0.03%	0.004%
60	8.548	2330	2335	2340	rBV3	492	553	0.04%	0.005%
61	8.587	2343	2347	2350	rBV2	438	466	0.03%	0.005%
62	8.664	2369	2371	2372	rBV	208	75	0.01%	0.001%
63	8.751	2394	2398	2399	rBV	493	320	0.02%	0.003%
64	8.789	2406	2410	2411	rBV	297	232	0.02%	0.002%
65	8.809	2414	2416	2417	rBV	224	87	0.01%	0.001%
66	8.850	2417	2429	2463	rVV	567109	930454	65.36%	9.035%
67	9.214	2539	2542	2544	rBV2	420	270	0.02%	0.003%
68	9.384	2593	2595	2598	rBV	190	68	0.00%	0.001%
69	9.420	2601	2606	2609	rVB	425	370	0.03%	0.004%
70	9.455	2614	2617	2619	rBV2	364	173	0.01%	0.002%
71	9.558	2642	2649	2655	rVB5	1689	2477	0.17%	0.024%
72	9.590	2657	2659	2661	rBV3	423	228	0.02%	0.002%
73	9.744	2704	2707	2710	rBV3	327	213	0.01%	0.002%
74	9.770	2713	2715	2717	rVB	490	161	0.01%	0.002%
75	9.793	2720	2722	2725	rBV	312	172	0.01%	0.002%
76	9.818	2728	2730	2733	rBV	310	199	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060222\
 Data File : VV025982.D
 Acq On : 02 Jun 2022 14:21
 Operator : SY/MD
 Sample : N3173-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXEK5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Title : VOC Analysis

77	9.985	2780	2782	2787	rBV2	277	263	0.02%	0.003%
78	10.056	2801	2804	2806	rBV2	320	164	0.01%	0.002%
79	10.127	2819	2826	2835	rVB6	2168	3380	0.24%	0.033%
80	10.214	2841	2853	2877	rBV	425674	669323	47.01%	6.499%
81	10.381	2898	2905	2915	rVB3	4917	7923	0.56%	0.077%
82	10.445	2922	2925	2927	rBV2	608	463	0.03%	0.004%
83	10.577	2963	2966	2970	rBV3	805	603	0.04%	0.006%
84	10.657	2989	2991	2992	rBV	389	178	0.01%	0.002%
85	10.805	3035	3037	3040	rBV	558	316	0.02%	0.003%
86	10.889	3061	3063	3064	rBV	444	209	0.01%	0.002%
87	10.960	3084	3085	3088	rVB2	479	150	0.01%	0.001%
88	11.027	3103	3106	3110	rBV3	827	492	0.03%	0.005%
89	11.249	3163	3175	3196	rBV	546374	841265	59.09%	8.169%
90	11.532	3259	3263	3264	rBV5	844	608	0.04%	0.006%
91	11.622	3280	3291	3307	rBV	607541	954299	67.03%	9.266%
92	12.349	3512	3517	3526	rBV4	2534	3315	0.23%	0.032%
93	12.493	3559	3562	3565	rBV	385	267	0.02%	0.003%
94	12.886	3682	3684	3688	rVB2	650	342	0.02%	0.003%
95	13.850	3981	3984	3986	rBV	539	333	0.02%	0.003%


Sum of corrected areas: 10298444

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060222\
Data File : VV025982.D
Acq On : 02 Jun 2022 14:21
Operator : SY/MD
Sample : N3173-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXEK5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

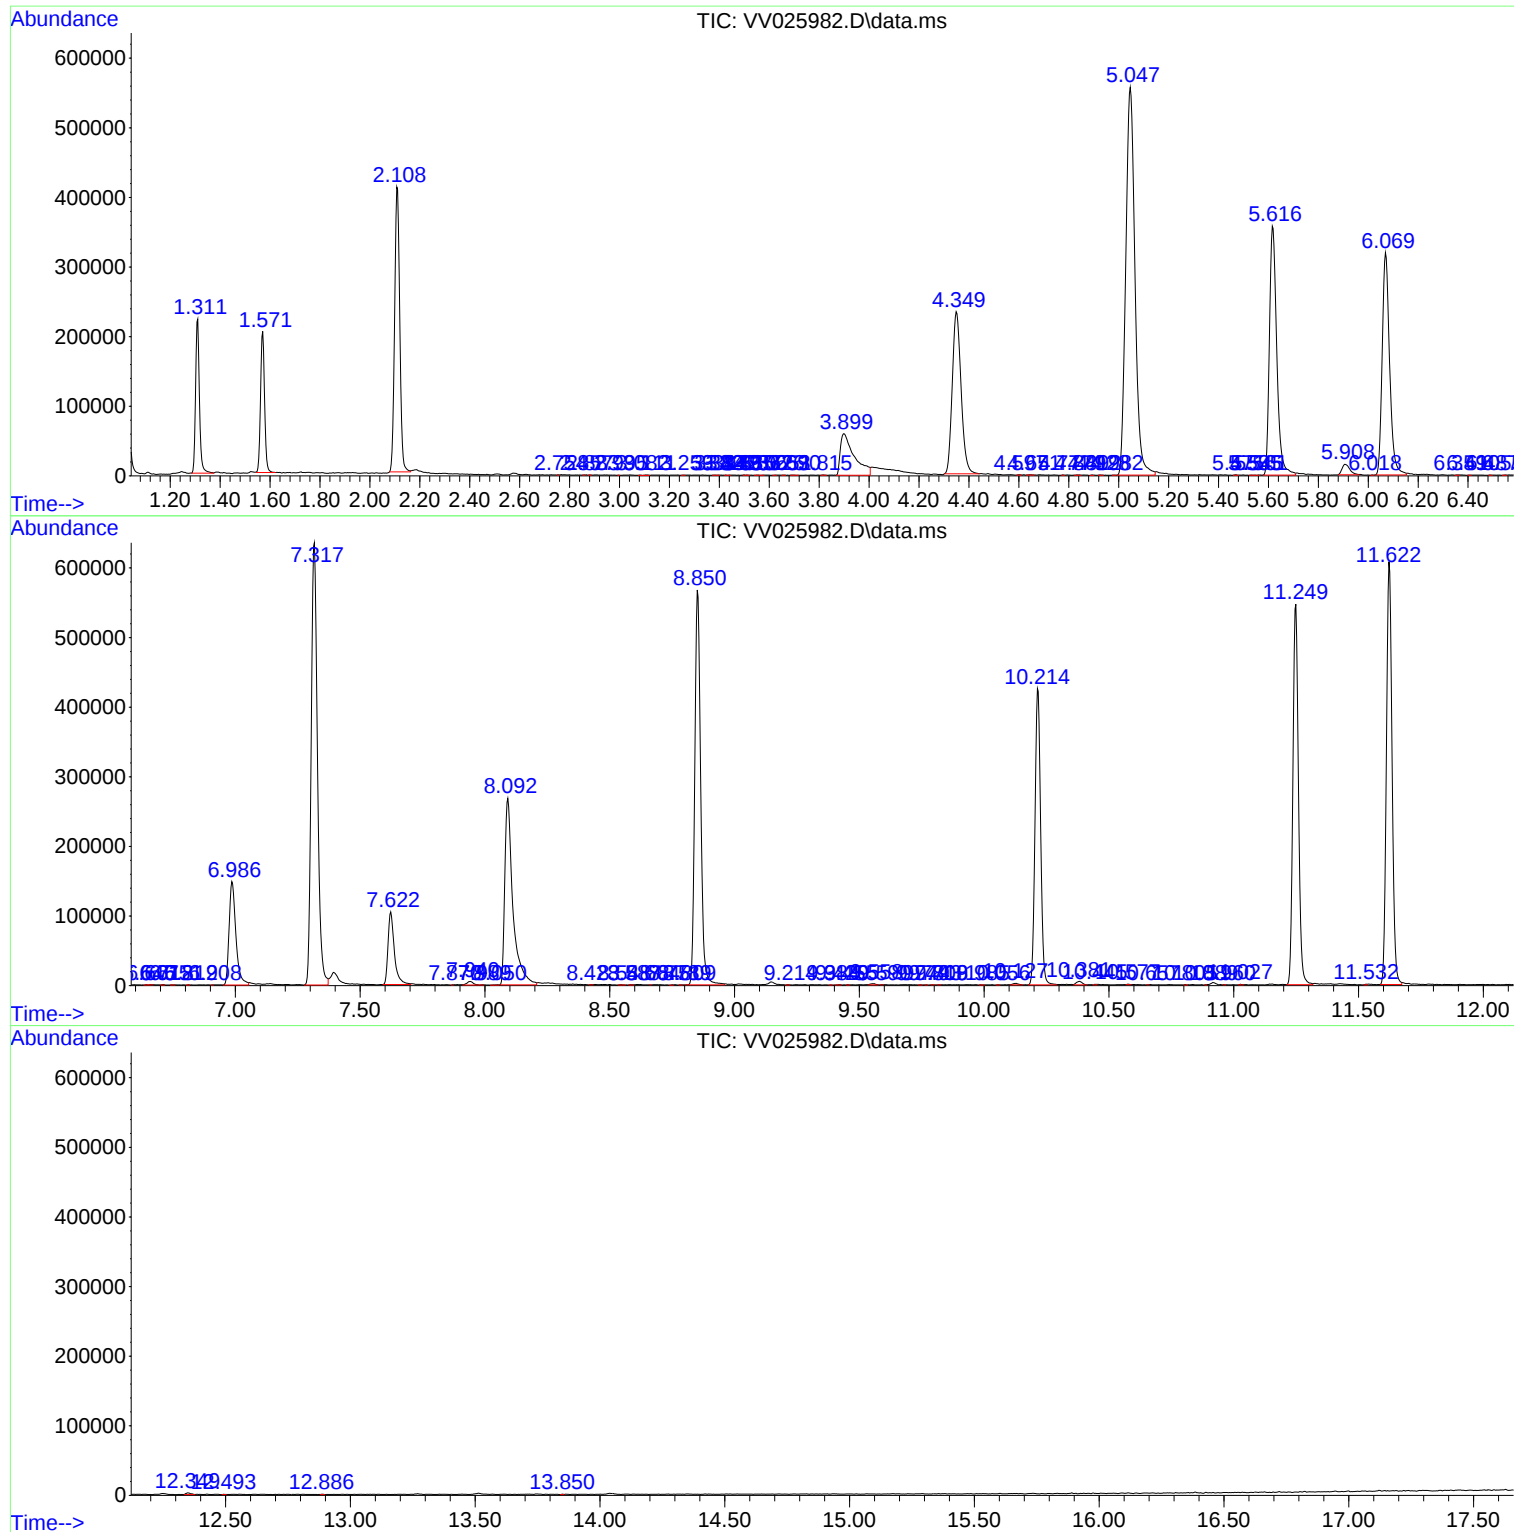

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060222\
Data File : VV025982.D
Acq On : 02 Jun 2022 14:21
Operator : SY/MD
Sample : N3173-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXEK5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060222\
Data File : VV025982.D
Acq On : 02 Jun 2022 14:21
Operator : SY/MD
Sample : N3173-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXEK5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc