

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060222\
 Data File : VV025987.D
 Acq On : 02 Jun 2022 16:22
 Operator : SY/MD
 Sample : N3171-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBTZ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Title : VOC Analysis

Signal : TIC: VV025987.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	77	84	101	rVB	228346	243960	16.47%	2.295%
2	1.571	158	165	181	rVB	204758	233399	15.76%	2.195%
3	2.111	323	333	350	rBV	422788	597557	40.34%	5.621%
4	2.603	483	486	489	rVB2	335	222	0.01%	0.002%
5	2.651	498	501	503	rBV	336	217	0.01%	0.002%
6	2.667	503	506	508	rBV2	410	308	0.02%	0.003%
7	2.716	519	521	526	rBV2	265	188	0.01%	0.002%
8	2.741	526	529	531	rBV3	491	281	0.02%	0.003%
9	2.757	532	534	535	rBV	372	156	0.01%	0.001%
10	2.822	551	554	556	rBV2	406	202	0.01%	0.002%
11	2.957	591	596	597	rBV4	537	444	0.03%	0.004%
12	3.105	639	642	646	rBV2	319	234	0.02%	0.002%
13	3.185	665	667	670	rBV2	325	139	0.01%	0.001%
14	3.288	697	699	702	rBV	336	277	0.02%	0.003%
15	3.391	728	731	734	rBV2	349	322	0.02%	0.003%
16	3.429	739	743	747	rBV2	305	331	0.02%	0.003%
17	3.696	822	826	828	rBV2	312	284	0.02%	0.003%
18	3.773	848	850	853	rVB2	440	237	0.02%	0.002%
19	3.851	871	874	876	rBV2	260	136	0.01%	0.001%
20	3.902	881	890	918	rBV	61269	221487	14.95%	2.083%
21	4.352	1016	1030	1057	rVB	240115	586221	39.57%	5.514%
22	4.760	1155	1157	1160	rVB	243	135	0.01%	0.001%
23	4.777	1160	1162	1163	rBV2	321	116	0.01%	0.001%
24	4.870	1188	1191	1195	rBV2	515	493	0.03%	0.005%
25	4.934	1209	1211	1217	rVB2	452	418	0.03%	0.004%
26	4.969	1217	1222	1227	rBV3	290	389	0.03%	0.004%
27	5.050	1227	1247	1290	rBV2	578955	1481381	100.00%	13.934%
28	5.352	1338	1341	1345	rBV5	860	586	0.04%	0.006%
29	5.375	1346	1348	1350	rBV2	472	159	0.01%	0.001%
30	5.484	1380	1382	1383	rBV2	283	131	0.01%	0.001%
31	5.619	1413	1424	1447	rBV	359985	724224	48.89%	6.812%
32	5.912	1505	1515	1533	rBV2	14811	32505	2.19%	0.306%
33	6.072	1550	1565	1595	rBV	329664	676312	45.65%	6.362%
34	6.265	1623	1625	1628	rBV3	571	412	0.03%	0.004%
35	6.336	1644	1647	1651	rVB3	499	293	0.02%	0.003%
36	6.355	1651	1653	1658	rBV4	635	482	0.03%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW060222\
 Data File : VW025987.D
 Acq On : 02 Jun 2022 16:22
 Operator : SY/MD
 Sample : N3171-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBTZ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Title : VOC Analysis

37	6.397	1664	1666	1670	rVB2	711	415	0.03%	0.004%
38	6.423	1670	1674	1678	rBV3	833	659	0.04%	0.006%
39	6.503	1696	1699	1701	rBV2	261	148	0.01%	0.001%
40	6.526	1704	1706	1709	rBV2	317	173	0.01%	0.002%
41	6.567	1717	1719	1720	rBV	269	128	0.01%	0.001%
42	6.612	1730	1733	1735	rBV	236	121	0.01%	0.001%
43	6.632	1737	1739	1741	rBV	389	201	0.01%	0.002%
44	6.703	1759	1761	1764	rBV	441	297	0.02%	0.003%
45	6.821	1795	1798	1800	rVB2	386	158	0.01%	0.001%
46	6.834	1800	1802	1806	rVB	670	362	0.02%	0.003%
47	6.857	1806	1809	1811	rBV	194	122	0.01%	0.001%
48	6.918	1825	1828	1831	rVB	322	161	0.01%	0.002%
49	6.947	1831	1837	1838	rBV2	329	325	0.02%	0.003%
50	6.989	1838	1850	1880	rBV	157165	294542	19.88%	2.771%
51	7.256	1931	1933	1936	rBV	532	365	0.02%	0.003%
52	7.317	1940	1952	1971	rBV	669768	1150576	77.67%	10.823%
53	7.577	2031	2033	2035	rBV3	260	128	0.01%	0.001%
54	7.622	2038	2047	2075	rVV	107667	192199	12.97%	1.808%
55	7.802	2101	2103	2104	rBV	487	218	0.01%	0.002%
56	7.863	2121	2122	2124	rBV	320	111	0.01%	0.001%
57	7.895	2129	2132	2134	rBV2	451	245	0.02%	0.002%
58	8.030	2171	2174	2176	rBV	261	154	0.01%	0.001%
59	8.092	2183	2193	2229	rBV	298462	647243	43.69%	6.088%
60	8.667	2368	2372	2375	rVB2	498	378	0.03%	0.004%
61	8.683	2375	2377	2378	rBV	295	130	0.01%	0.001%
62	8.744	2393	2396	2399	rBV2	516	511	0.03%	0.005%
63	8.786	2405	2409	2410	rBV	310	213	0.01%	0.002%
64	8.854	2418	2430	2454	rBV	569727	917883	61.96%	8.634%
65	9.111	2505	2510	2513	rBV5	656	712	0.05%	0.007%
66	9.143	2516	2520	2521	rBV	516	400	0.03%	0.004%
67	9.239	2546	2550	2553	rBV2	372	344	0.02%	0.003%
68	9.419	2601	2606	2610	rBV2	291	342	0.02%	0.003%
69	9.442	2612	2613	2616	rVV	323	111	0.01%	0.001%
70	9.461	2616	2619	2623	rVV2	222	154	0.01%	0.001%
71	9.526	2638	2639	2644	rBV	235	165	0.01%	0.002%
72	9.606	2663	2664	2668	rVB	305	148	0.01%	0.001%
73	9.628	2668	2671	2673	rBV3	337	230	0.02%	0.002%
74	9.709	2692	2696	2697	rBV2	245	158	0.01%	0.001%
75	9.812	2725	2728	2730	rBV2	371	217	0.01%	0.002%
76	9.834	2730	2735	2738	rBV2	776	866	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060222\
 Data File : VV025987.D
 Acq On : 02 Jun 2022 16:22
 Operator : SY/MD
 Sample : N3171-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBTZ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Title : VOC Analysis

77	9.879	2746	2749	2752	rVB2	455	308	0.02%	0.003%
78	9.950	2769	2771	2774	rVB2	304	123	0.01%	0.001%
79	9.992	2782	2784	2787	rBV2	251	112	0.01%	0.001%
80	10.017	2790	2792	2794	rVV2	258	119	0.01%	0.001%
81	10.127	2818	2826	2835	rBV5	3210	4827	0.33%	0.045%
82	10.214	2842	2853	2872	rBV	446588	704268	47.54%	6.625%
83	10.529	2948	2951	2953	rBV	412	245	0.02%	0.002%
84	10.545	2953	2956	2959	rBV2	350	263	0.02%	0.002%
85	10.574	2962	2965	2966	rBV3	982	633	0.04%	0.006%
86	10.754	3018	3021	3023	rBV2	333	170	0.01%	0.002%
87	10.780	3026	3029	3031	rVB2	264	139	0.01%	0.001%
88	10.792	3031	3033	3035	rBV2	334	171	0.01%	0.002%
89	11.249	3163	3175	3197	rBV	543609	843395	56.93%	7.933%
90	11.532	3255	3263	3270	rBV8	4435	6719	0.45%	0.063%
91	11.622	3280	3291	3309	rBV	637645	1000782	67.56%	9.414%
92	11.892	3372	3375	3377	rBV	462	288	0.02%	0.003%
93	11.927	3383	3386	3387	rBV2	491	253	0.02%	0.002%
94	11.960	3392	3396	3402	rVV2	648	638	0.04%	0.006%
95	12.217	3473	3476	3479	rBV	519	395	0.03%	0.004%
96	13.030	3726	3729	3731	rBV	345	261	0.02%	0.002%
97	13.204	3780	3783	3785	rBV	443	297	0.02%	0.003%
98	13.506	3869	3877	3892	rVB	15286	24542	1.66%	0.231%
99	14.638	4222	4229	4241	rVB2	6403	9700	0.65%	0.091%
100	14.815	4278	4284	4295	rVB	10484	15937	1.08%	0.150%




Sum of corrected areas: 10631236

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060222\
Data File : VV025987.D
Acq On : 02 Jun 2022 16:22
Operator : SY/MD
Sample : N3171-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBTZ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

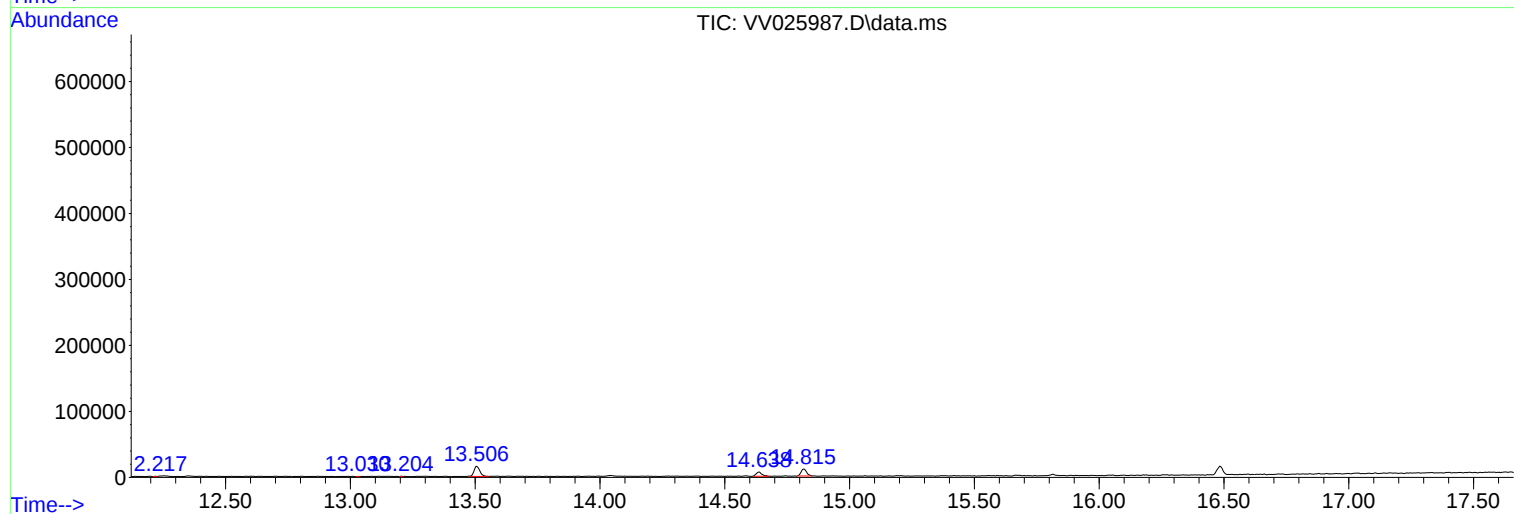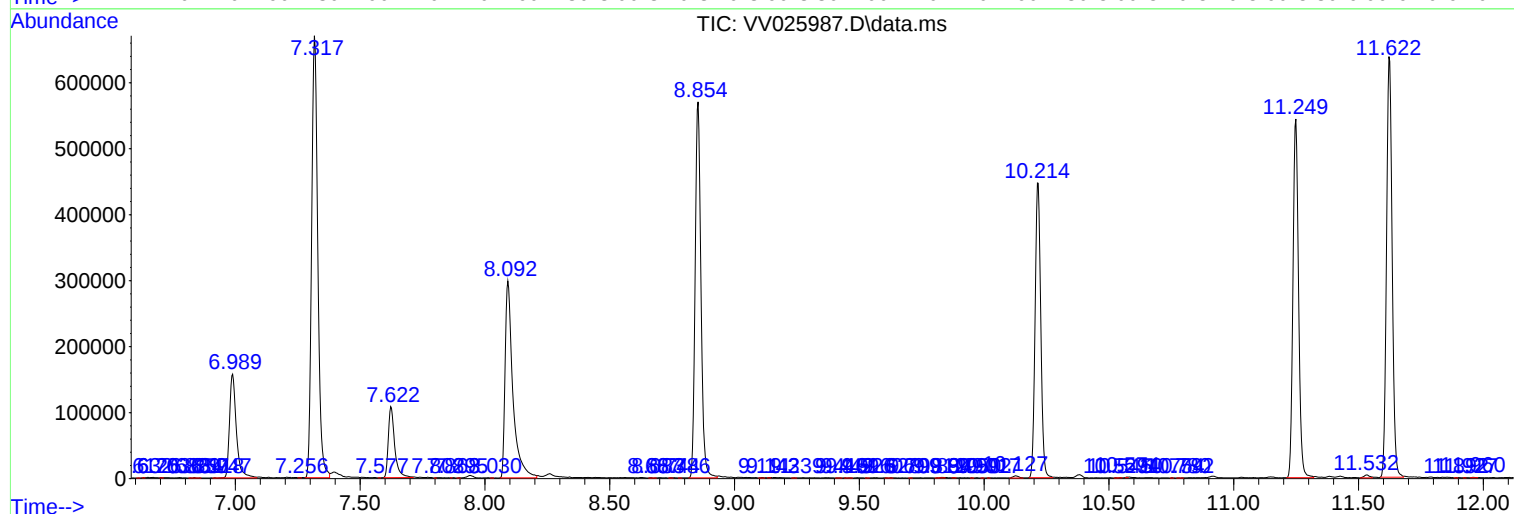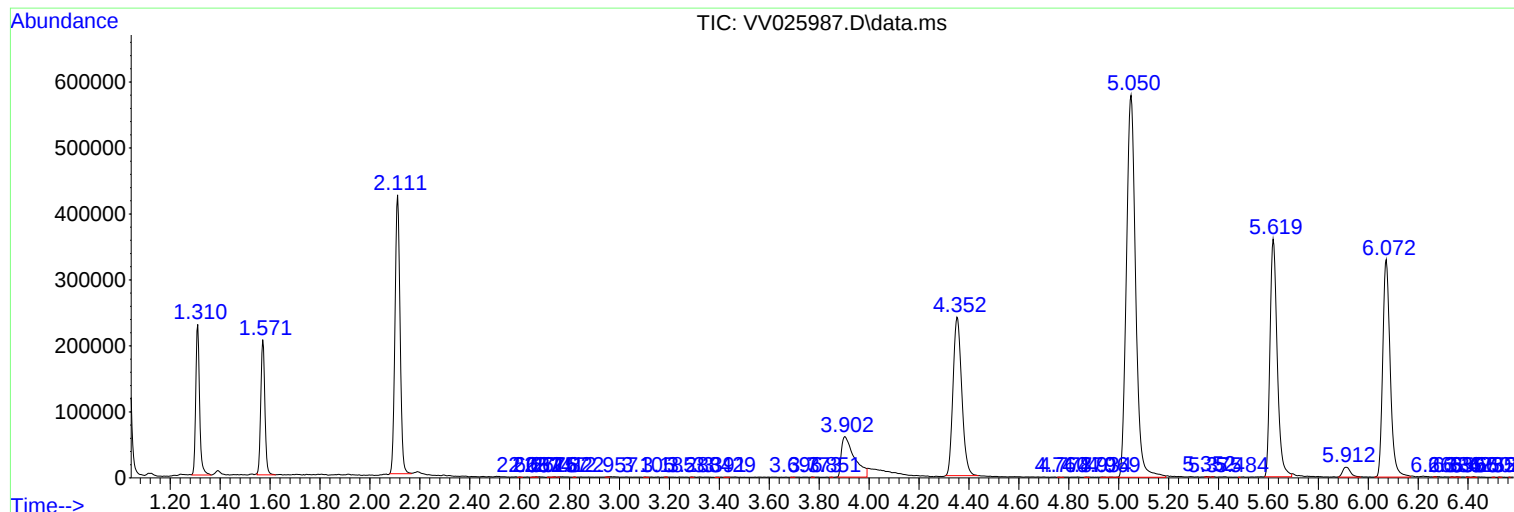

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060222\
Data File : VV025987.D
Acq On : 02 Jun 2022 16:22
Operator : SY/MD
Sample : N3171-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBTZ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060222\
Data File : VV025987.D
Acq On : 02 Jun 2022 16:22
Operator : SY/MD
Sample : N3171-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBTZ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------