


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060222\
 Data File : VV025978.D
 Acq On : 02 Jun 2022 09:07
 Operator : SY/MD
 Sample : BFB285
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB285

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Title : VOC Analysis
 Last Update : Fri Jun 03 00:06:32 2022

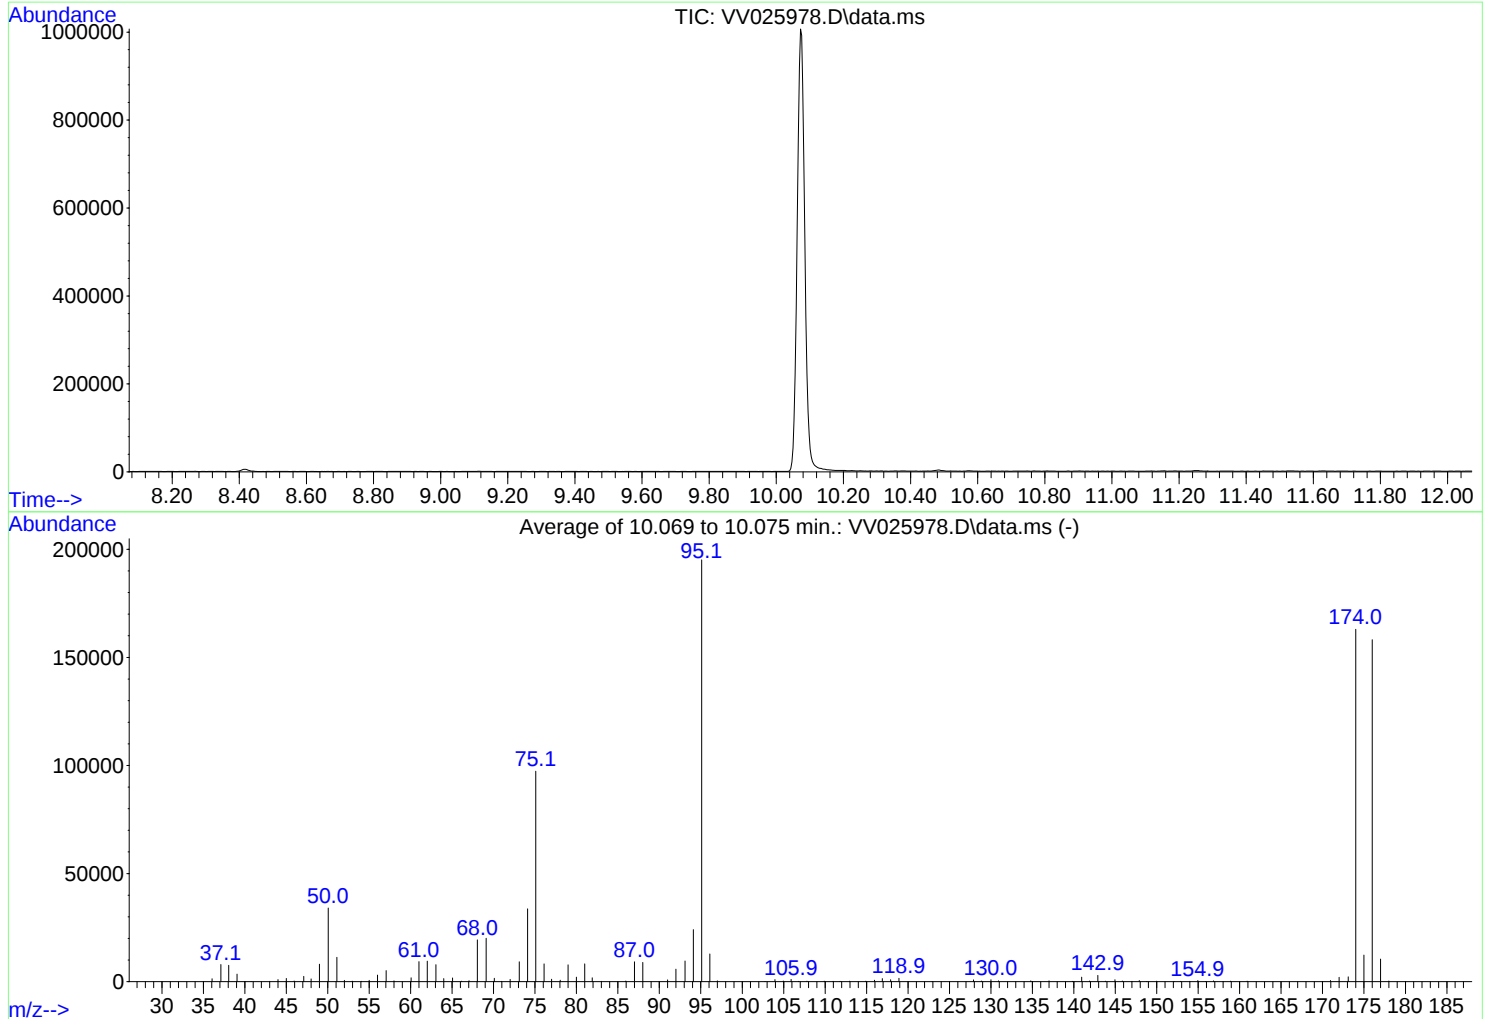

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	34083	PASS
75	95	30	80	49.9	97344	PASS
95	95	100	100	100.0	195136	PASS
96	95	5	9	6.6	12799	PASS
173	174	0.00	2	1.4	2220	PASS
174	95	50	120	83.5	163029	PASS
175	174	5	9	7.5	12279	PASS
176	174	95	105	97.0	158208	PASS
177	176	5	10	6.6	10460	PASS

Scan 2796 (10.030 min): VV025978.D\data.ms
BFB285

m/z	Abundance
40.00	591.0
44.00	500.0

Instrument :
MSVOA_V
ClientSampleId :
BFB285

m/z	Abundance
36.10	1373.0
37.10	7780.0
38.10	7295.0
39.10	3251.0
40.00	691.0
40.80	146.0
43.00	120.0
44.00	1403.0
45.00	1465.0
46.00	322.0
47.10	2493.0
48.00	1270.0
49.00	7589.0
50.10	32688.0
51.10	10656.0
52.00	618.0
53.00	216.0
54.00	167.0
55.00	620.0
56.00	2778.0
57.00	5089.0
58.00	353.0
60.00	1759.0
61.00	8986.0
62.00	9303.0
63.00	7607.0
64.00	1271.0
65.00	1646.0
66.20	247.0
67.00	526.0
68.00	18648.0
69.10	18904.0
70.10	1516.0
71.00	128.0
72.00	1000.0
73.10	8783.0
74.10	32752.0
75.10	92064.0
76.10	7969.0
77.00	963.0
78.10	636.0
79.00	7590.0
80.00	2151.0
81.00	8033.0
81.90	1797.0
83.10	191.0
86.00	258.0
87.00	8662.0
88.00	8427.0
91.00	819.0
92.00	5614.0
93.10	8971.0
94.10	22672.0
95.10	185280.0
96.10	12584.0
97.00	357.0
102.80	122.0
104.00	908.0
104.90	248.0
105.90	944.0
106.80	212.0
107.80	200.0
109.90	183.0
110.90	166.0
111.80	197.0
112.90	216.0
114.80	178.0
115.90	665.0
116.90	1376.0
117.90	910.0
118.90	1484.0
127.90	748.0
128.90	327.0
130.00	777.0
130.90	308.0
134.80	376.0
137.00	350.0
139.90	174.0
141.00	1924.0
141.90	297.0
142.90	2739.0
143.80	241.0
144.90	845.0
145.90	286.0
147.00	115.0
147.90	529.0
150.00	196.0
152.80	133.0
154.00	108.0
155.00	467.0
155.90	147.0
156.80	310.0

Instrument :
MSVOA_V
ClientSampleId :
BFB285

158.00	111.0
158.90	220.0
160.90	213.0
170.90	554.0
172.00	1881.0
173.10	2066.0
174.00	151744.0
175.00	11668.0
176.00	146688.0
177.00	9845.0
178.00	286.0

Instrument :
MSVOA_V
ClientSampleId :
BFB285

m/z	Abundance
36.00	1402.0
37.10	8191.0
38.00	7834.0
39.10	3716.0
40.00	645.0
40.70	157.0
43.00	163.0
44.00	1508.0
45.00	1493.0
45.90	309.0
47.10	2574.0
48.00	1272.0
49.00	8486.0
50.00	35032.0
51.10	11638.0
52.00	627.0
53.00	208.0
54.10	169.0
55.00	611.0
56.00	3146.0
57.00	5285.0
58.00	348.0
60.10	1804.0
61.00	9521.0
62.00	9726.0
63.00	8150.0
64.00	1517.0
65.10	1778.0
66.20	214.0
67.10	461.0
68.10	19992.0
69.10	20760.0
70.10	1601.0
70.90	154.0
72.00	1091.0
73.10	9567.0
74.10	34880.0
75.10	100624.0
76.10	8439.0
77.00	1127.0
78.10	630.0
79.00	7973.0
80.00	2160.0
81.00	8523.0
81.90	1839.0
83.00	172.0
85.90	314.0
87.00	9542.0
88.00	9282.0
91.00	787.0
92.00	5927.0
93.10	10017.0
94.10	25056.0
95.10	201984.0
96.10	13237.0
97.00	378.0
102.70	127.0
103.90	966.0
105.00	326.0
105.90	1082.0
106.80	186.0
107.80	232.0
109.90	221.0
111.00	161.0
111.80	192.0
113.00	243.0
114.90	209.0
116.00	697.0
116.90	1470.0
117.90	928.0
118.90	1629.0
122.90	115.0
127.90	847.0
128.90	317.0
130.00	906.0
130.90	366.0
134.80	391.0
137.00	415.0
139.80	170.0
140.90	2195.0
141.90	314.0
142.90	2985.0
143.80	234.0
145.00	888.0
145.80	299.0
147.00	132.0
147.90	553.0
148.80	107.0
150.00	255.0
152.80	148.0
154.00	137.0
155.00	531.0

Instrument :
MSVOA_V
ClientSampleId :
BFB285

155.90	118.0
156.80	412.0
158.00	126.0
158.90	272.0
160.90	229.0
170.90	521.0
172.00	2127.0
173.10	2286.0
174.00	168320.0
175.00	12664.0
176.00	163776.0
177.00	10849.0
178.00	313.0

Instrument :
MSVOA_V
ClientSampleId :
BFB285

m/z	Abundance
36.00	1346.0
37.10	7885.0
38.00	7553.0
39.00	3576.0
40.00	666.0
43.00	195.0
44.00	1489.0
45.00	1447.0
46.00	300.0
47.10	2382.0
48.00	1132.0
49.00	8196.0
50.00	34528.0
51.10	11524.0
52.00	612.0
52.90	216.0
54.10	150.0
55.00	544.0
56.00	3145.0
57.10	4933.0
58.00	308.0
60.00	1755.0
61.00	9265.0
62.00	9374.0
63.10	7885.0
64.00	1495.0
65.10	1697.0
66.00	180.0
67.10	456.0
68.10	19328.0
69.10	20520.0
70.10	1557.0
70.90	137.0
72.00	1075.0
73.10	9086.0
74.10	33344.0
75.10	99344.0
76.10	8189.0
77.00	1189.0
78.00	689.0
79.00	7687.0
80.00	2001.0
81.00	8016.0
81.90	1718.0
82.90	186.0
85.90	321.0
87.00	9419.0
88.00	8863.0
91.00	758.0
92.00	5782.0
93.10	9751.0
94.10	24512.0
95.10	198144.0
96.10	12576.0
97.00	395.0
102.70	108.0
103.90	950.0
105.00	370.0
105.90	1018.0
106.80	137.0
107.80	207.0
109.90	234.0
111.00	177.0
111.80	162.0
112.90	244.0
115.00	232.0
116.00	671.0
116.90	1463.0
117.90	794.0
118.90	1484.0
122.90	106.0
127.90	908.0
128.80	308.0
130.00	903.0
130.90	397.0
134.80	308.0
137.00	424.0
139.80	154.0
140.90	2205.0
141.90	276.0
142.90	3027.0
143.80	186.0
145.00	865.0
145.80	303.0
147.00	146.0
147.90	480.0
148.80	133.0
150.00	279.0
152.10	126.0
152.90	148.0
154.00	151.0
154.90	530.0

Instrument :
MSVOA_V
ClientSampleId :
BFB285

156.90	467.0
158.00	102.0
158.90	280.0
160.90	187.0
171.00	411.0
172.00	2096.0
173.10	2308.0
174.00	169024.0
175.00	12505.0
176.00	164160.0
177.00	10685.0
178.00	354.0

Instrument :
MSVOA_V
ClientSampleId :
BFB285