
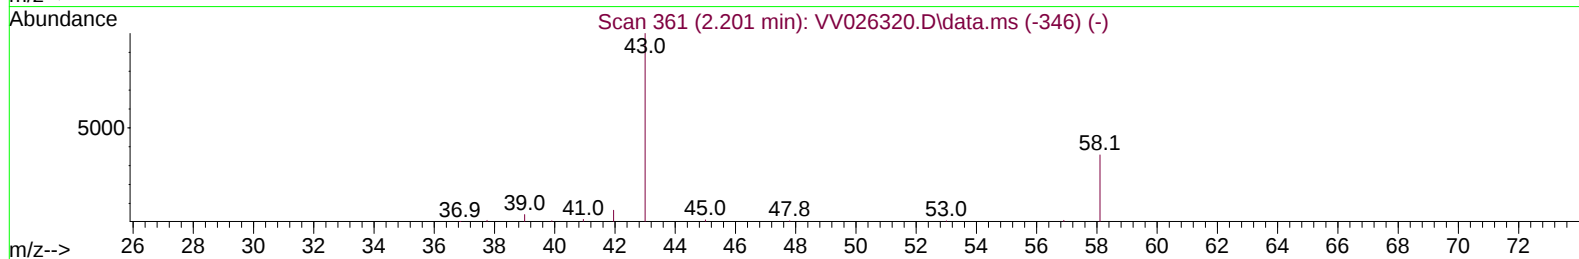
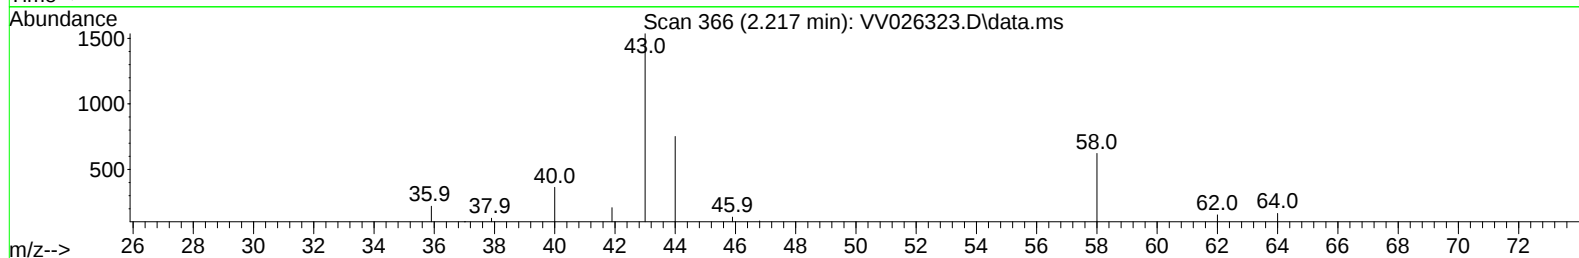


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061622\
Data File : VV026323.D
Acq On : 16 Jun 2022 11:00
Operator : SY/MD
Sample : N3274-09DL 10X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Jun 17 05:18:33 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jun 17 05:16:46 2022
Response via : Initial Calibration

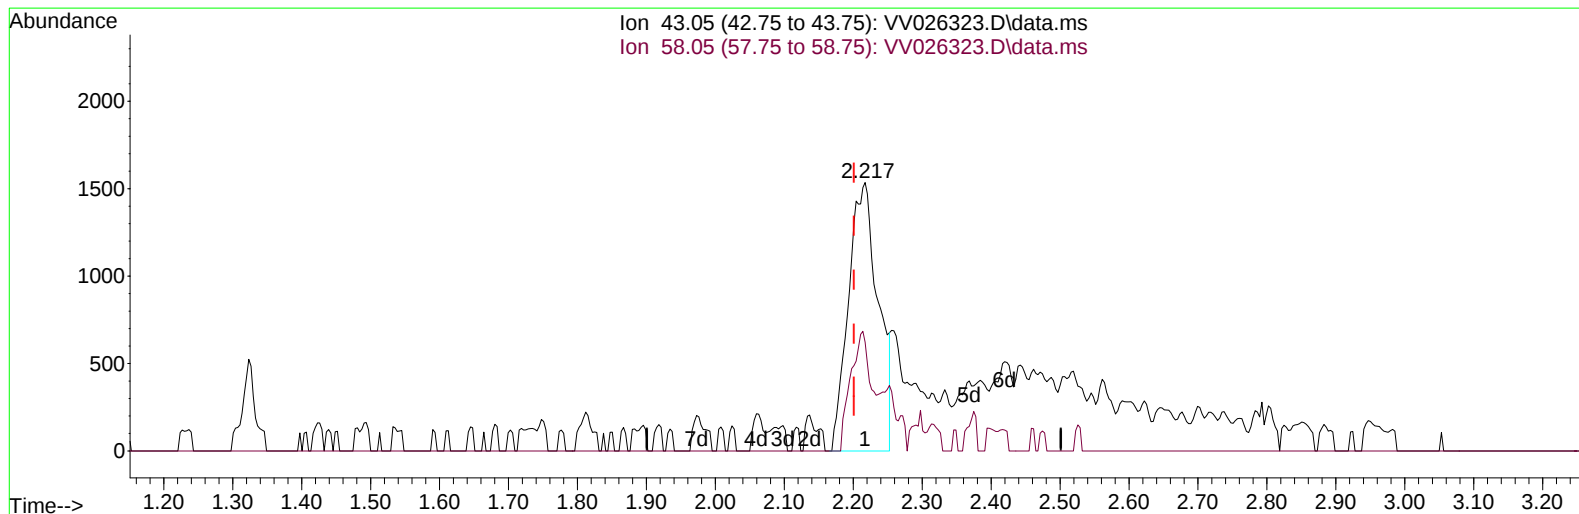

TIC: VV026323.D\data.ms

(13) Acetone (T)

2.217min (+ 0.016) 3.57 ug/L

response 4601

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	30.00	29.82
0.00	0.00	0.00
0.00	0.00	0.00