




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061622\
 Data File : VV026331.D
 Acq On : 16 Jun 2022 14:11
 Operator : SY/MD
 Sample : N3275-03
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BD5

Manual IntegrationsAPPROVED

Quant Time: Jun 17 05:20:27 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jun 17 05:16:46 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/17/2022
 Supervised By :Mahesh Dadoda 06/20/2022

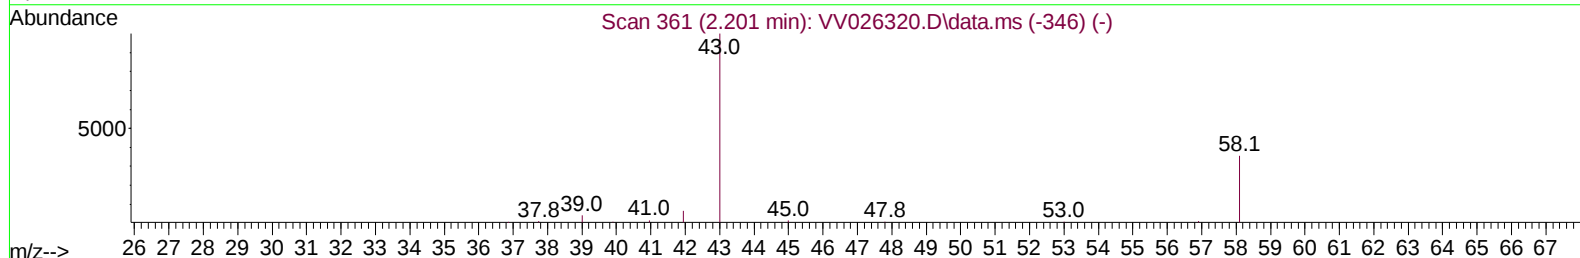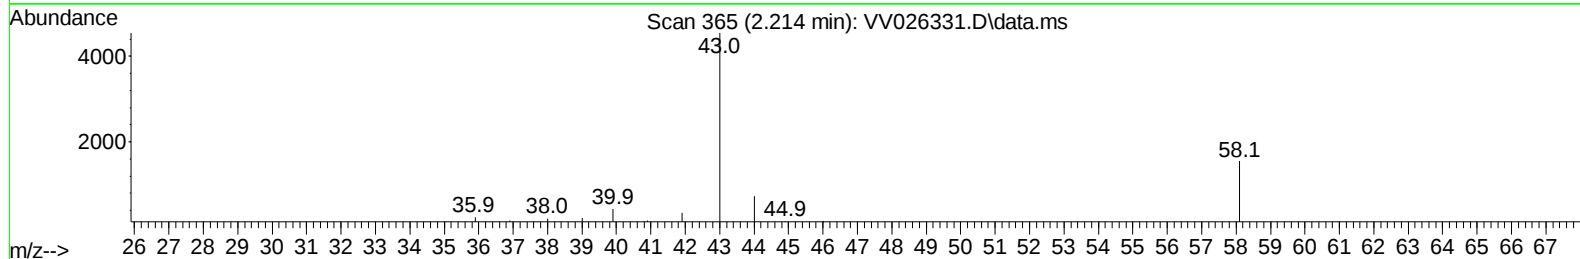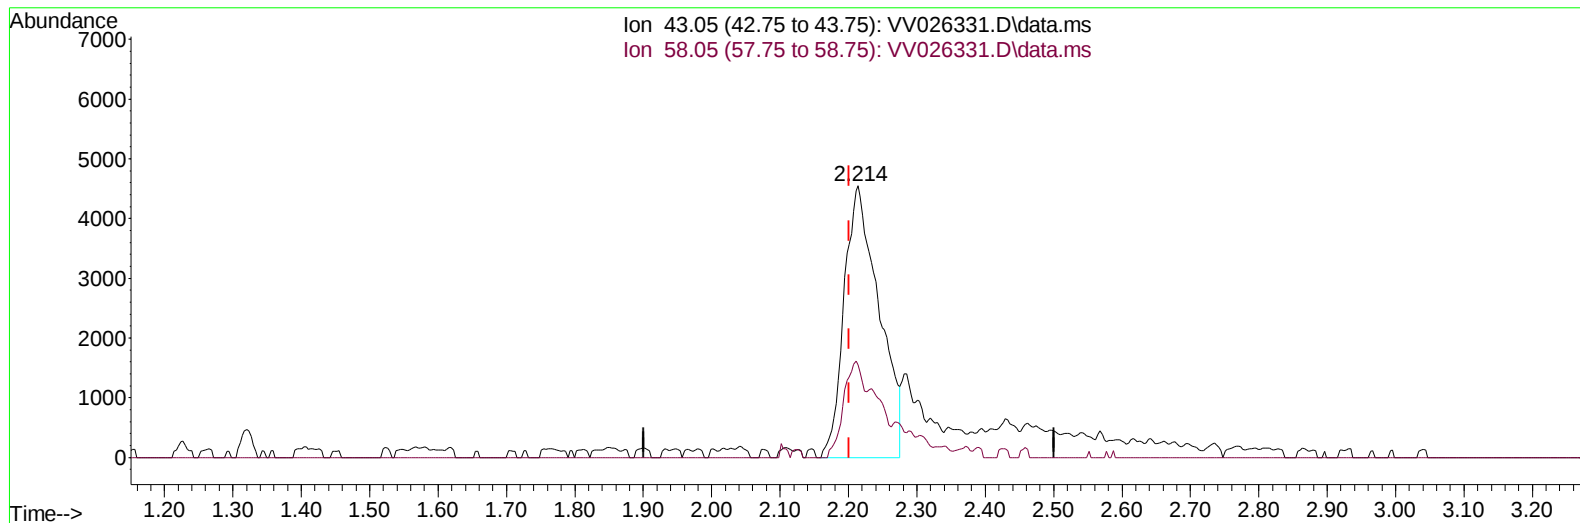

TIC: VV026331.D\data.ms

(13) Acetone (T)

2.214min (+ 0.013) 10.14 ug/L

response 16138

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	30.00	20.86
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061622\
 Data File : VV026331.D
 Acq On : 16 Jun 2022 14:11
 Operator : SY/MD
 Sample : N3275-03
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BD5

Manual IntegrationsAPPROVED

Quant Time: Jun 17 05:20:27 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jun 17 05:16:46 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/17/2022
 Supervised By :Mahesh Dadoda 06/20/2022

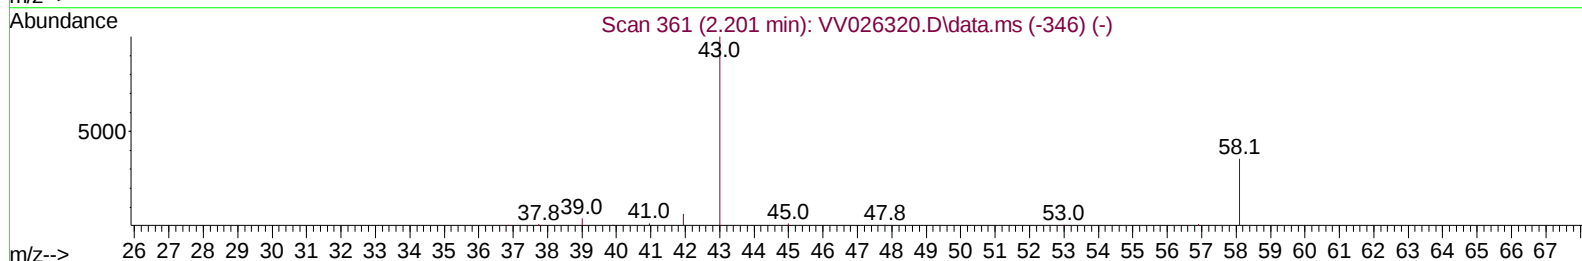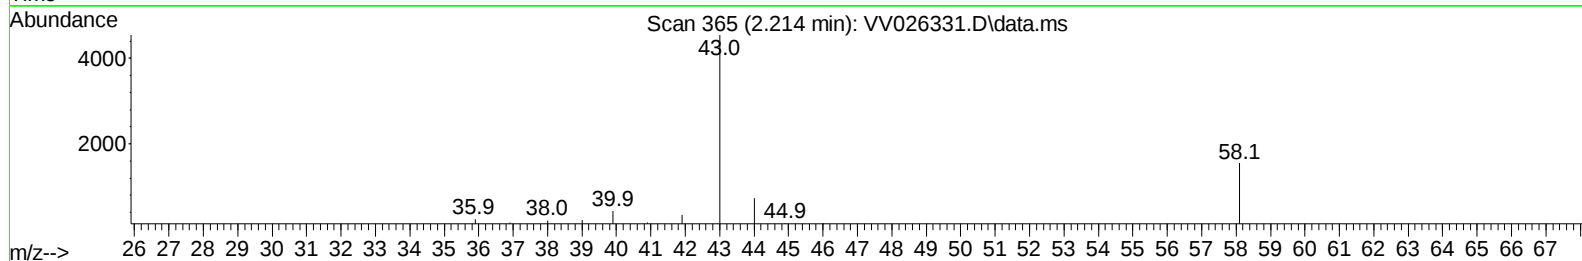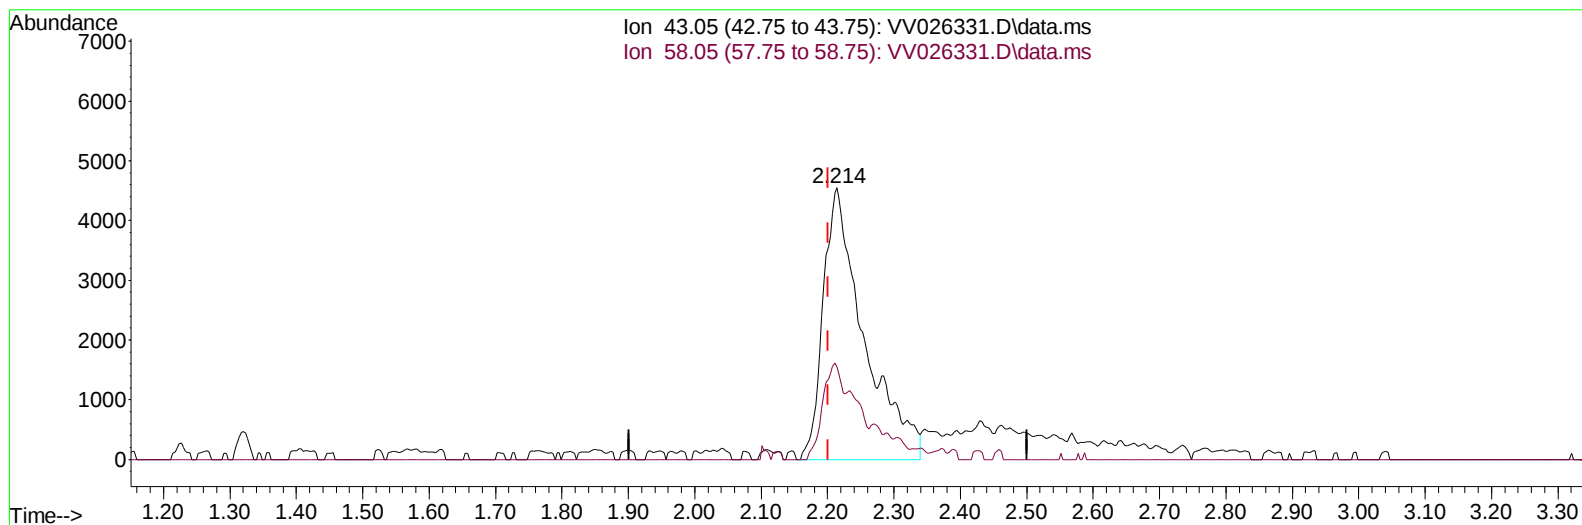

TIC: VV026331.D\data.ms

(13) Acetone (T)

2.214min (+ 0.013) 12.15 ug/L m

response 19339

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	30.00	17.41
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061622\
 Data File : VV026331.D
 Acq On : 16 Jun 2022 14:11
 Operator : SY/MD
 Sample : N3275-03
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BD5

Manual IntegrationsAPPROVED

Quant Time: Jun 17 05:20:27 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jun 17 05:16:46 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/17/2022
 Supervised By :Mahesh Dadoda 06/20/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.625	114	242368	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	230496	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	93283	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.320	65	67780	3.220	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	64.400%	
7) Chloroethane-d5	1.581	69	58857	3.556	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	71.200%	
11) 1,1-Dichloroethene-d2	2.121	63	95373	2.638	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	=	52.800%#	
20) 2-Butanone-d5	3.925	46	85507	41.627	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130	Recovery	=	83.260%	
24) Chloroform-d	4.362	84	118488	3.840	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	76.800%	
26) 1,2-Dichloroethane-d4	5.044	65	49355	3.781	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	75.600%	
32) Benzene-d6	5.060	84	228171	3.703	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	74.000%	
36) 1,2-Dichloropropane-d6	6.076	67	69542	3.867	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery	=	77.400%	
41) Toluene-d8	7.320	98	180935	3.220	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	64.400%#	
43) trans-1,3-Dichloroprop...	7.629	79	17965	3.080	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery	=	61.600%	
46) 2-Hexanone-d5	8.092	63	61008	34.630	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130	Recovery	=	69.260%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	40775	3.680	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	73.600%	
66) 1,2-Dichlorobenzene-d4	11.625	152	62237	4.331	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	86.600%	
Target Compounds						
9) Trichlorofluoromethane	1.764	101	3792	0.131	ug/L	99
13) Acetone	2.214	43	19339m	12.149	ug/L	
34) Trichloroethene	5.925	95	16489	1.022	ug/L	94
47) Tetrachloroethene	7.982	164	3268	0.273	ug/L	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061622\
Data File : VV026331.D
Acq On : 16 Jun 2022 14:11
Operator : SY/MD
Sample : N3275-03
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BD5

Manual IntegrationsAPPROVED

Quant Time: Jun 17 05:20:27 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jun 17 05:16:46 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 06/17/2022
Supervised By :Mahesh Dadoda 06/20/2022

