




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061622\
Data File : VV026333.D
Acq On : 16 Jun 2022 14:59
Operator : SY/MD
Sample : N3275-06
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BD8

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 06/17/2022
Supervised By :Mahesh Dadoda 06/20/2022

Quant Time: Jun 17 05:21:04 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jun 17 05:16:46 2022
Response via : Initial Calibration

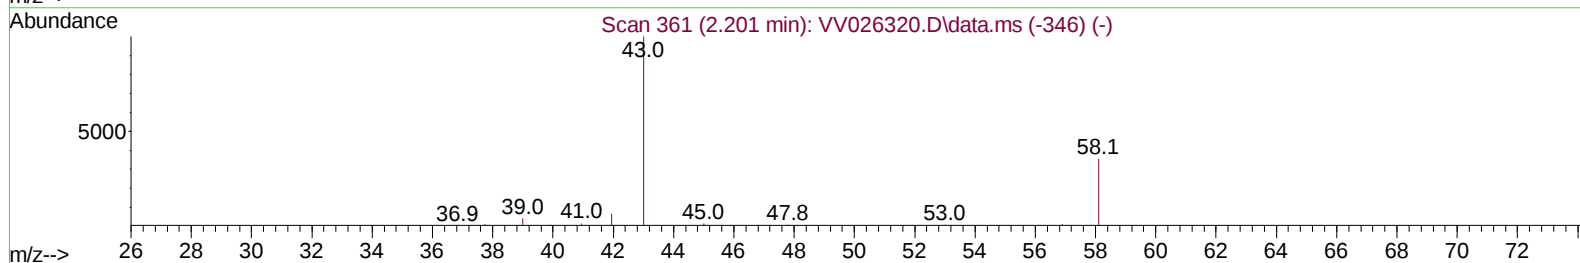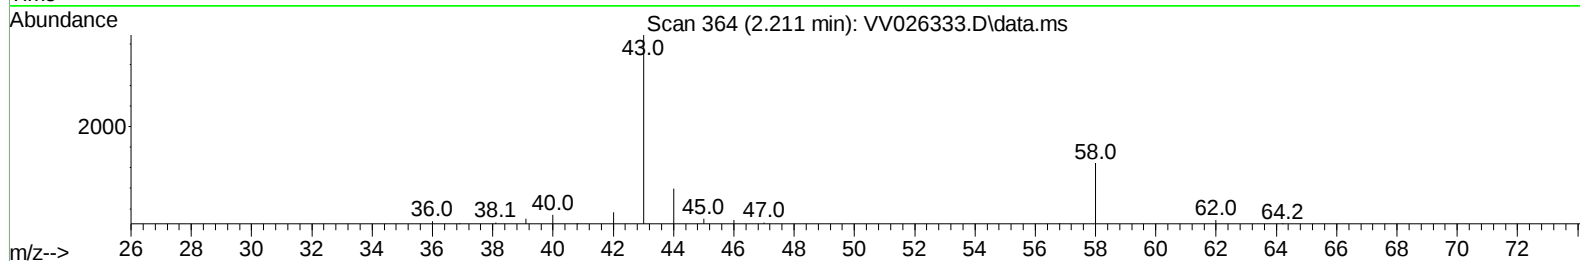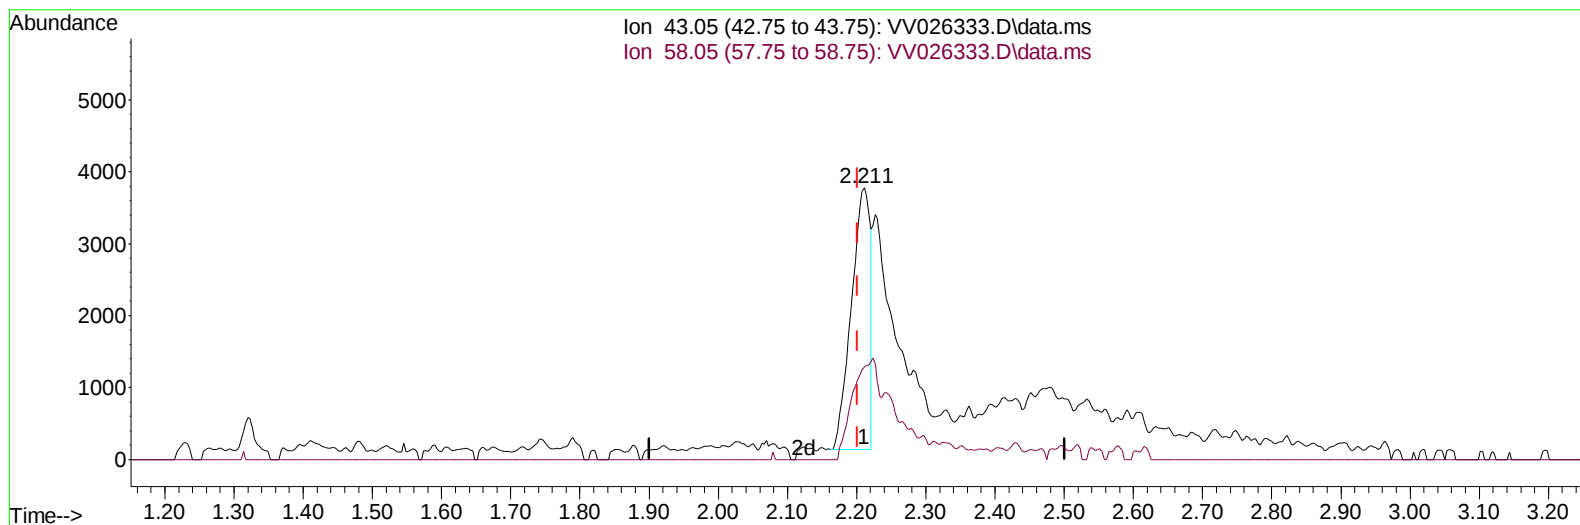

TIC: VV026333.D\data.ms

(13) Acetone (T)

2.211min (+ 0.010) 4.60 ug/L

response 6855

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	30.00	53.65
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061622\
Data File : VV026333.D
Acq On : 16 Jun 2022 14:59
Operator : SY/MD
Sample : N3275-06
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BD8

Manual IntegrationsAPPROVED

Quant Time: Jun 17 05:21:04 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jun 17 05:16:46 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 06/17/2022
Supervised By :Mahesh Dadoda 06/20/2022

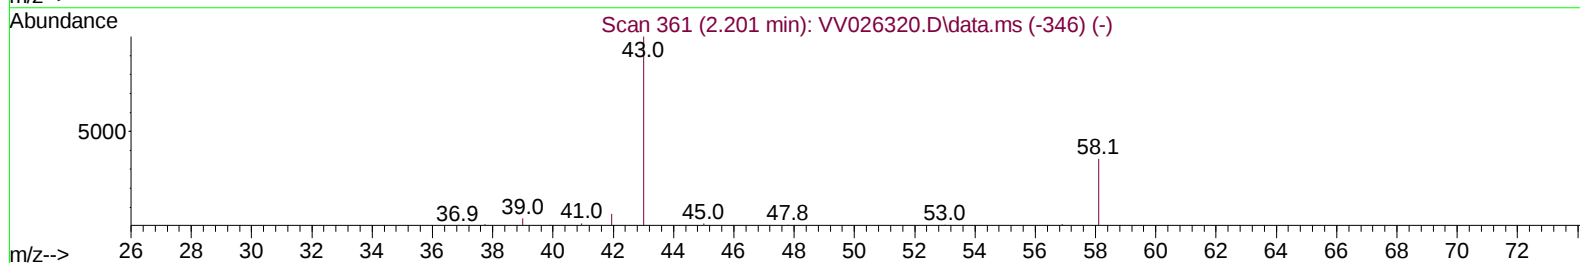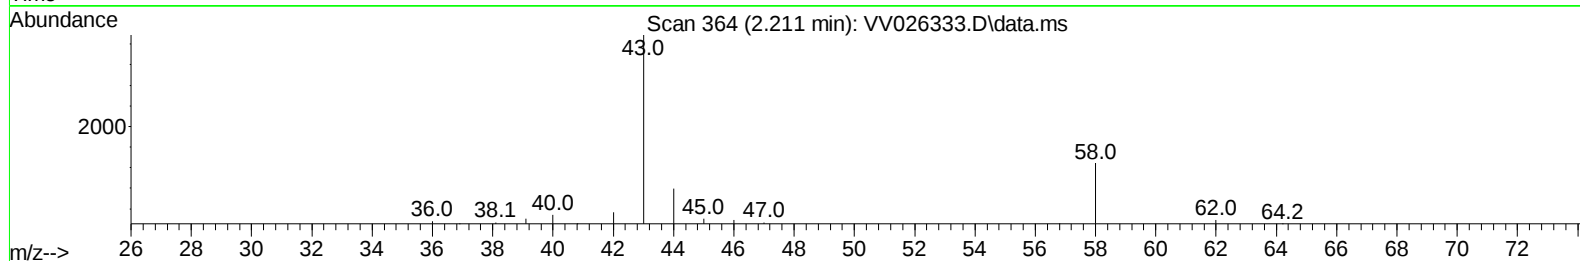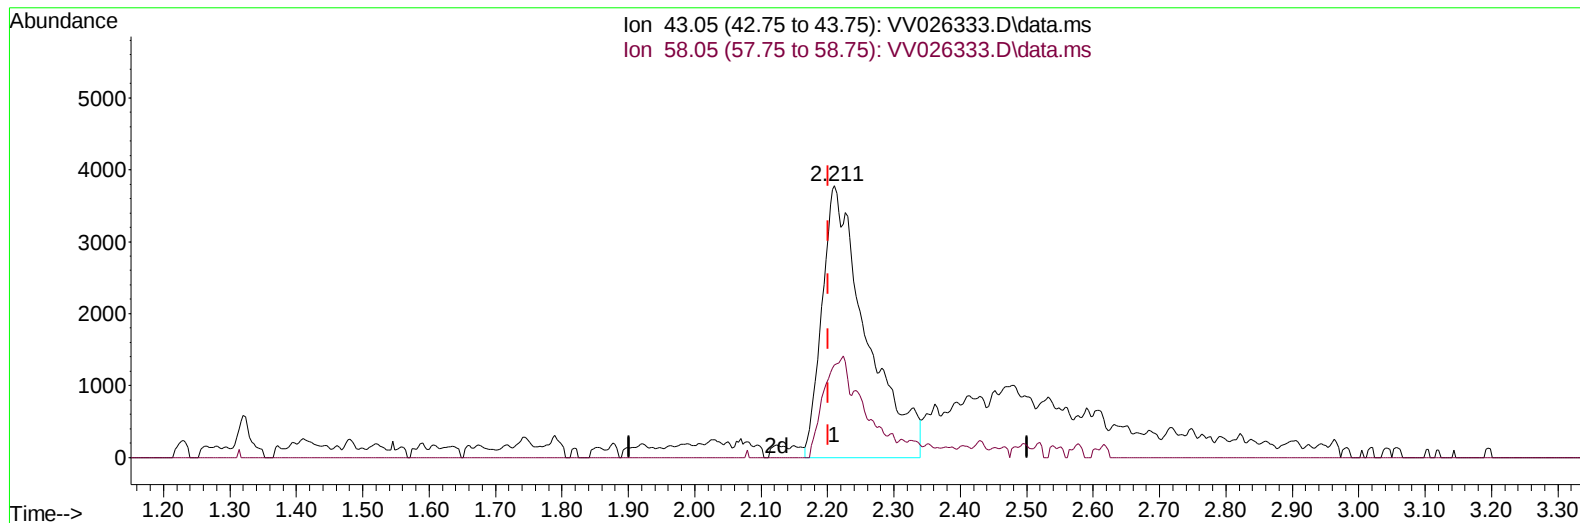

TIC: VV026333.D\data.ms

(13) Acetone (T)

2.211min (+ 0.010) 11.71 ug/L m

response 17461

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	30.00	21.06
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061622\
 Data File : VV026333.D
 Acq On : 16 Jun 2022 14:59
 Operator : SY/MD
 Sample : N3275-06
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BD8

Manual IntegrationsAPPROVED

Quant Time: Jun 17 05:21:04 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jun 17 05:16:46 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/17/2022
 Supervised By :Mahesh Dadoda 06/20/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	227104	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	218250	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	85517	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.320	65	67045	3.399	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	68.000%	
7) Chloroethane-d5	1.581	69	57582	3.713	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	74.200%	
11) 1,1-Dichloroethene-d2	2.121	63	95663	2.824	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	=	56.400%#	
20) 2-Butanone-d5	3.918	46	85646	44.497	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130	Recovery	=	89.000%	
24) Chloroform-d	4.362	84	121359	4.198	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	84.000%	
26) 1,2-Dichloroethane-d4	5.043	65	48519	3.967	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	79.400%	
32) Benzene-d6	5.060	84	229492	3.933	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	78.600%	
36) 1,2-Dichloropropane-d6	6.076	67	72339	4.248	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery	=	85.000%	
41) Toluene-d8	7.320	98	182166	3.424	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	68.400%#	
43) trans-1,3-Dichloroprop...	7.629	79	19280	3.491	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery	=	69.800%	
46) 2-Hexanone-d5	8.092	63	62686	37.579	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130	Recovery	=	75.160%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	42492	4.050	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	81.000%	
66) 1,2-Dichlorobenzene-d4	11.622	152	62473	4.743	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	94.800%	
Target Compounds						
					Qvalue	
9) Trichlorofluoromethane	1.767	101	2860	0.106	ug/L	100
13) Acetone	2.211	43	17461m	11.706	ug/L	
34) Trichloroethene	5.931	95	3019	0.198	ug/L	89
47) Tetrachloroethene	7.986	164	2543	0.225	ug/L	91

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061622\
Data File : VV026333.D
Acq On : 16 Jun 2022 14:59
Operator : SY/MD
Sample : N3275-06
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BD8

Manual IntegrationsAPPROVED

Quant Time: Jun 17 05:21:04 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jun 17 05:16:46 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 06/17/2022
Supervised By :Mahesh Dadoda 06/20/2022

