




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061622\
 Data File : VV026345.D
 Acq On : 16 Jun 2022 20:05
 Operator : SY/MD
 Sample : N3320-12 5X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGJ87

Manual IntegrationsAPPROVED

Quant Time: Jun 17 05:25:05 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jun 17 05:16:46 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/17/2022
 Supervised By :Mahesh Dadoda 06/20/2022

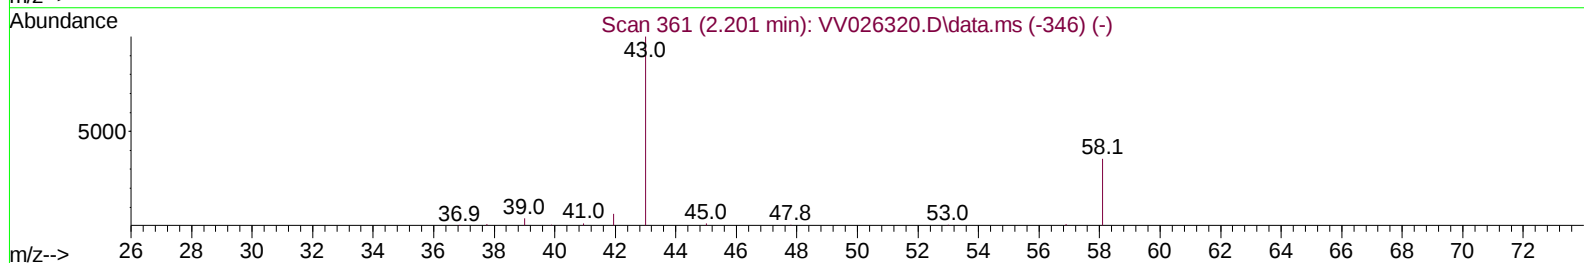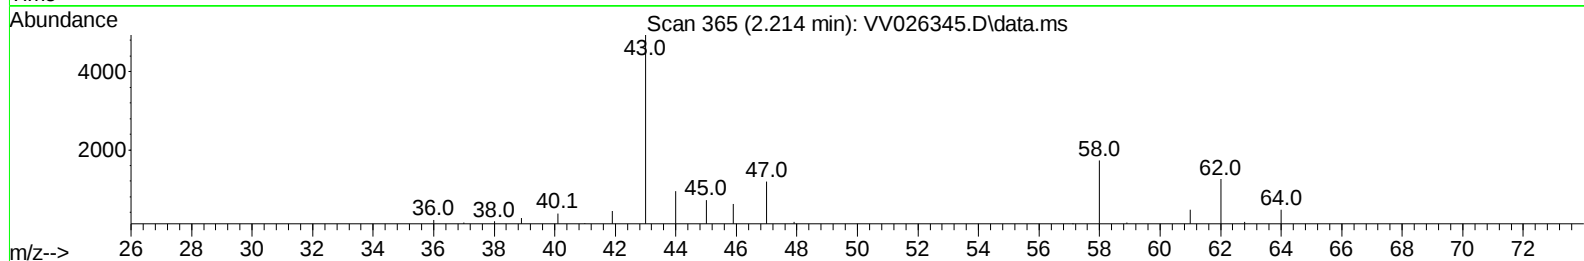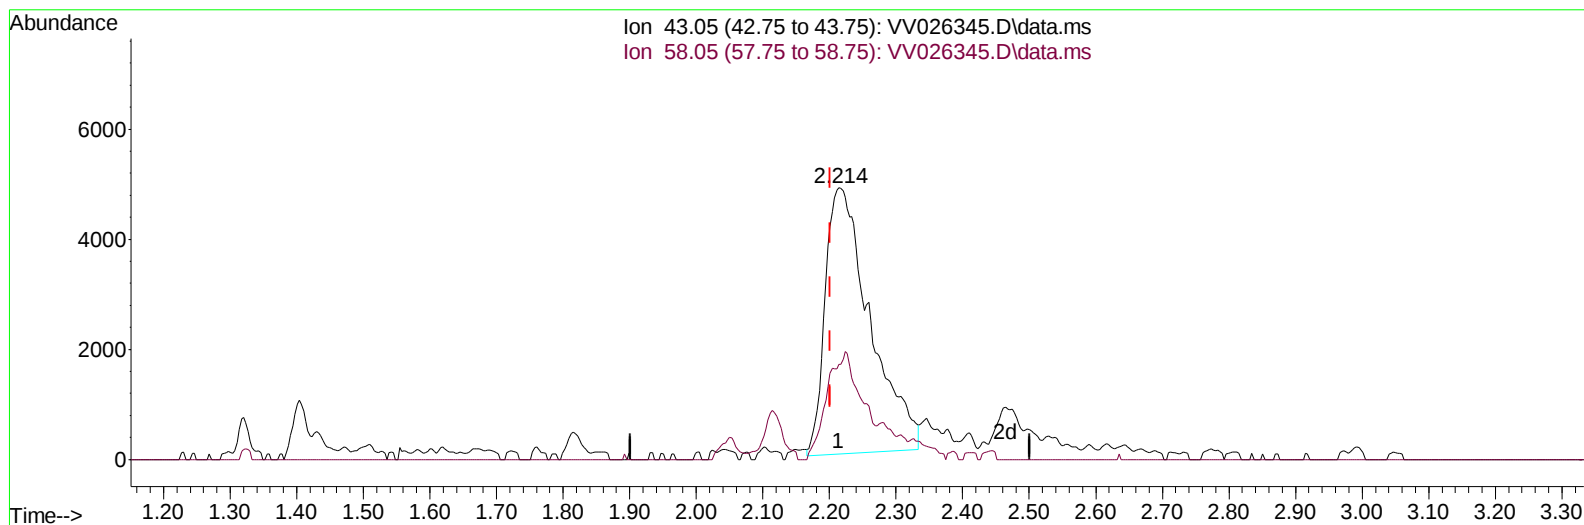

TIC: VV026345.D\data.ms

(13) Acetone (T)

2.214min (+ 0.013) 17.40 ug/L

response 22582

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	30.00	30.71
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061622\
 Data File : VV026345.D
 Acq On : 16 Jun 2022 20:05
 Operator : SY/MD
 Sample : N3320-12 5X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGJ87

Manual IntegrationsAPPROVED

Quant Time: Jun 17 05:25:05 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jun 17 05:16:46 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/17/2022
 Supervised By :Mahesh Dadoda 06/20/2022

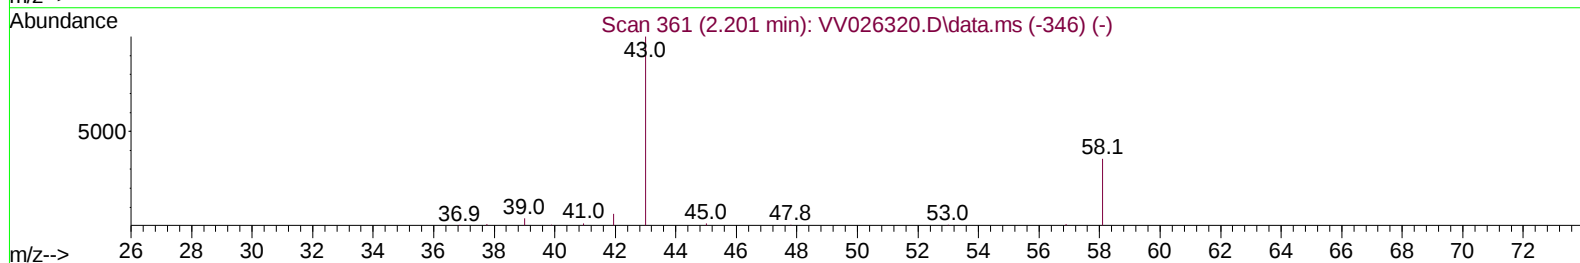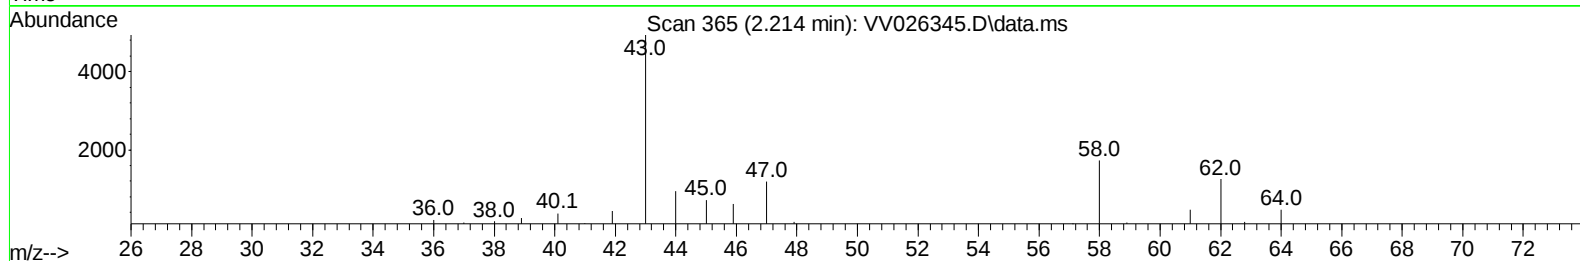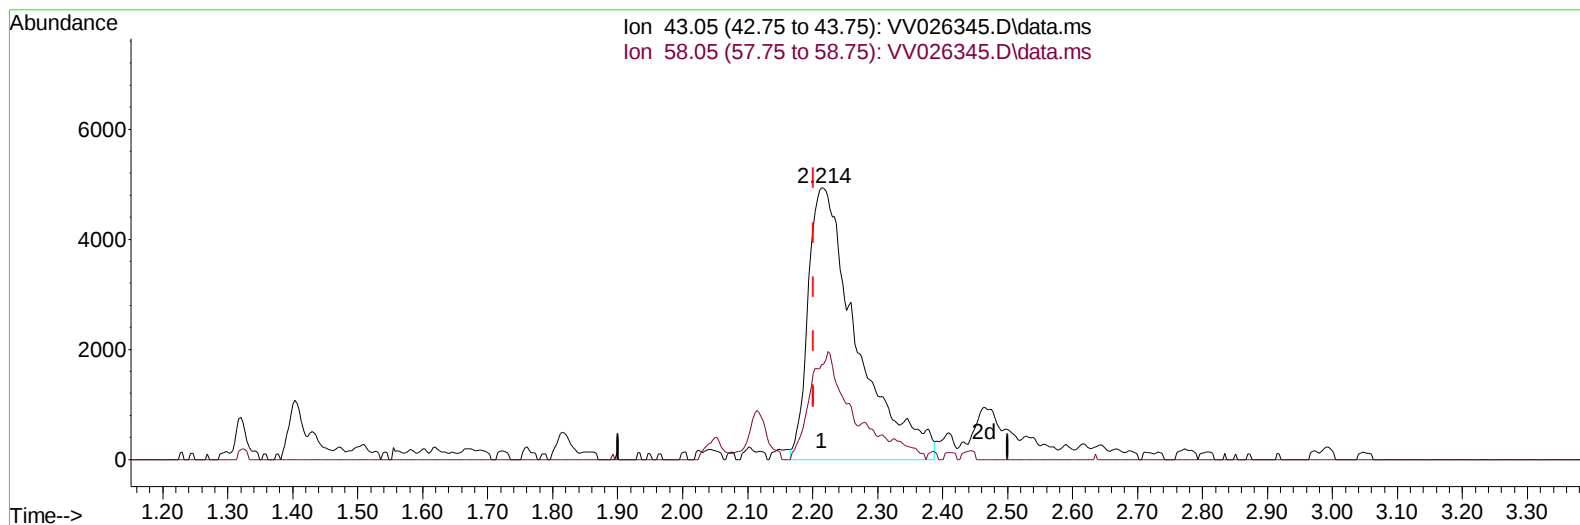

TIC: VV026345.D\data.ms

(13) Acetone (T)

2.214min (+ 0.013) 19.73 ug/L m

response 25598

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	30.00	27.10
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061622\
 Data File : VV026345.D
 Acq On : 16 Jun 2022 20:05
 Operator : SY/MD
 Sample : N3320-12 5X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGJ87

Manual IntegrationsAPPROVED

Quant Time: Jun 17 05:25:05 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jun 17 05:16:46 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/17/2022
 Supervised By :Mahesh Dadoda 06/20/2022

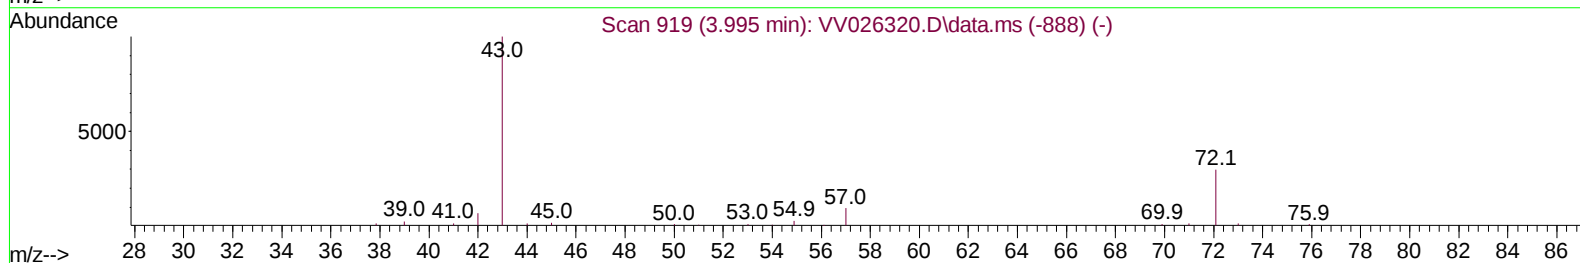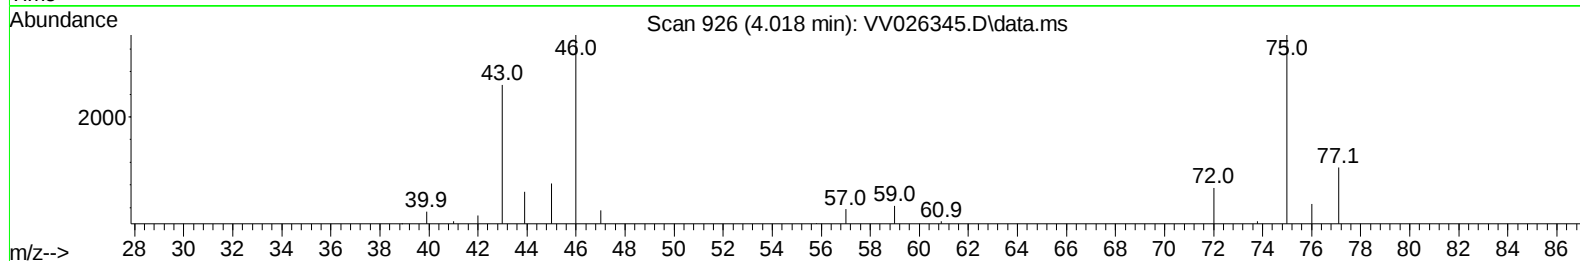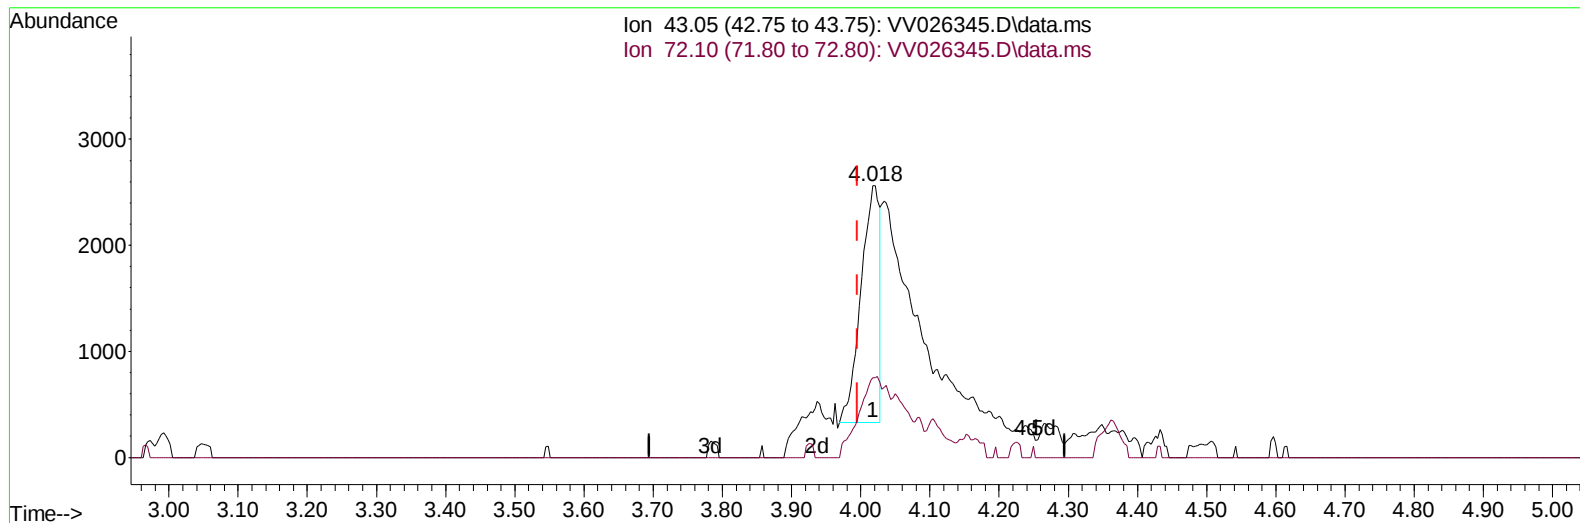

TIC: VV026345.D\data.ms

(21) 2-Butanone (T)

4.018min (+ 0.023) 2.45 ug/L

response 4119

Ion	Exp%	Act%
43.05	100.00	100.00
72.10	25.30	53.29#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061622\
 Data File : VV026345.D
 Acq On : 16 Jun 2022 20:05
 Operator : SY/MD
 Sample : N3320-12 5X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGJ87

Manual IntegrationsAPPROVED

Quant Time: Jun 17 05:25:05 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jun 17 05:16:46 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/17/2022
 Supervised By :Mahesh Dadoda 06/20/2022

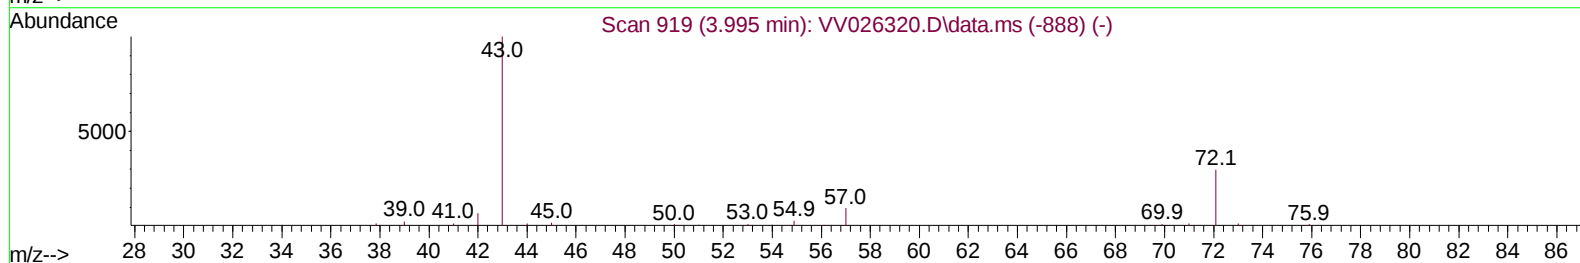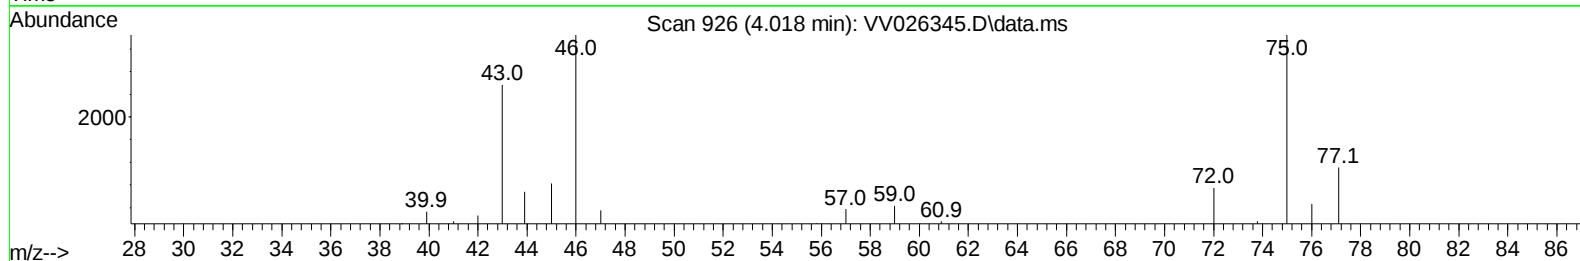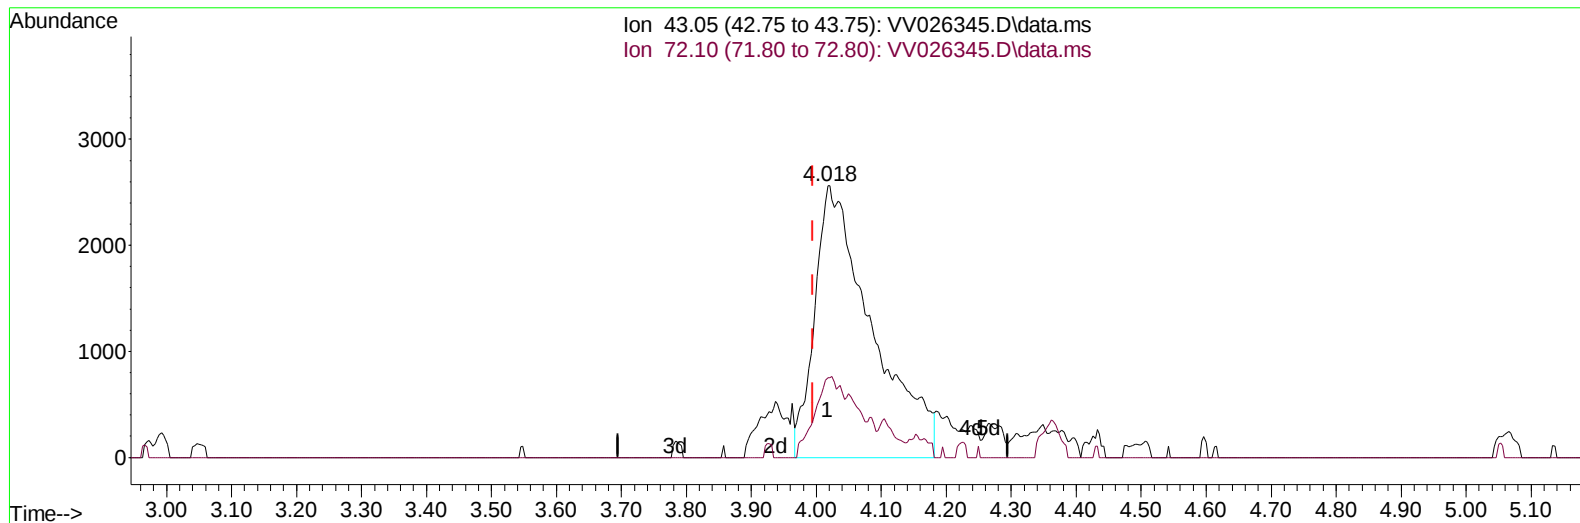

TIC: VV026345.D\data.ms

(21) 2-Butanone (T)

4.018min (+ 0.023) 9.30 ug/L m

response 15616

Ion	Exp%	Act%
43.05	100.00	100.00
72.10	25.30	14.06
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061622\
 Data File : VV026345.D
 Acq On : 16 Jun 2022 20:05
 Operator : SY/MD
 Sample : N3320-12 5X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGJ87

Manual IntegrationsAPPROVED

Quant Time: Jun 17 05:25:05 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jun 17 05:16:46 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/17/2022
 Supervised By :Mahesh Dadoda 06/20/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.625	114	197580	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	187234	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	77793	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.320	65	65952	3.843	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	76.800%	
7) Chloroethane-d5	1.581	69	57655	4.273	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	85.400%	
11) 1,1-Dichloroethene-d2	2.121	63	93045	3.157	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	=	63.200%	
20) 2-Butanone-d5	3.928	46	73681	44.001	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130	Recovery	=	88.000%	
24) Chloroform-d	4.362	84	119524	4.752	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	95.000%	
26) 1,2-Dichloroethane-d4	5.043	65	47726	4.485	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	89.600%	
32) Benzene-d6	5.059	84	227376	4.542	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	90.800%	
36) 1,2-Dichloropropane-d6	6.075	67	70329	4.814	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery	=	96.200%	
41) Toluene-d8	7.320	98	182687	4.002	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	80.000%	
43) trans-1,3-Dichloroprop...	7.628	79	17483	3.690	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery	=	73.800%	
46) 2-Hexanone-d5	8.091	63	55923	39.079	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130	Recovery	=	78.160%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	41916	4.657	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	93.200%	
66) 1,2-Dichlorobenzene-d4	11.625	152	59751	4.986	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	99.800%	
Target Compounds						
3) Chloromethane	1.256	50	1338	0.082	ug/L	100
13) Acetone	2.214	43	25598m	19.725	ug/L	
14) Carbon disulfide	2.310	76	6283	0.204	ug/L #	93
16) Methylene chloride	2.523	84	6502	0.408	ug/L	96
19) 1,1-Dichloroethane	3.211	63	4414	0.191	ug/L	96
21) 2-Butanone	4.018	43	15616m	9.300	ug/L	
22) cis-1,2-Dichloroethene	3.928	96	5209	0.425	ug/L	99
34) Trichloroethene	5.921	95	8656	0.660	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061622\
Data File : VV026345.D
Acq On : 16 Jun 2022 20:05
Operator : SY/MD
Sample : N3320-12 5X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGJ87

Manual IntegrationsAPPROVED

Quant Time: Jun 17 05:25:05 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jun 17 05:16:46 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 06/17/2022
Supervised By :Mahesh Dadoda 06/20/2022

