




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061622\
 Data File : VV026349.D
 Acq On : 16 Jun 2022 22:05
 Operator : SY/MD
 Sample : N3318-07
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGJ61

Manual IntegrationsAPPROVED

Quant Time: Jun 17 07:19:03 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jun 17 06:57:04 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/17/2022
 Supervised By :Mahesh Dadoda 06/20/2022

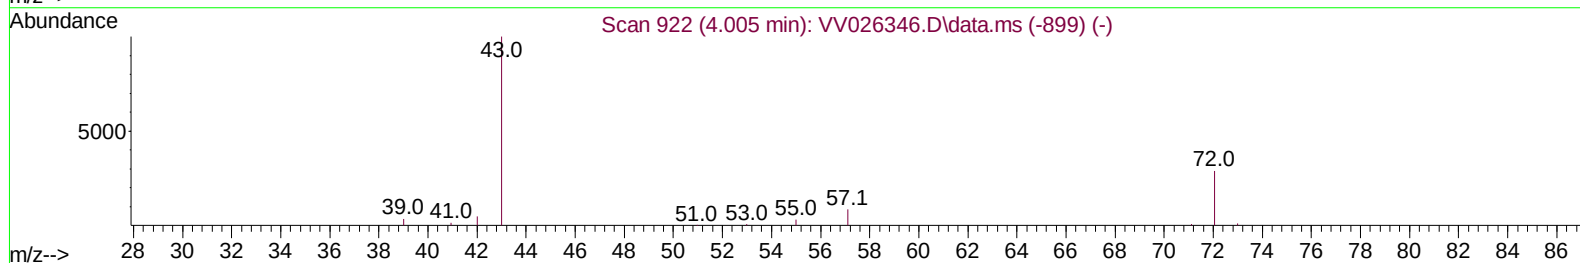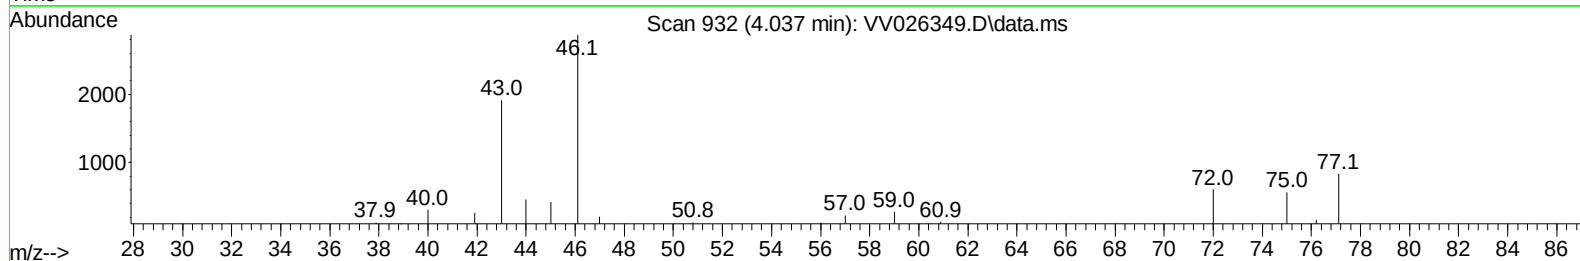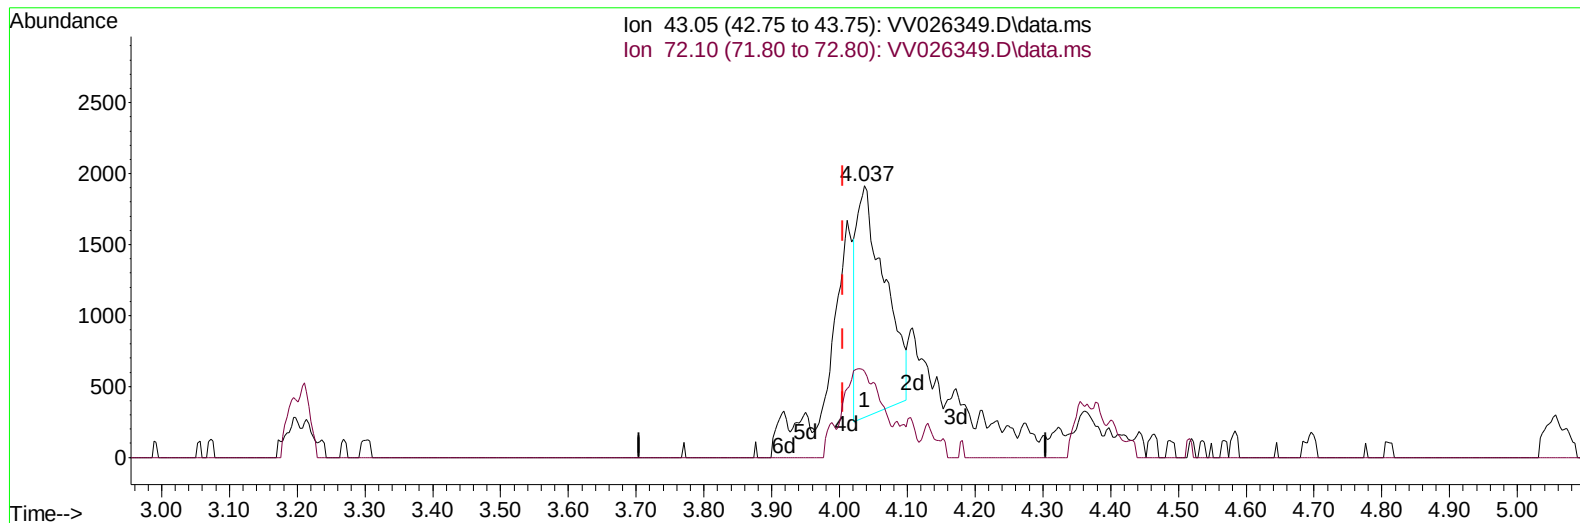

TIC: VV026349.D\data.ms

(21) 2-Butanone (T)

4.037min (+ 0.032) 2.99 ug/L

response 4652

Ion	Exp%	Act%
43.05	100.00	100.00
72.10	25.30	36.18
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061622\
 Data File : VV026349.D
 Acq On : 16 Jun 2022 22:05
 Operator : SY/MD
 Sample : N3318-07
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGJ61

Manual IntegrationsAPPROVED

Quant Time: Jun 17 07:19:03 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jun 17 06:57:04 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/17/2022
 Supervised By :Mahesh Dadoda 06/20/2022

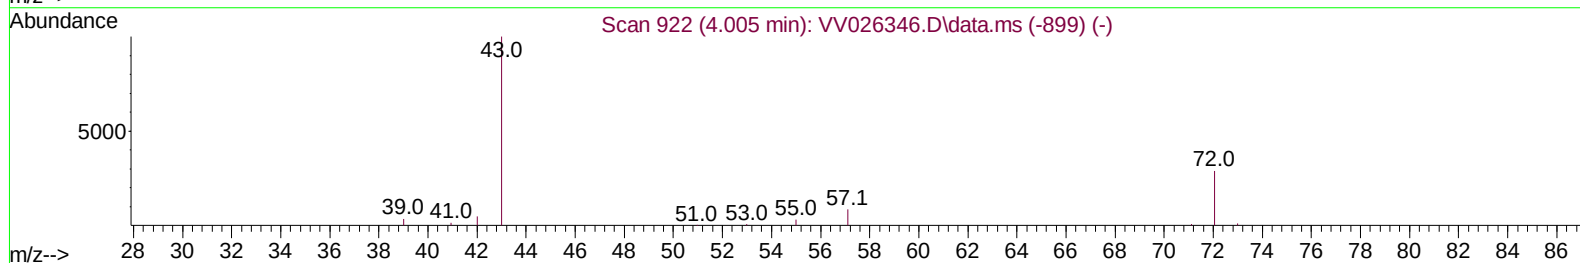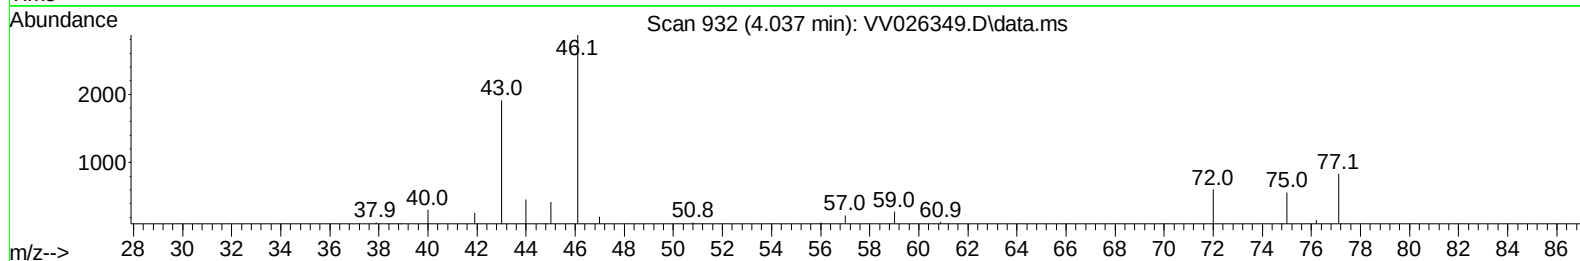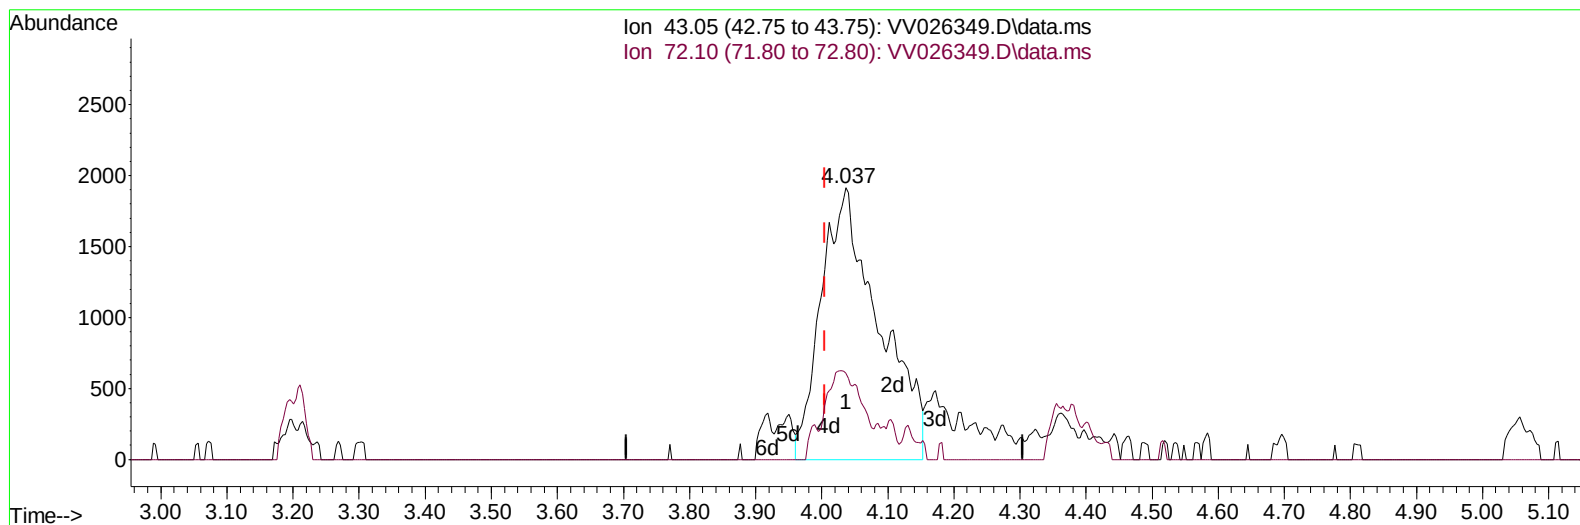

TIC: VV026349.D\data.ms

(21) 2-Butanone (T)

4.037min (+ 0.032) 7.46 ug/L m

response 11601

Ion	Exp%	Act%
43.05	100.00	100.00
72.10	25.30	14.51
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061622\
 Data File : VV026349.D
 Acq On : 16 Jun 2022 22:05
 Operator : SY/MD
 Sample : N3318-07
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGJ61

Manual IntegrationsAPPROVED

Quant Time: Jun 17 07:19:03 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jun 17 06:57:04 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/17/2022
 Supervised By :Mahesh Dadoda 06/20/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.625	114	182990	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	179154	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	73541	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.320	65	59716	3.757	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	75.200%	
7) Chloroethane-d5	1.581	69	54518	4.362	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	87.200%	
11) 1,1-Dichloroethene-d2	2.127	63	234732	8.600	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	=	172.000%#	
20) 2-Butanone-d5	3.921	46	90458	58.327	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130	Recovery	=	116.660%	
24) Chloroform-d	4.362	84	119153	5.115	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	102.200%	
26) 1,2-Dichloroethane-d4	5.043	65	50455	5.119	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	102.400%	
32) Benzene-d6	5.059	84	221037	4.615	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	92.200%	
36) 1,2-Dichloropropane-d6	6.076	67	69898	5.000	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery	=	100.000%	
41) Toluene-d8	7.320	98	175799	4.025	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	80.600%	
43) trans-1,3-Dichloroprop...	7.629	79	15436	3.405	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery	=	68.200%	
46) 2-Hexanone-d5	8.092	63	67579	49.354	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130	Recovery	=	98.700%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	46202	5.365	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	107.400%	
66) 1,2-Dichlorobenzene-d4	11.622	152	60089	5.305	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	106.000%	
Target Compounds						
					Qvalue	
12) 1,1-Dichloroethene	2.134	96	280813	24.290	ug/L #	72
13) Acetone	2.214	43	18396	15.306	ug/L	89
14) Carbon disulfide	2.310	76	10091	0.354	ug/L	98
15) Methyl Acetate	2.462	43	6554	2.273	ug/L	97
16) Methylene chloride	2.523	84	3160	0.214	ug/L	100
17) Methyl tert-butyl Ether	2.786	73	3316	0.167	ug/L #	84
18) trans-1,2-Dichloroethene	2.780	96	1544	0.138	ug/L	89
19) 1,1-Dichloroethane	3.201	63	854518	39.963	ug/L	98
21) 2-Butanone	4.037	43	11601m	7.460	ug/L	
22) cis-1,2-Dichloroethene	3.928	96	12511	1.103	ug/L	99
27) 1,2-Dichloroethane	5.153	62	9589	0.908	ug/L #	90
33) Benzene	5.114	78	32141	0.700	ug/L	100
34) Trichloroethene	5.924	95	11442	0.912	ug/L	96
37) 1,2-Dichloropropane	6.188	63	4979	0.414	ug/L #	94
47) Tetrachloroethene	7.989	164	532	0.057	ug/L	90
52) Ethylbenzene	9.018	91	7495	0.155	ug/L	91
53) m,p-Xylene	9.143	106	2839	0.150	ug/L	94
54) o-Xylene	9.548	106	1669	0.091	ug/L	87

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061622\
 Data File : VV026349.D
 Acq On : 16 Jun 2022 22:05
 Operator : SY/MD
 Sample : N3318-07
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGJ61

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 06/17/2022
 Supervised By :Mahesh Dadoda 06/20/2022

Quant Time: Jun 17 07:19:03 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jun 17 06:57:04 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev	(Min)

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061622\
Data File : VV026349.D
Acq On : 16 Jun 2022 22:05
Operator : SY/MD
Sample : N3318-07
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGJ61

Manual IntegrationsAPPROVED

Quant Time: Jun 17 07:19:03 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jun 17 06:57:04 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 06/17/2022
Supervised By :Mahesh Dadoda 06/20/2022

