

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW061622\
 Data File : VW026327.D
 Acq On : 16 Jun 2022 12:35
 Operator : SY/MD
 Sample : N3274-21
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Jun 17 05:19:33 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jun 17 05:16:46 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.625	114	188510	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	183835	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	73053	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.320	65	72129	4.405	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	88.200%	
7) Chloroethane-d5	1.581	69	61370	4.767	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	95.400%	
11) 1,1-Dichloroethene-d2	2.121	63	99687	3.545	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	71.000%	
20) 2-Butanone-d5	3.921	46	60703	37.995	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	76.000%	
24) Chloroform-d	4.362	84	123325	5.139	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	102.800%	
26) 1,2-Dichloroethane-d4	5.043	65	48403	4.767	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	95.400%	
32) Benzene-d6	5.060	84	234753	4.776	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	95.600%	
36) 1,2-Dichloropropane-d6	6.076	67	71588	4.991	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	99.800%	
41) Toluene-d8	7.320	98	190322	4.247	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	85.000%	
43) trans-1,3-Dichloroprop...	7.629	79	18759	4.033	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	80.600%	
46) 2-Hexanone-d5	8.092	63	56406	40.145	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	80.280%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	40830	4.621	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	92.400%	
66) 1,2-Dichlorobenzene-d4	11.622	152	60032	5.335	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	106.600%	
Target Compounds						
16) Methylene chloride	2.519	84	3316	0.218	ug/L	Qvalue 86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061622\
Data File : VV026327.D
Acq On : 16 Jun 2022 12:35
Operator : SY/MD
Sample : N3274-21
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001


Quant Time: Jun 17 05:19:33 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jun 17 05:16:46 2022
Response via : Initial Calibration

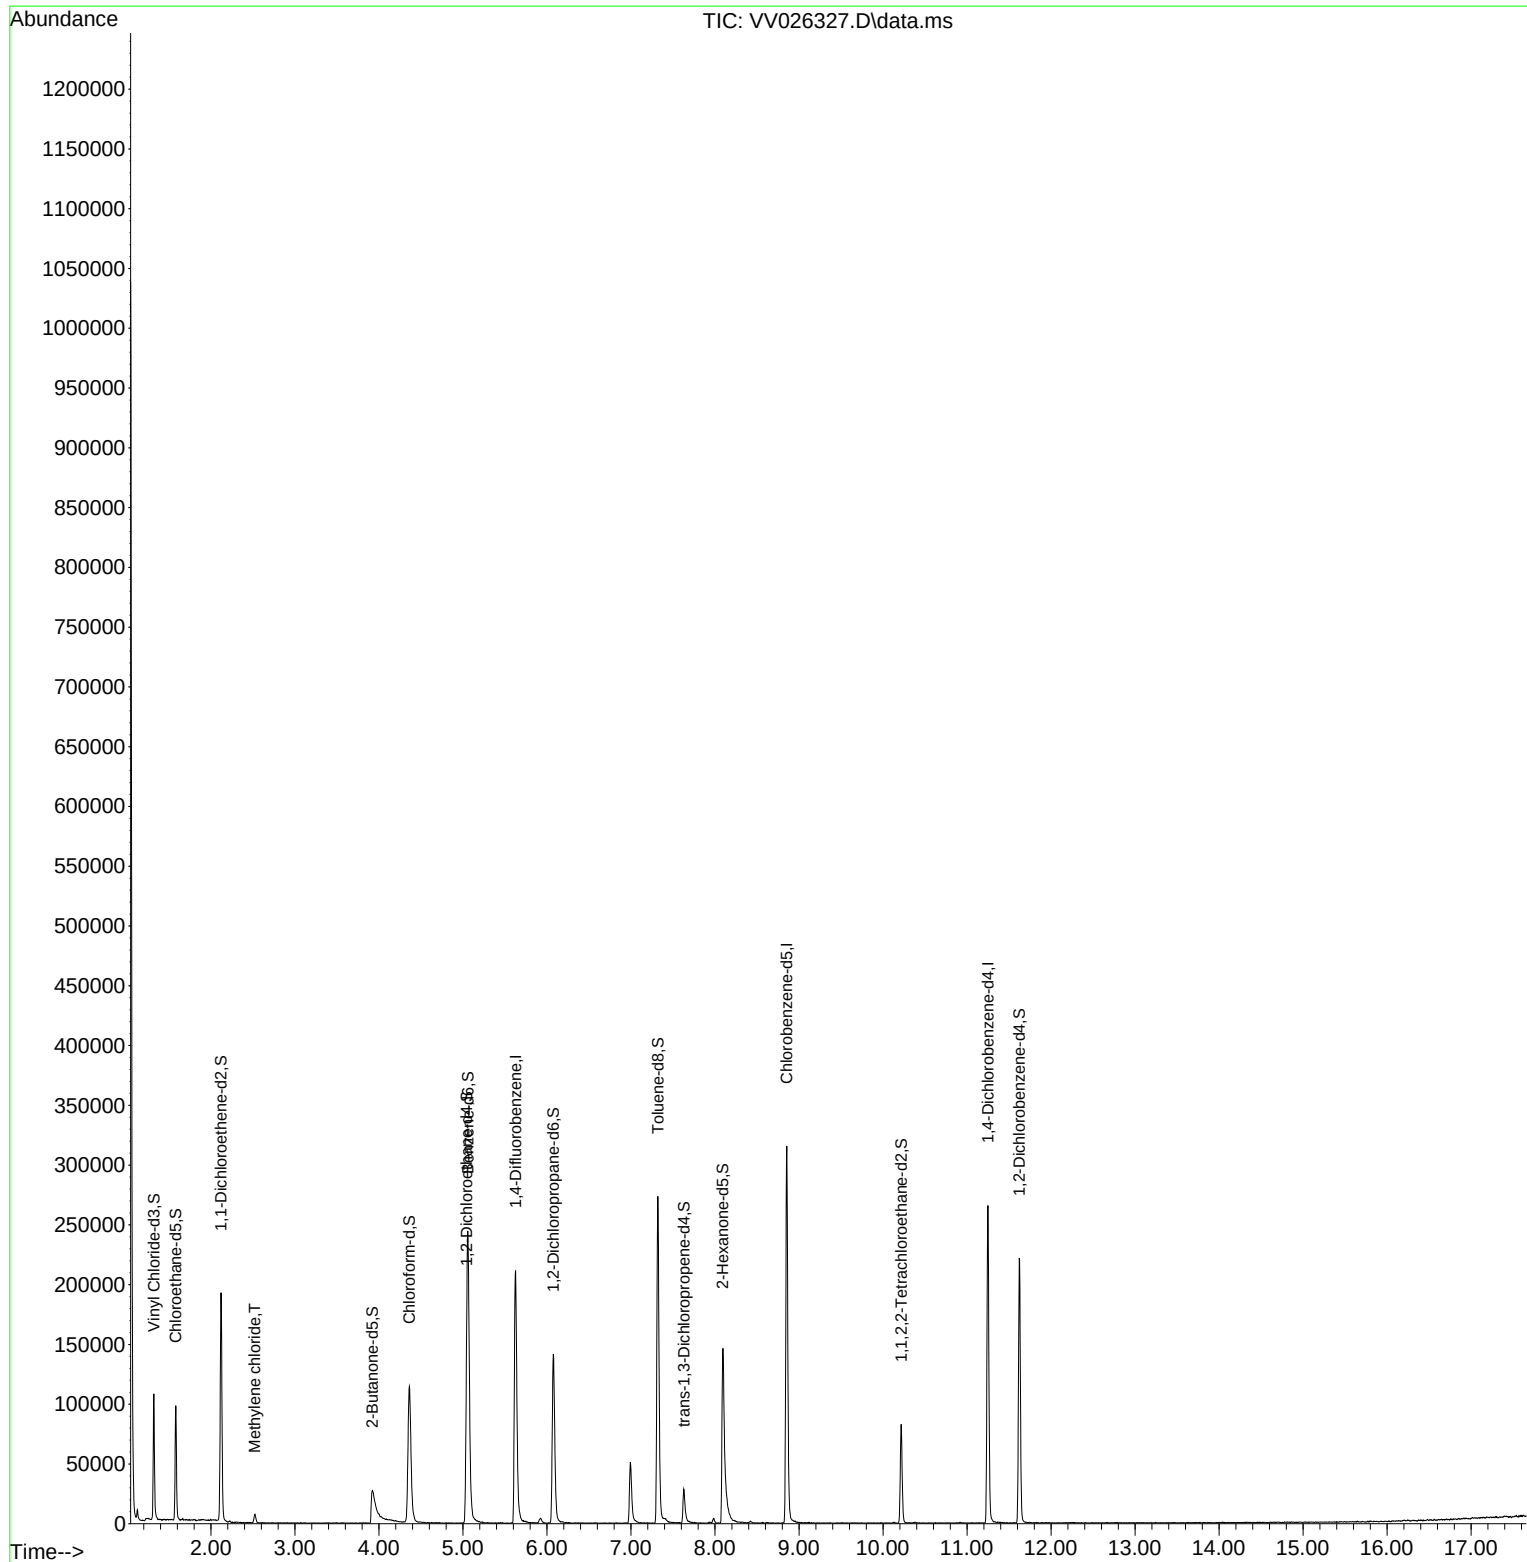

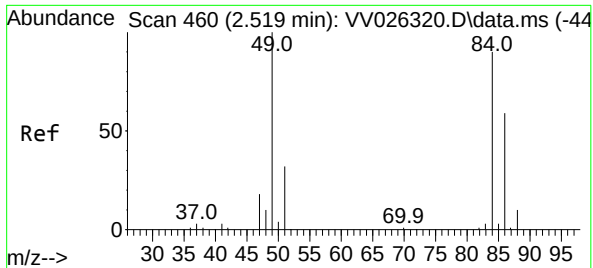

#16
Methylene chloride
Concen: 0.218 ug/L
RT: 2.519 min Scan# 4
Delta R.T. 0.000 min
Lab File: VV026327.D
Acq: 16 Jun 2022 12:35

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

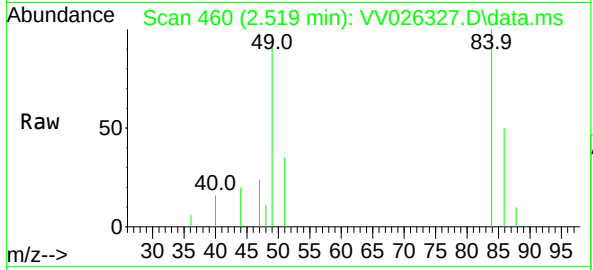

Tgt Ion:	84	Resp:	3316
Ion	Ratio	Lower	Upper
84	100		
86	49.9	44.0	81.8
49	96.5	77.3	143.7

