

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW061622\
 Data File : VW026364.D
 Acq On : 17 Jun 2022 04:03
 Operator : SY/MD
 Sample : N3318-06 10X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGJ60

Manual Integrations
 APPROVED

Reviewed By :Krupa Patel 06/17/2022
 Supervised By :Mahesh Dadoda 06/20/2022

Quant Time: Jun 17 07:23:02 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jun 17 06:57:04 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.625	114	192791	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	184491	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	74435	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.320	65	62283	3.719	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	74.400%
7) Chloroethane-d5	1.584	69	55073	4.183	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	83.600%
11) 1,1-Dichloroethene-d2	2.121	63	89756	3.121	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	62.400%
20) 2-Butanone-d5	3.928	46	70444	43.113	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	86.220%
24) Chloroform-d	4.362	84	118614	4.833	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.600%
26) 1,2-Dichloroethane-d4	5.047	65	48309	4.652	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.000%
32) Benzene-d6	5.059	84	224697	4.556	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.200%
36) 1,2-Dichloropropane-d6	6.075	67	68237	4.740	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	94.800%
41) Toluene-d8	7.320	98	177543	3.948	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	79.000%
43) trans-1,3-Dichloroprop...	7.628	79	13351	2.860	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	57.200%
46) 2-Hexanone-d5	8.095	63	54333	38.532	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	77.060%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	41364	4.664	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	93.200%
66) 1,2-Dichlorobenzene-d4	11.625	152	56475	4.926	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	98.600%
Target Compounds						
5) Vinyl chloride	1.326	62	31755	1.908	ug/L #	63
12) 1,1-Dichloroethene	2.134	96	3192	0.262	ug/L #	1
13) Acetone	2.211	43	8634m	6.819	ug/L	
16) Methylene chloride	2.526	84	4733	0.305	ug/L	98
17) Methyl tert-butyl Ether	2.793	73	1354	0.065	ug/L #	90
18) trans-1,2-Dichloroethene	2.780	96	1401	0.119	ug/L	82
19) 1,1-Dichloroethane	3.207	63	16624	0.738	ug/L	95
22) cis-1,2-Dichloroethene	3.928	96	19881	1.663	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061622\
Data File : VV026364.D
Acq On : 17 Jun 2022 04:03
Operator : SY/MD
Sample : N3318-06 10X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 48 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
BGJ60

Manual Integrations
APPROVED

Reviewed By :Krupa Patel 06/17/2022
Supervised By :Mahesh Dadoda 06/20/2022


Quant Time: Jun 17 07:23:02 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jun 17 06:57:04 2022
Response via : Initial Calibration

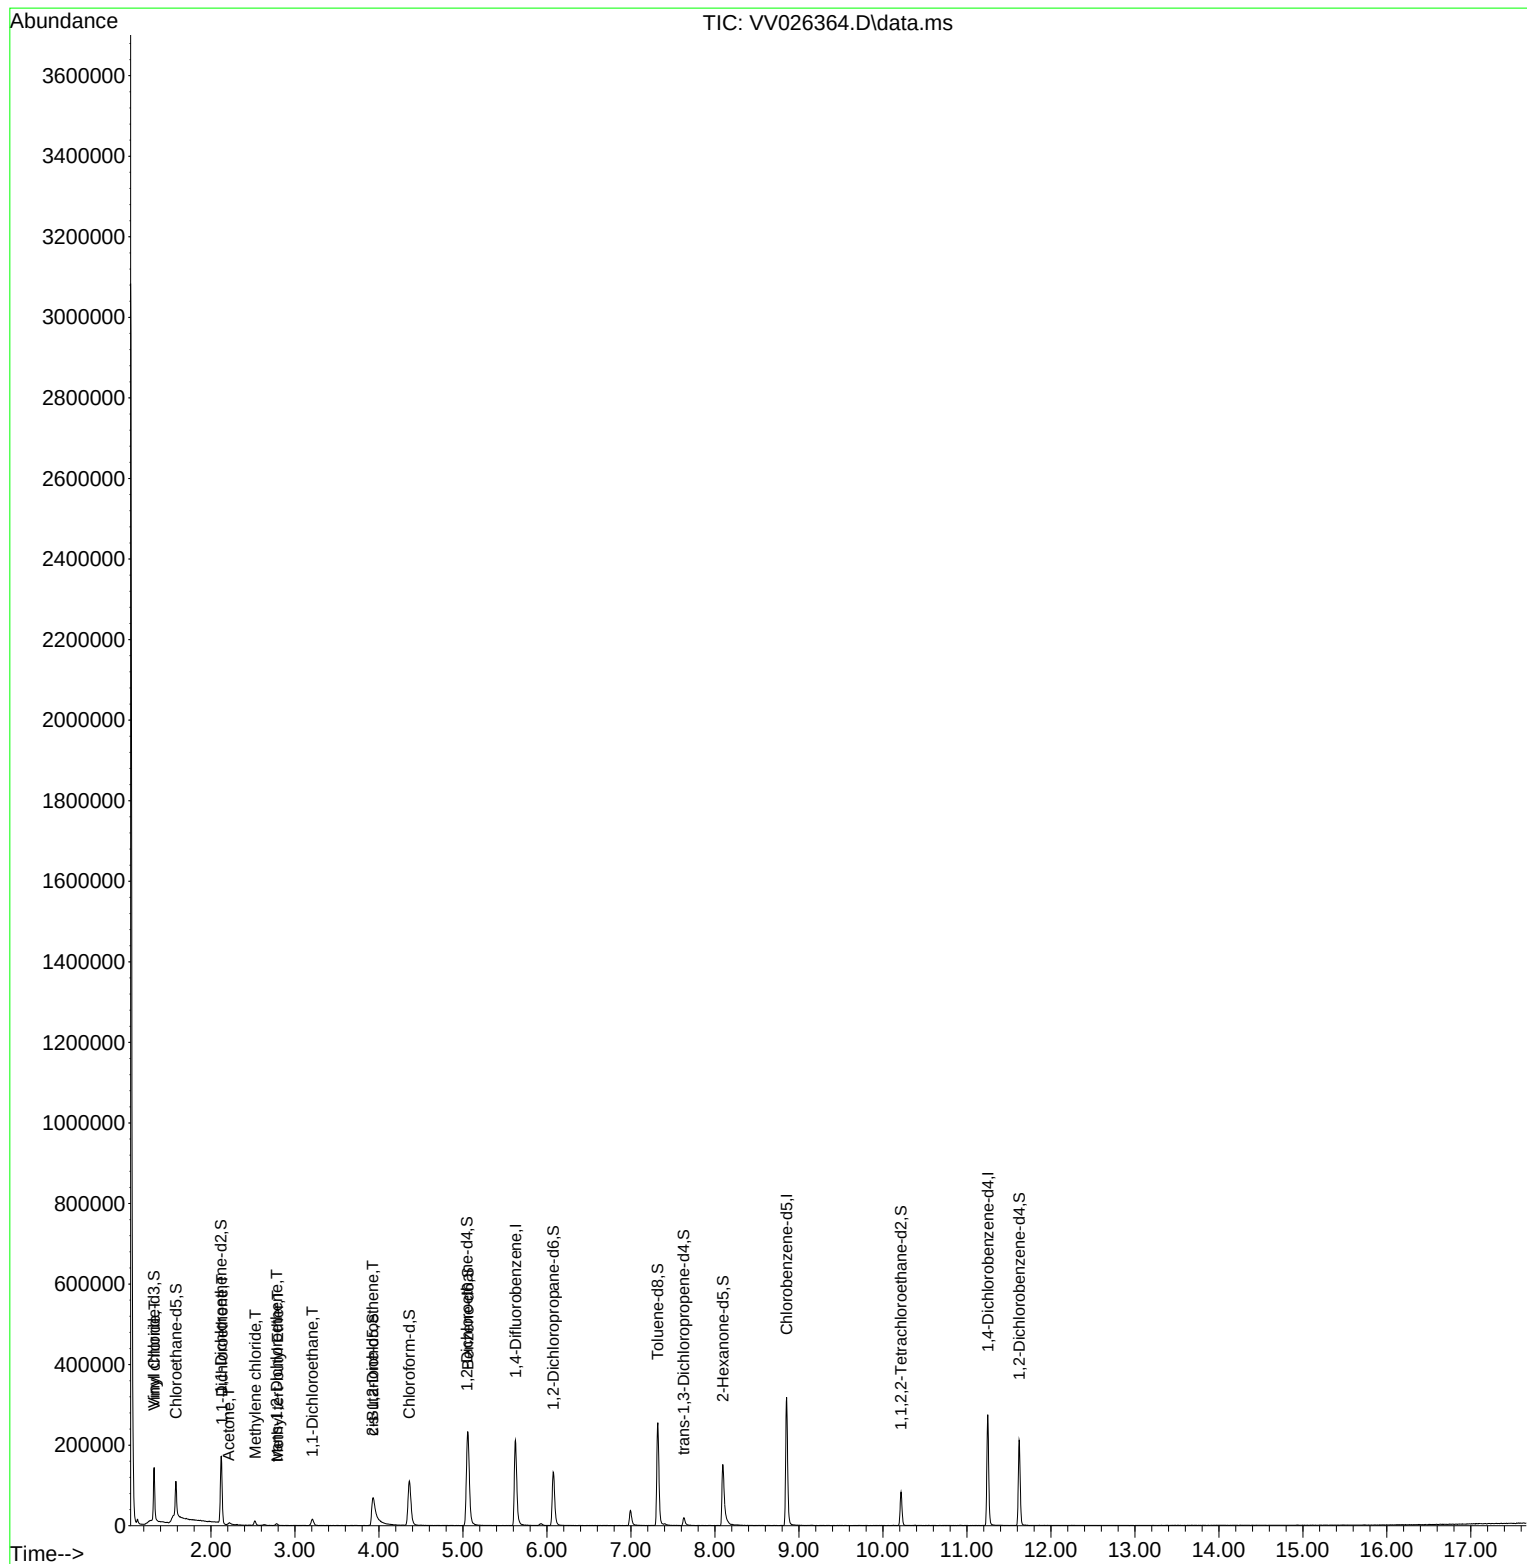

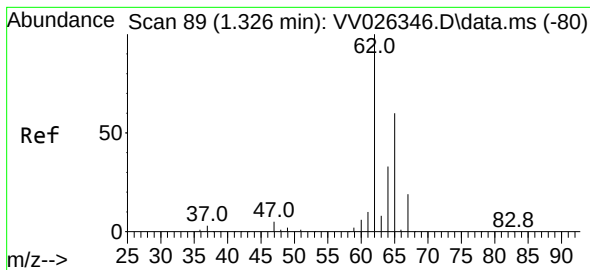

#5
 Vinyl chloride
 Concen: 1.908 ug/L
 RT: 1.326 min Scan# 89
 Delta R.T. 0.000 min
 Lab File: VV026364.D
 Acq: 17 Jun 2022 04:03




Instrument :
 MSVOA_V
 Client Sample Id :
 BGJ60

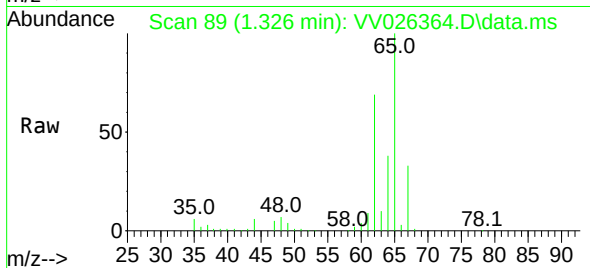

Tgt Ion: 62 Resp: 3175
 Ion Ratio Lower Upper
 62 100
 64 54.2 23.2 43.2




Manual Integrations
 APPROVED


Reviewed By :Krupa Patel 06/17/2022
 Supervised By :Mahesh Dadoda 06/20/2022

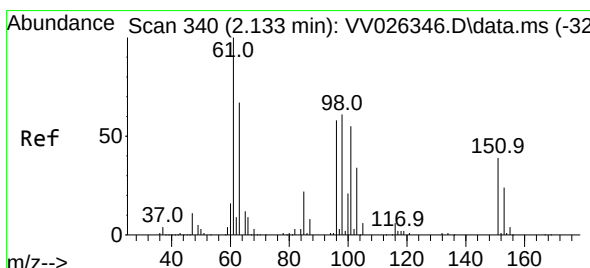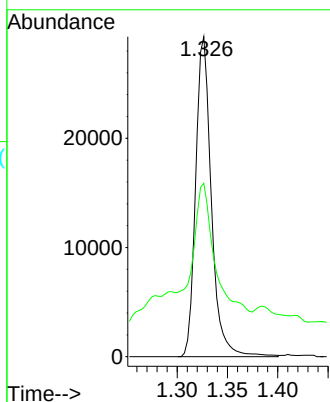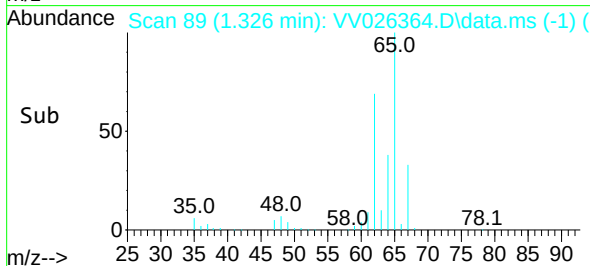

#12
 1,1-Dichloroethene
 Concen: 0.262 ug/L
 RT: 2.134 min Scan# 340
 Delta R.T. 0.000 min
 Lab File: VV026364.D
 Acq: 17 Jun 2022 04:03


Tgt Ion: 96 Resp: 3192
 Ion Ratio Lower Upper
 96 100
 61 278.3 117.1 217.5#
 63 1471.3 92.8 172.4#

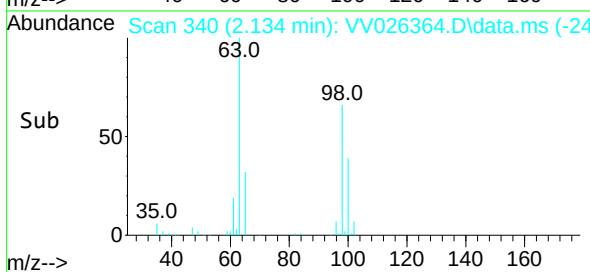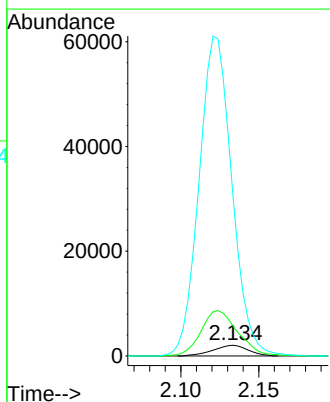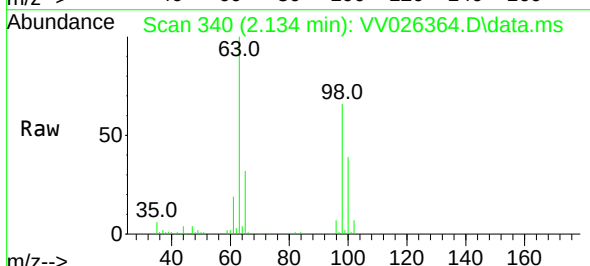

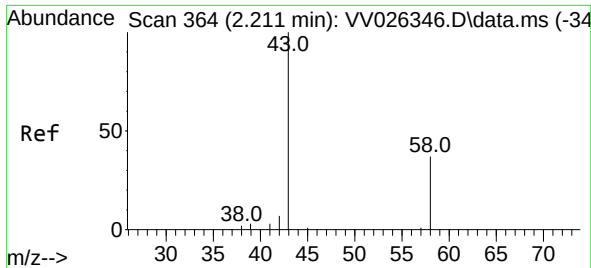

#13
Acetone
Concen: 6.819 ug/L m
RT: 2.211 min Scan# 30
Delta R.T. 0.000 min
Lab File: VV026364.D
Acq: 17 Jun 2022 04:03




Instrument :
MSVOA_V
ClientSampleId :
BGJ60

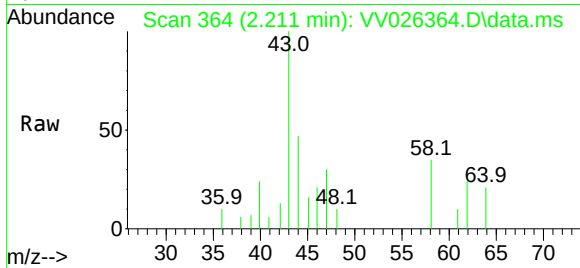


Tgt Ion: 43 Resp: 8634
Ion Ratio Lower Upper
43 100
58 17.5 0.0 60.0

Manual Integrations
APPROVED



Reviewed By :Krupa Patel 06/17/2022
Supervised By :Mahesh Dadoda 06/20/2022

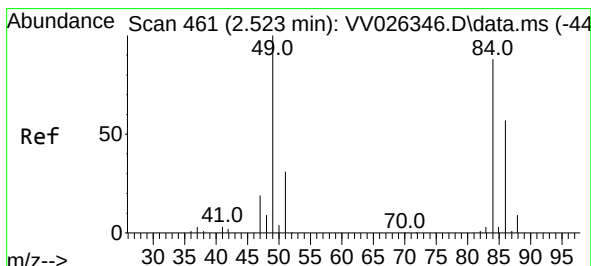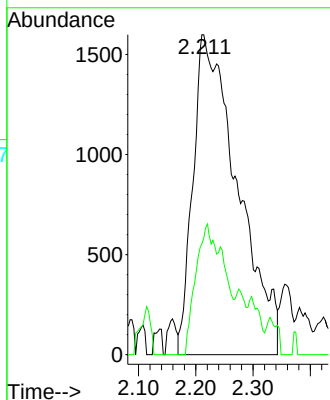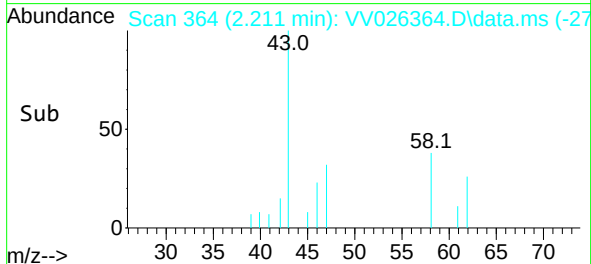


#16
Methylene chloride
Concen: 0.305 ug/L
RT: 2.526 min Scan# 462
Delta R.T. 0.003 min
Lab File: VV026364.D
Acq: 17 Jun 2022 04:03

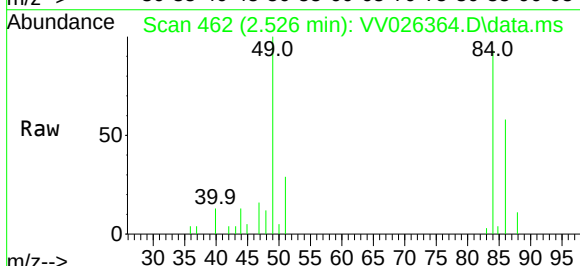

Tgt Ion: 84 Resp: 4733
Ion Ratio Lower Upper
84 100
86 62.1 44.0 81.8
49 107.3 77.3 143.7

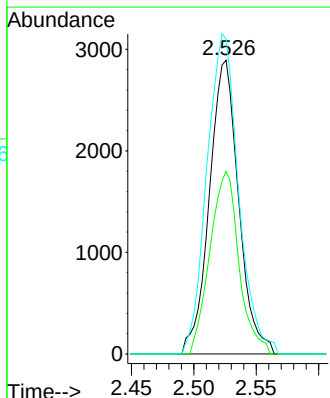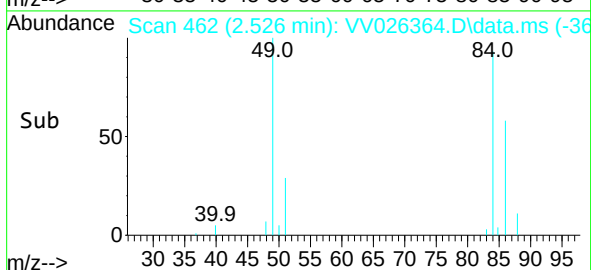

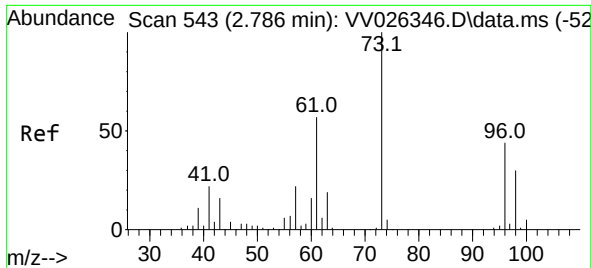





#17
Methyl tert-butyl Ether
Concen: 0.065 ug/L
RT: 2.793 min Scan# 541
Delta R.T. 0.006 min
Lab File: VV026364.D
Acq: 17 Jun 2022 04:03

Instrument :
MSVOA_V
ClientSampleId :
BGJ60

Tgt Ion: 73 Resp: 1354
Ion Ratio Lower Upper
73 100
43 26.6 13.0 19.6
57 21.9 17.6 26.4




Manual Integrations
APPROVED


Reviewed By :Krupa Patel 06/17/2022
Supervised By :Mahesh Dadoda 06/20/2022

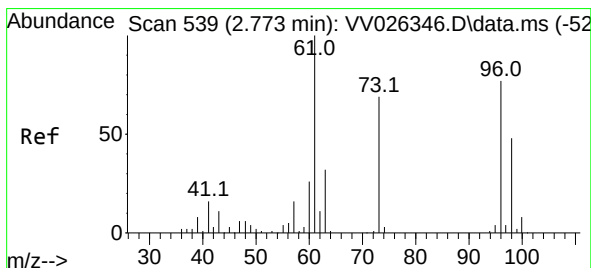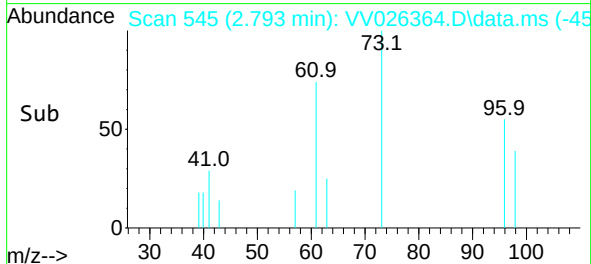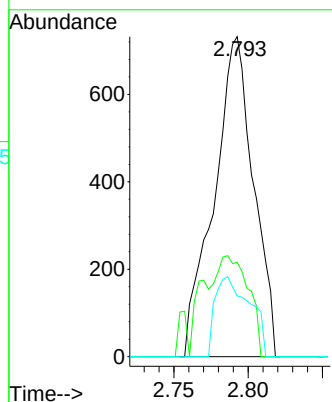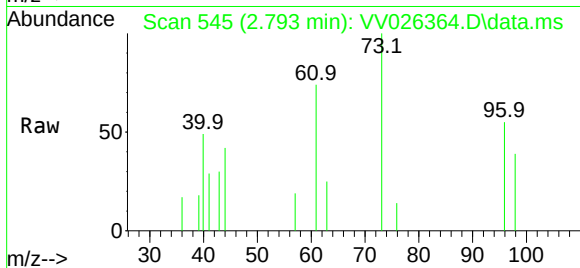

#18
trans-1,2-Dichloroethene
Concen: 0.119 ug/L
RT: 2.780 min Scan# 541
Delta R.T. 0.006 min
Lab File: VV026364.D
Acq: 17 Jun 2022 04:03

Tgt Ion: 96 Resp: 1401
Ion Ratio Lower Upper
96 100
61 107.6 91.3 169.6
98 54.3 45.3 84.1

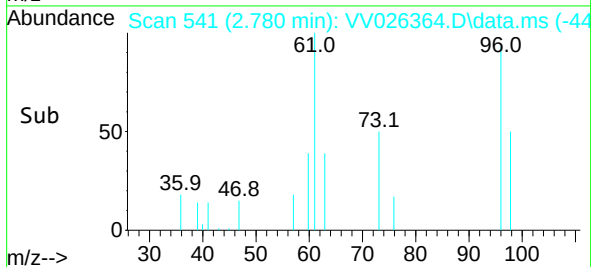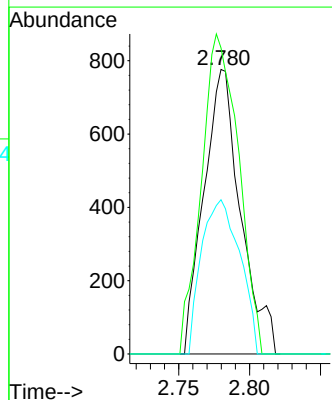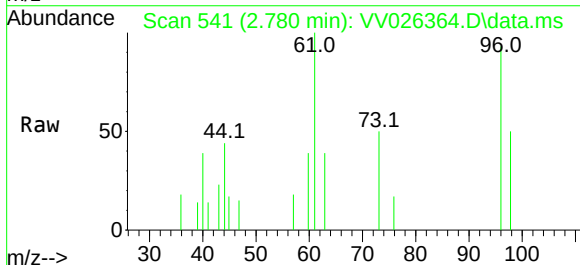

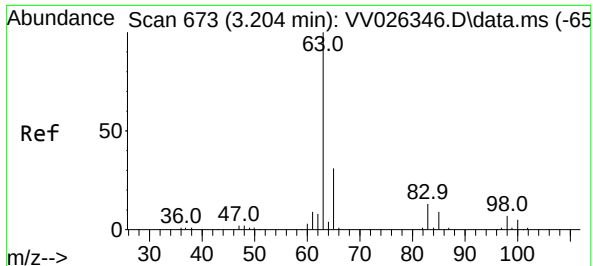





#19
1,1-Dichloroethane
Concen: 0.738 ug/L
RT: 3.207 min Scan# 61
Delta R.T. 0.003 min
Lab File: VV026364.D
Acq: 17 Jun 2022 04:03

Instrument :
MSVOA_V
ClientSampleId :
BGJ60

Tgt Ion: 63 Resp: 16624
Ion Ratio Lower Upper
63 100
65 33.7 22.3 41.3
83 15.9 8.9 16.5

Manual Integrations
APPROVED

Reviewed By :Krupa Patel 06/17/2022
Supervised By :Mahesh Dadoda 06/20/2022

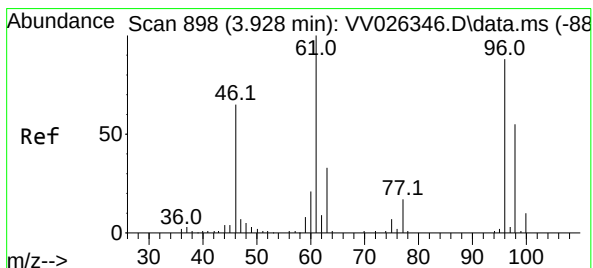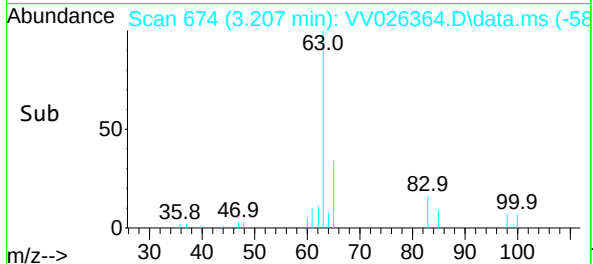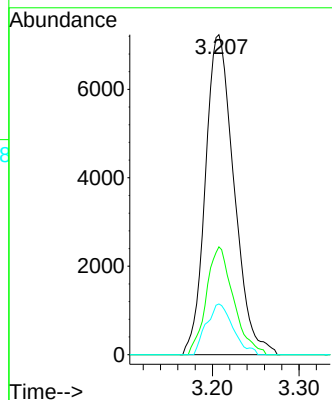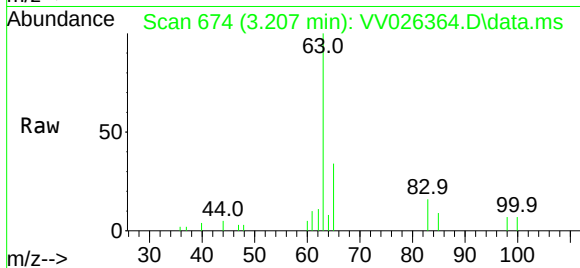

#22
cis-1,2-Dichloroethene
Concen: 1.663 ug/L
RT: 3.928 min Scan# 898
Delta R.T. 0.000 min
Lab File: VV026364.D
Acq: 17 Jun 2022 04:03

Tgt Ion: 96 Resp: 19881
Ion Ratio Lower Upper
96 100
61 118.5 83.6 155.2
68 0.0 0.0 0.0

