

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061622\
 Data File : VV026321.D
 Acq On : 16 Jun 2022 10:07
 Operator : SY/MD
 Sample : VV0616WBL01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK375

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026321.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.124	21	26	43	rVB3	9061	11142	1.61%	0.211%
2	1.320	79	87	101	rBV	129369	137134	19.83%	2.600%
3	1.580	160	168	183	rVB	109131	124837	18.06%	2.367%
4	2.121	324	336	358	rVB	223424	328234	47.47%	6.224%
5	2.523	451	461	472	rVB2	7818	13095	1.89%	0.248%
6	3.924	881	897	939	rBV2	37785	173828	25.14%	3.296%
7	4.359	1015	1032	1061	rBV	122975	312041	45.13%	5.917%
8	5.053	1232	1248	1277	rBV2	279453	691398	100.00%	13.110%
9	5.622	1413	1425	1451	rBV	217206	449650	65.03%	8.526%
10	5.918	1507	1517	1533	rVB7	5408	11923	1.72%	0.226%
11	6.072	1552	1565	1588	rBV	153013	324592	46.95%	6.155%
12	6.989	1840	1850	1874	rBV	54343	107338	15.52%	2.035%
13	7.317	1941	1952	1973	rBV	323539	563485	81.50%	10.684%
14	7.625	2039	2048	2068	rBV	30113	57227	8.28%	1.085%
15	8.091	2181	2193	2241	rBV2	181743	422481	61.11%	8.011%
16	8.850	2417	2429	2453	rBV	330885	546321	79.02%	10.359%
17	10.214	2841	2853	2871	rBV	92270	147923	21.39%	2.805%
18	11.249	3164	3175	3194	rBV	280321	443353	64.12%	8.407%
19	11.622	3277	3291	3311	rBV	259373	407886	58.99%	7.734%




Sum of corrected areas: 5273888

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061622\
Data File : VV026321.D
Acq On : 16 Jun 2022 10:07
Operator : SY/MD
Sample : VV0616WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK375

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

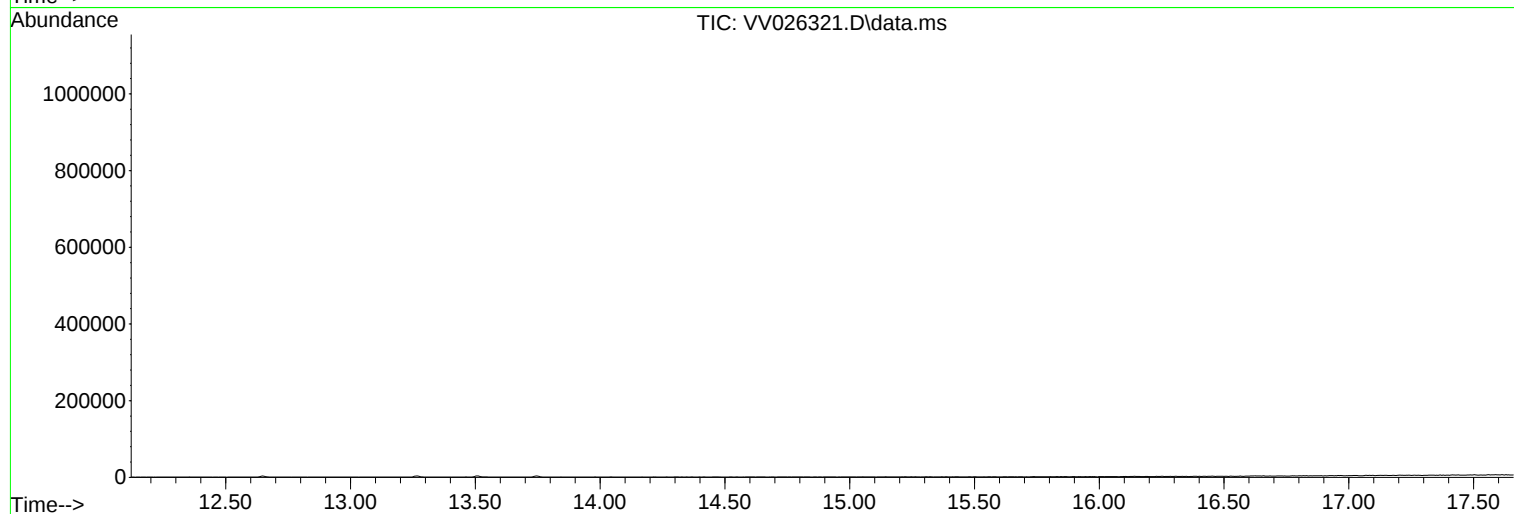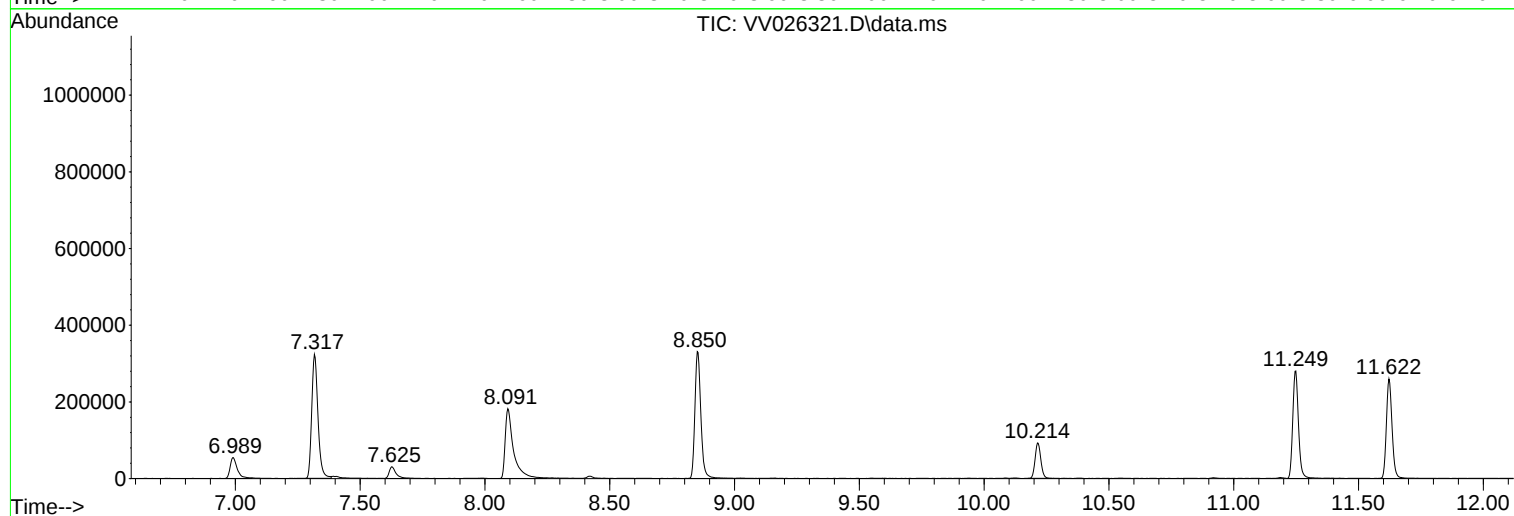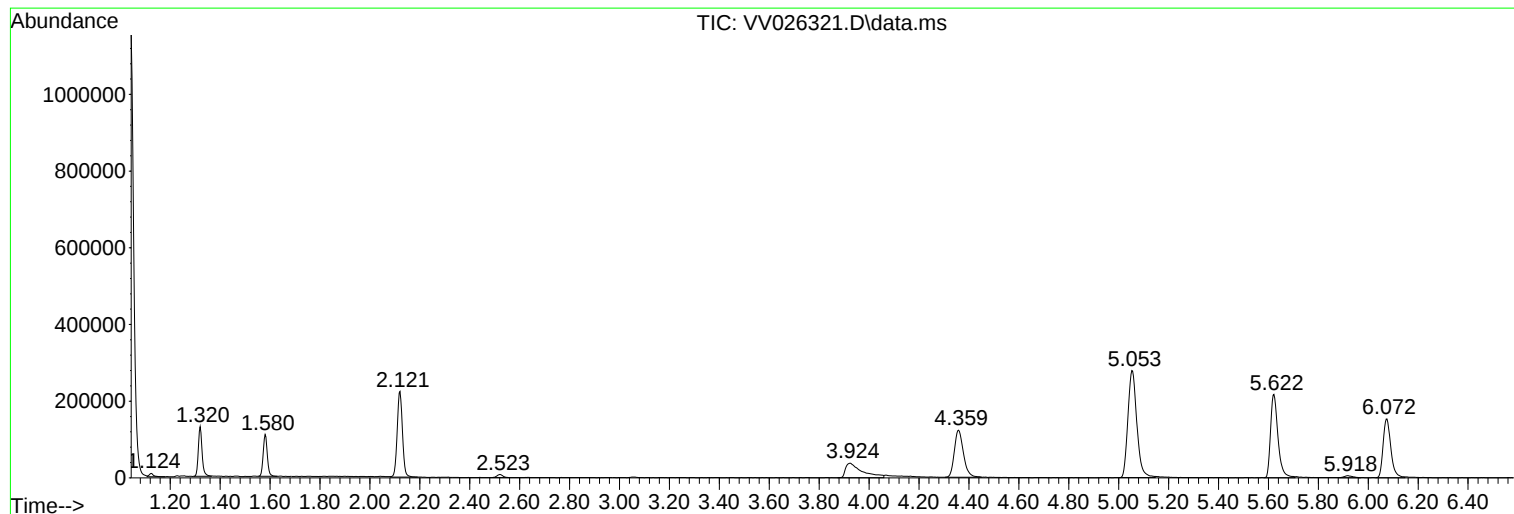

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061622\
Data File : VV026321.D
Acq On : 16 Jun 2022 10:07
Operator : SY/MD
Sample : VV0616WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK375

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061622\
Data File : VV026321.D
Acq On : 16 Jun 2022 10:07
Operator : SY/MD
Sample : VV0616WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK375

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc