

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061622\
 Data File : VV026322.D
 Acq On : 16 Jun 2022 10:36
 Operator : SY/MD
 Sample : N3273-09DL 10X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B79DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026322.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.124	21	26	42	rVB3	9494	11572	1.24%	0.180%
2	1.320	79	87	101	rBV	117404	126050	13.48%	1.959%
3	1.581	161	168	179	rBV	102974	117751	12.59%	1.830%
4	1.767	217	226	239	rVB	36858	48693	5.21%	0.757%
5	2.121	325	336	354	rVB	210525	304824	32.59%	4.736%
6	3.928	884	898	934	rBV3	32529	150355	16.07%	2.336%
7	4.359	1015	1032	1061	rBV2	123852	315491	33.73%	4.902%
8	5.056	1233	1249	1270	rBV2	274613	669103	71.53%	10.396%
9	5.622	1413	1425	1452	rBV	281761	571222	61.07%	8.876%
10	5.921	1507	1518	1537	rVB7	8924	20922	2.24%	0.325%
11	6.076	1552	1566	1593	rBV	154890	320133	34.22%	4.974%
12	6.992	1839	1851	1876	rBV	58994	115530	12.35%	1.795%
13	7.317	1941	1952	1971	rBV	309617	548051	58.59%	8.515%
14	7.625	2039	2048	2066	rBV2	31331	58893	6.30%	0.915%
15	7.976	2144	2157	2180	rBV	562567	935426	100.00%	14.534%
16	8.092	2183	2193	2230	rBV2	177489	378435	40.46%	5.880%
17	8.850	2418	2429	2450	rBV	410568	674788	72.14%	10.485%
18	10.217	2840	2854	2874	rBV	86520	139500	14.91%	2.168%
19	11.249	3164	3175	3195	rBV	350342	539017	57.62%	8.375%
20	11.622	3280	3291	3309	rBV	244144	390171	41.71%	6.062%




Sum of corrected areas: 6435927

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061622\
Data File : VV026322.D
Acq On : 16 Jun 2022 10:36
Operator : SY/MD
Sample : N3273-09DL 10X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B79DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

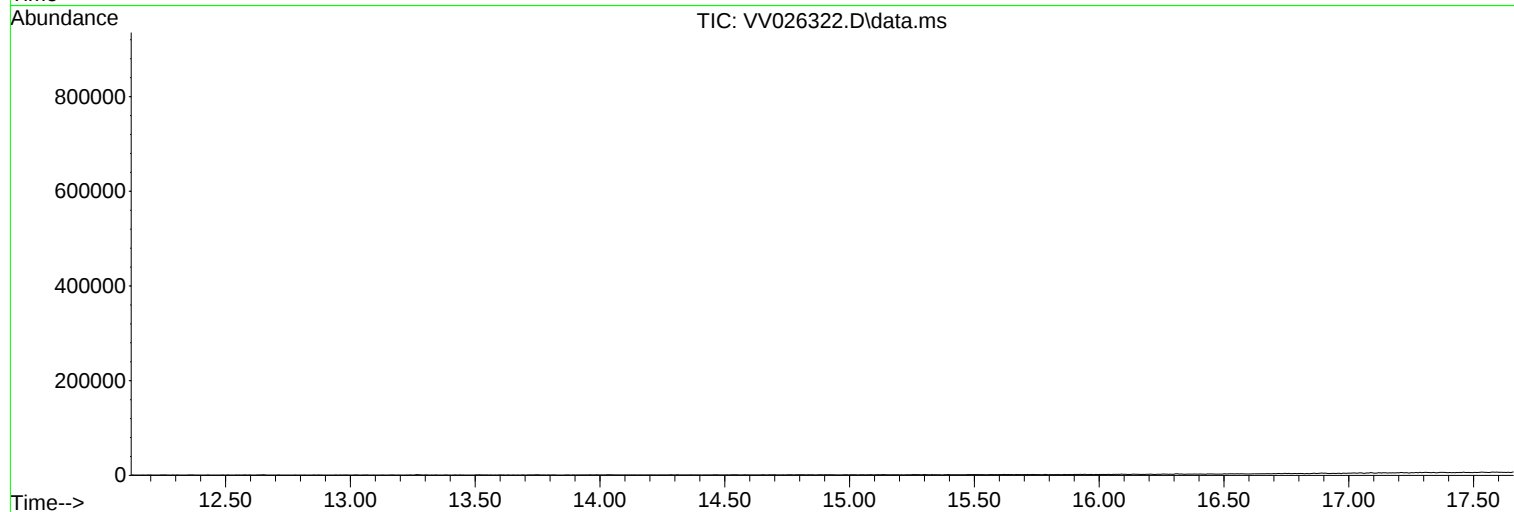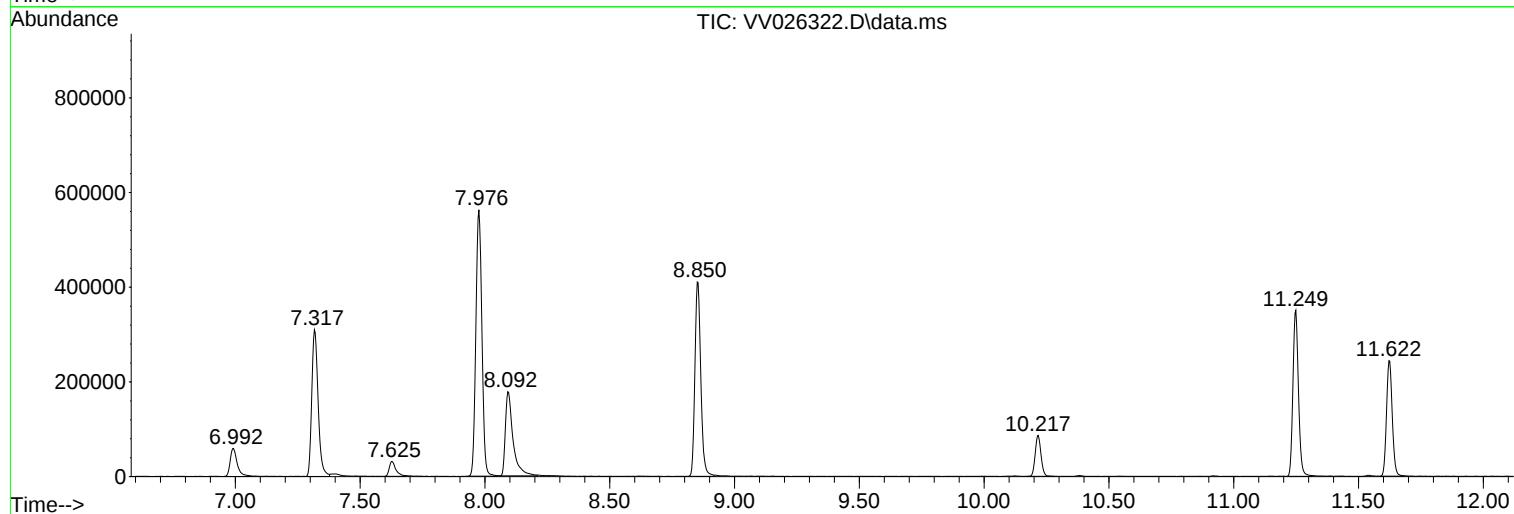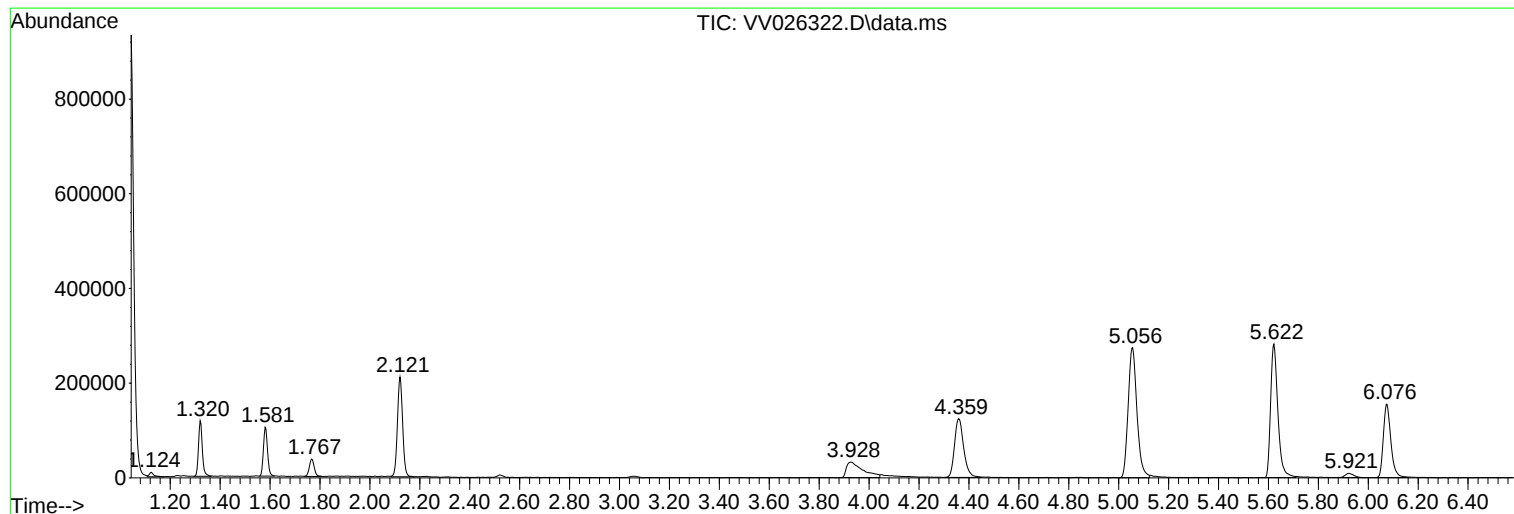

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061622\
Data File : VV026322.D
Acq On : 16 Jun 2022 10:36
Operator : SY/MD
Sample : N3273-09DL 10X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B79DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061622\
Data File : VV026322.D
Acq On : 16 Jun 2022 10:36
Operator : SY/MD
Sample : N3273-09DL 10X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B79DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc