

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061622\
 Data File : VV026323.D
 Acq On : 16 Jun 2022 11:00
 Operator : SY/MD
 Sample : N3274-09DL 10X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B99DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026323.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.124	21	26	40	rVB4	9802	11964	1.99%	0.224%
2	1.320	80	87	104	rVB	103391	110676	18.43%	2.074%
3	1.584	161	169	182	rBV	91836	105522	17.57%	1.978%
4	1.767	218	226	235	rBV	25756	32435	5.40%	0.608%
5	2.121	324	336	354	rVB	186044	271668	45.25%	5.092%
6	3.924	884	897	928	rBV3	29463	119246	19.86%	2.235%
7	4.362	1015	1033	1060	rBV	110653	281711	46.92%	5.280%
8	5.059	1230	1250	1283	rBV2	241068	600415	100.00%	11.253%
9	5.625	1411	1426	1450	rBV	215345	443013	73.78%	8.303%
10	5.921	1504	1518	1542	rBV	102066	214203	35.68%	4.015%
11	6.075	1553	1566	1593	rBV	139324	288374	48.03%	5.405%
12	6.992	1840	1851	1871	rBV	51608	99770	16.62%	1.870%
13	7.320	1938	1953	1973	rBV	268899	482906	80.43%	9.051%
14	7.628	2041	2049	2072	rBV2	27976	53945	8.98%	1.011%
15	7.976	2133	2157	2179	rBV	279465	470456	78.36%	8.817%
16	8.095	2184	2194	2227	rBV2	146350	326018	54.30%	6.110%
17	8.854	2418	2430	2452	rBV	321027	527758	87.90%	9.891%
18	10.217	2843	2854	2868	rBV	78466	125752	20.94%	2.357%
19	11.249	3162	3175	3194	rBV	271447	424473	70.70%	7.955%
20	11.622	3278	3291	3310	rBV	217448	345344	57.52%	6.472%




Sum of corrected areas: 5335649

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061622\
Data File : VV026323.D
Acq On : 16 Jun 2022 11:00
Operator : SY/MD
Sample : N3274-09DL 10X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B99DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

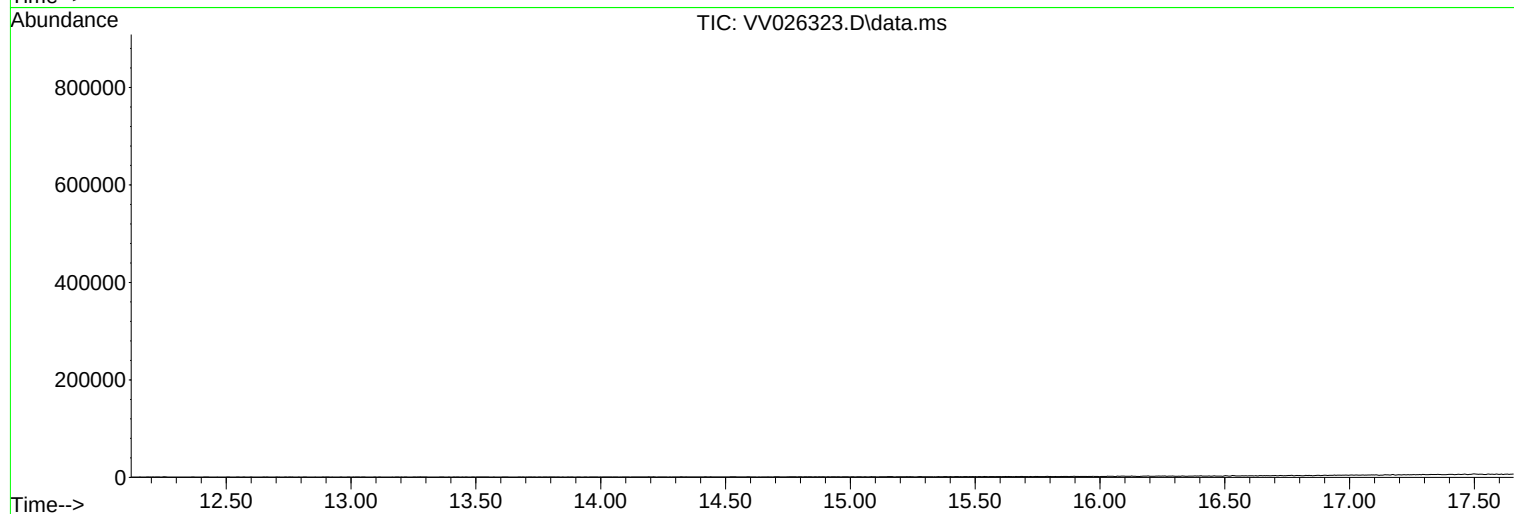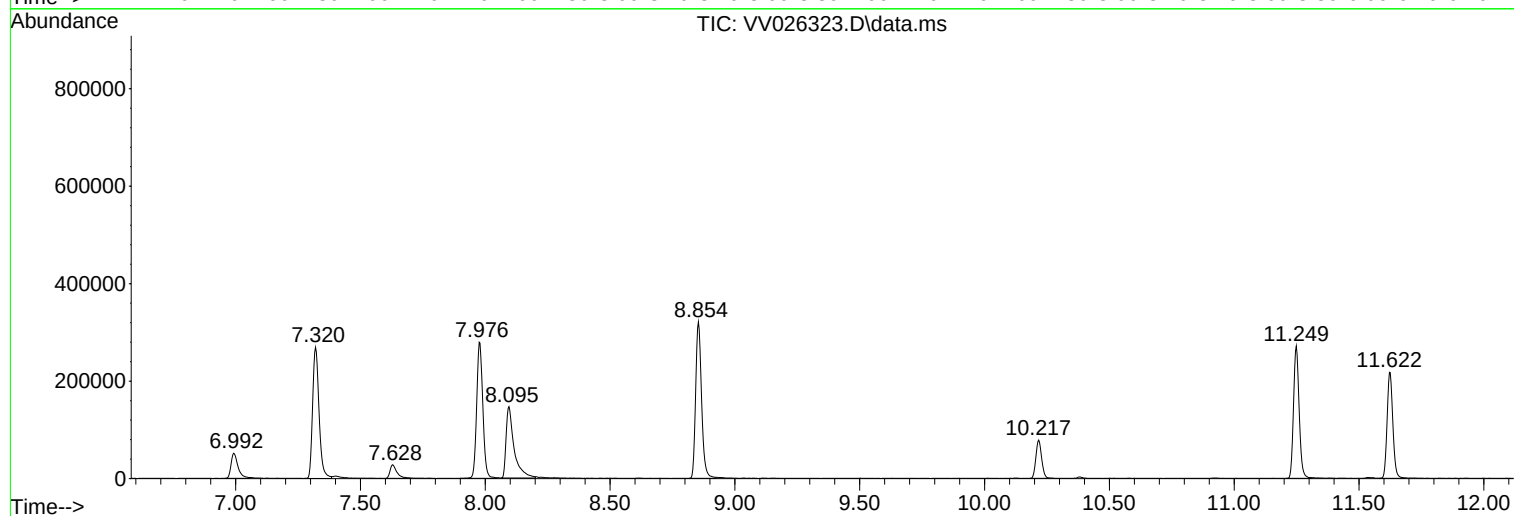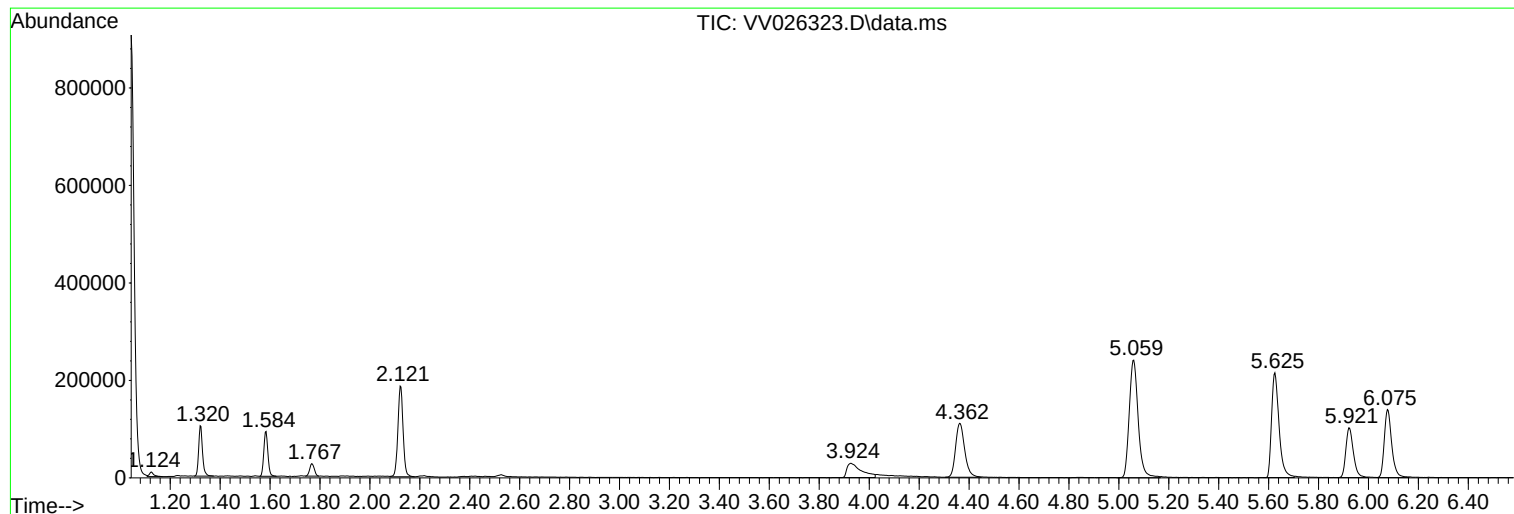

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061622\
Data File : VV026323.D
Acq On : 16 Jun 2022 11:00
Operator : SY/MD
Sample : N3274-09DL 10X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B99DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061622\
Data File : VV026323.D
Acq On : 16 Jun 2022 11:00
Operator : SY/MD
Sample : N3274-09DL 10X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B99DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc