

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061622\
 Data File : VV026324.D
 Acq On : 16 Jun 2022 11:24
 Operator : SY/MD
 Sample : N3274-10DL 10X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BA0DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026324.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.320	80	87	100	rBV	106017	112612	18.49%	2.090%
2	1.581	160	168	181	rVB	93312	108466	17.81%	2.013%
3	1.767	217	226	236	rVB	23927	31902	5.24%	0.592%
4	2.121	325	336	353	rVB	189445	276402	45.40%	5.130%
5	2.523	453	461	472	rVB4	5699	9687	1.59%	0.180%
6	3.918	885	895	923	rBV3	30357	111629	18.33%	2.072%
7	4.362	1016	1033	1057	rBV2	114371	286709	47.09%	5.322%
8	5.056	1232	1249	1279	rBV2	245713	608880	100.00%	11.302%
9	5.625	1414	1426	1450	rBV	231428	472276	77.56%	8.766%
10	5.921	1504	1518	1543	rBV2	89570	189849	31.18%	3.524%
11	6.076	1554	1566	1589	rBV	141682	291139	47.82%	5.404%
12	6.992	1841	1851	1873	rBV	53571	100848	16.56%	1.872%
13	7.320	1942	1953	1974	rBV	277068	496534	81.55%	9.216%
14	7.629	2040	2049	2066	rBV2	28456	52930	8.69%	0.982%
15	7.979	2139	2158	2179	rBV	246763	420155	69.00%	7.799%
16	8.092	2184	2193	2226	rBV2	146578	331665	54.47%	6.156%
17	8.854	2414	2430	2453	rBV	339895	562599	92.40%	10.443%
18	10.217	2842	2854	2872	rBV2	79596	128587	21.12%	2.387%
19	11.249	3163	3175	3198	rBV	286312	446651	73.36%	8.291%
20	11.622	3280	3291	3311	rBV	218888	347960	57.15%	6.459%




Sum of corrected areas: 5387480

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061622\
Data File : VV026324.D
Acq On : 16 Jun 2022 11:24
Operator : SY/MD
Sample : N3274-10DL 10X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BA0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

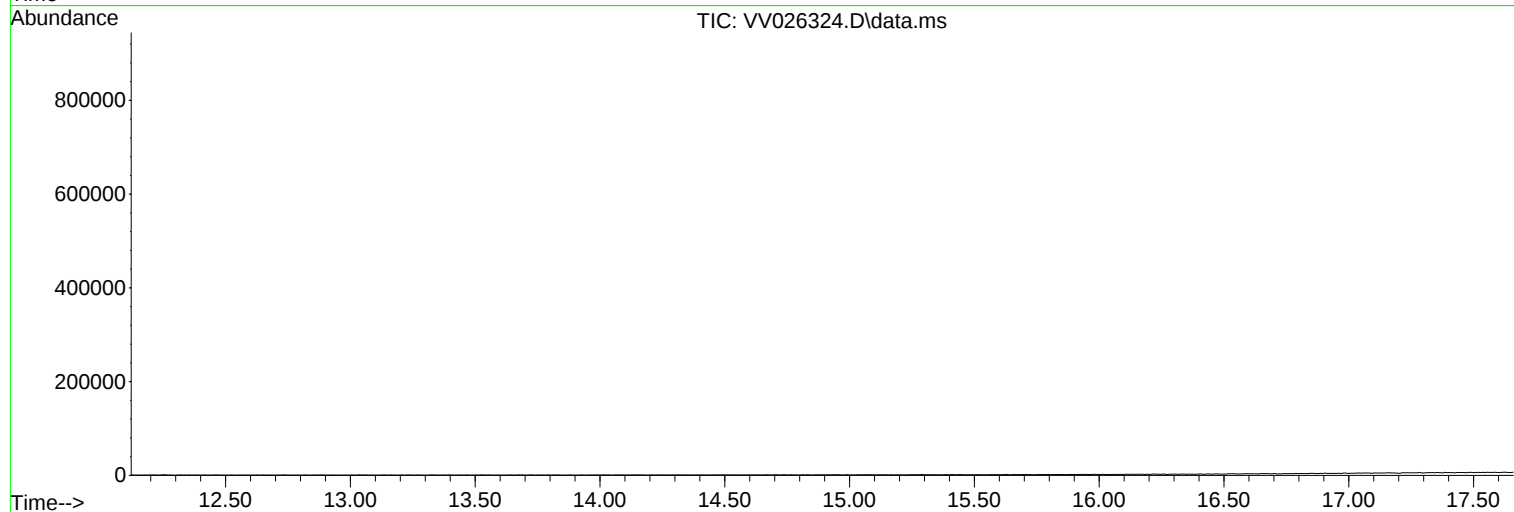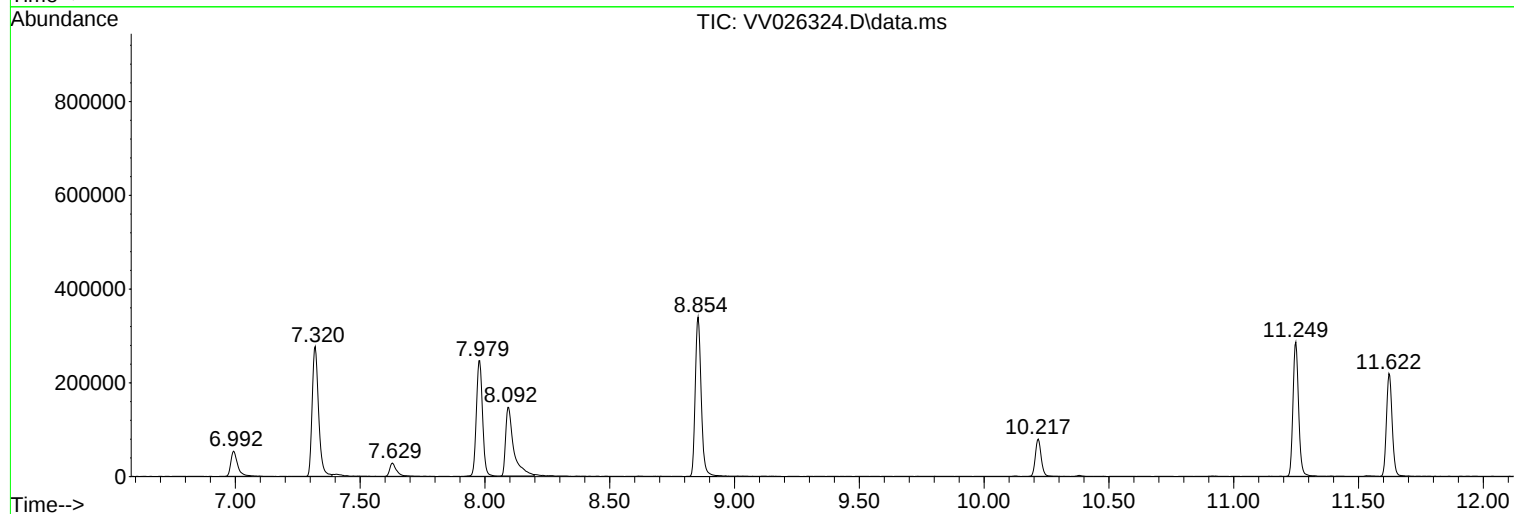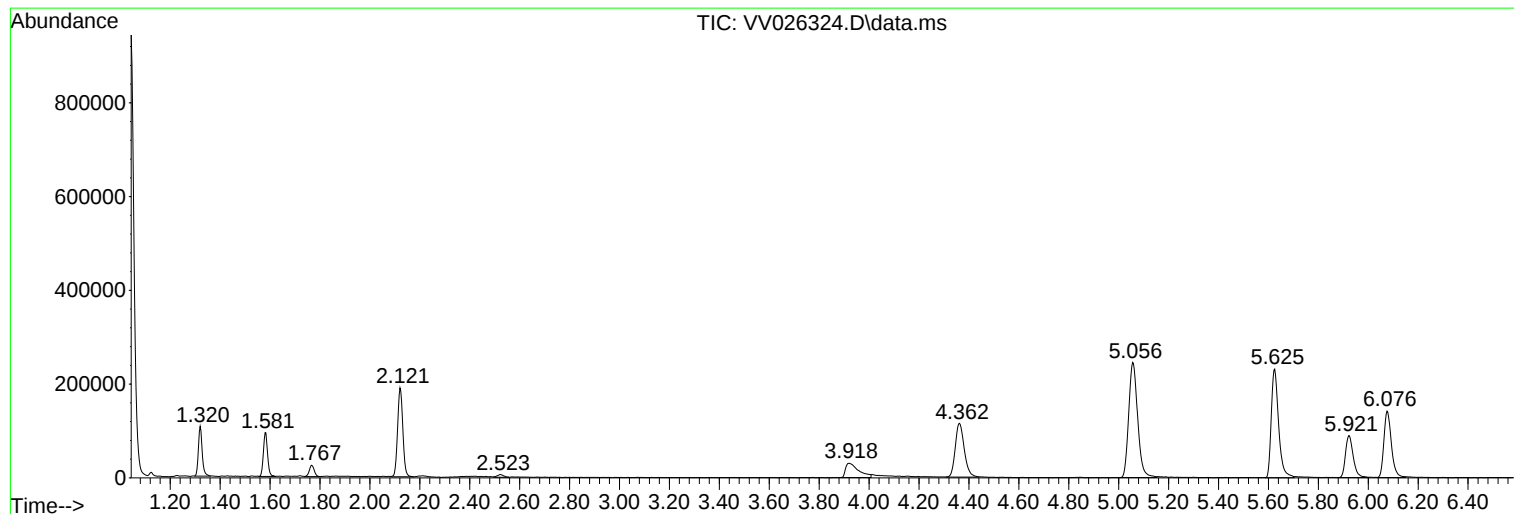

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061622\
Data File : VV026324.D
Acq On : 16 Jun 2022 11:24
Operator : SY/MD
Sample : N3274-10DL 10X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BA0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061622\
Data File : VV026324.D
Acq On : 16 Jun 2022 11:24
Operator : SY/MD
Sample : N3274-10DL 10X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BA0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc