

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061622\
 Data File : VV026326.D
 Acq On : 16 Jun 2022 12:11
 Operator : SY/MD
 Sample : N3273-16
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026326.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.320	79	87	103	rBV	105710	114923	18.83%	2.464%
2	1.580	160	168	180	rBV	96529	109541	17.95%	2.348%
3	2.121	325	336	357	rVB	191909	279979	45.88%	6.003%
4	2.519	451	460	473	rBV2	7790	13235	2.17%	0.284%
5	3.921	886	896	923	rBV2	29434	105221	17.24%	2.256%
6	4.362	1016	1033	1059	rBV	115143	284515	46.62%	6.100%
7	5.056	1233	1249	1280	rBV2	246725	610294	100.00%	13.084%
8	5.625	1414	1426	1446	rBV	213336	434453	71.19%	9.314%
9	6.075	1552	1566	1589	rBV	140143	290221	47.55%	6.222%
10	6.992	1838	1851	1876	rBV	52211	99869	16.36%	2.141%
11	7.320	1941	1953	1973	rBV	278905	486675	79.74%	10.434%
12	7.628	2039	2049	2066	rBV	29119	52020	8.52%	1.115%
13	7.982	2151	2159	2176	rVB4	14460	26332	4.31%	0.565%
14	8.095	2184	2194	2233	rBV2	150694	334273	54.77%	7.167%
15	8.853	2418	2430	2451	rBV	314813	518863	85.02%	11.124%
16	10.217	2843	2854	2871	rBV2	79478	127881	20.95%	2.742%
17	10.384	2897	2906	2920	rBV2	8590	14051	2.30%	0.301%
18	11.249	3158	3175	3198	rBV	266774	417403	68.39%	8.949%
19	11.622	3280	3291	3306	rBV	217653	344602	56.46%	7.388%




Sum of corrected areas: 4664351

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061622\
Data File : VV026326.D
Acq On : 16 Jun 2022 12:11
Operator : SY/MD
Sample : N3273-16
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

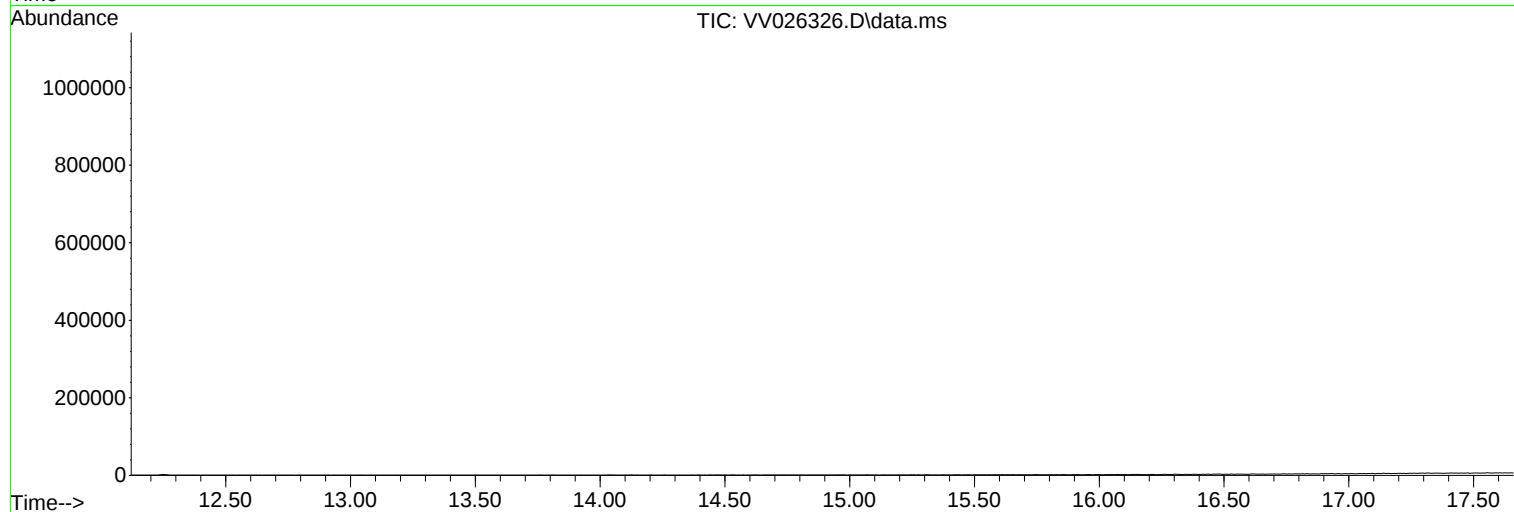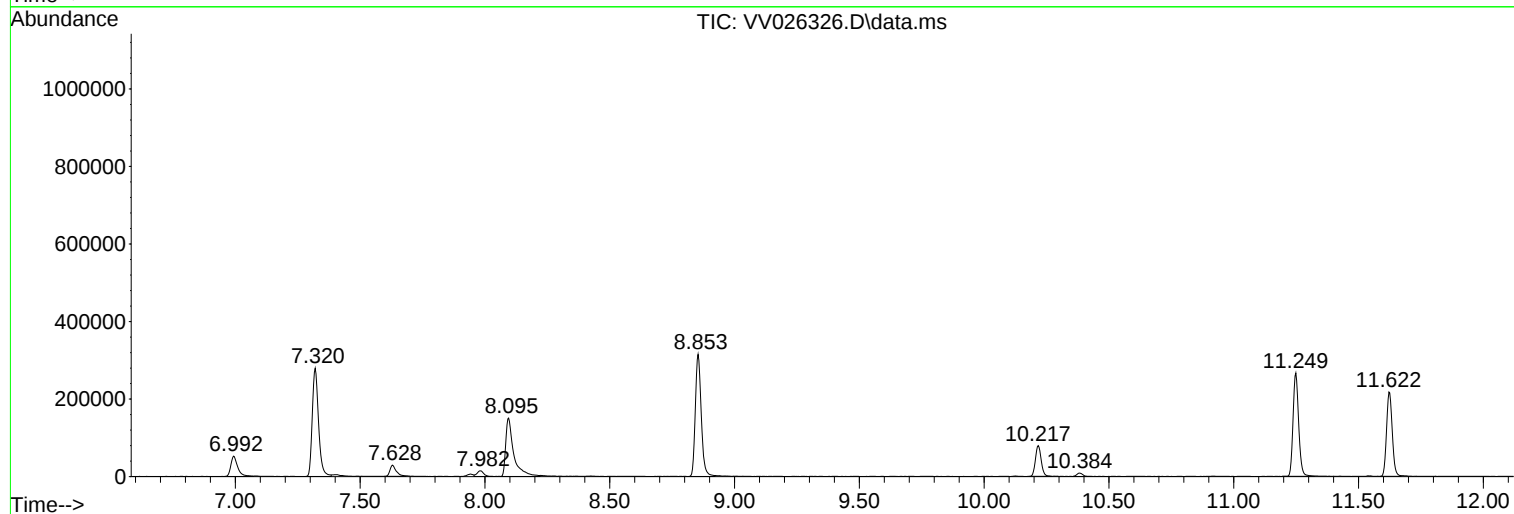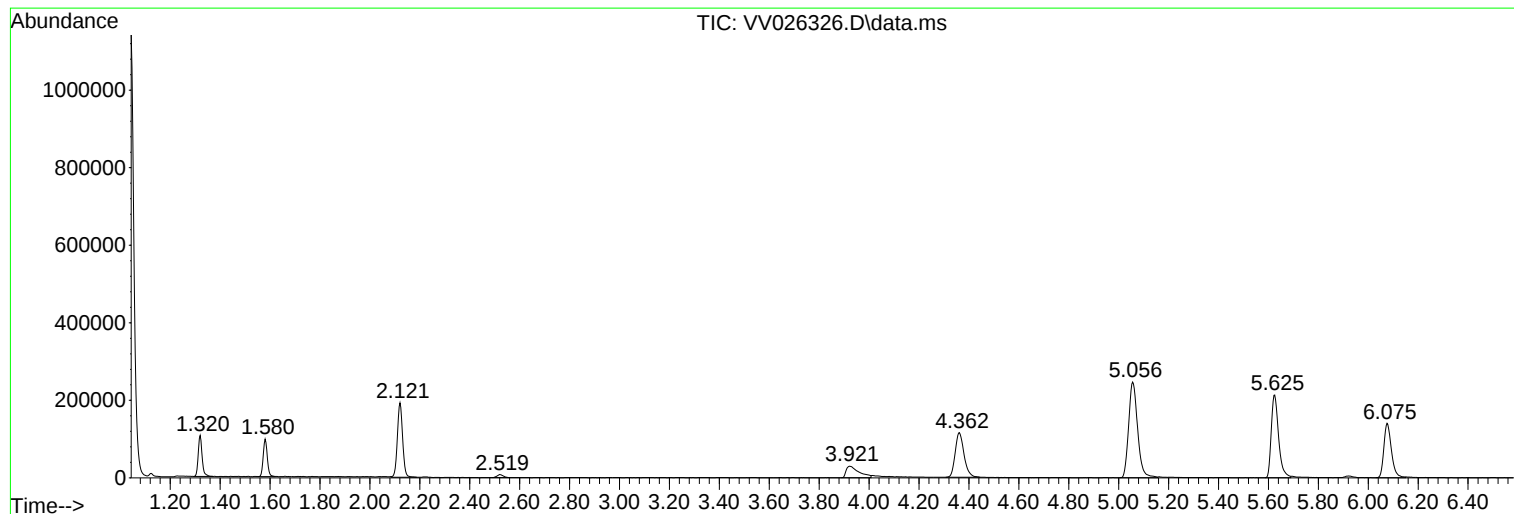

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061622\
Data File : VV026326.D
Acq On : 16 Jun 2022 12:11
Operator : SY/MD
Sample : N3273-16
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061622\
Data File : VV026326.D
Acq On : 16 Jun 2022 12:11
Operator : SY/MD
Sample : N3273-16
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
