

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061622\
 Data File : VV026328.D
 Acq On : 16 Jun 2022 12:59
 Operator : SY/MD
 Sample : N3275-01DL 5X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BC4DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026328.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.124	21	26	37	rVB4	8923	9826	1.64%	0.206%
2	1.320	79	87	96	rBV	101241	109298	18.26%	2.292%
3	1.581	159	168	181	rBV	93555	107851	18.02%	2.261%
4	2.121	324	336	351	rBV	184496	270197	45.15%	5.665%
5	2.211	351	364	399	rBV2	29408	110980	18.54%	2.327%
6	2.519	453	460	474	rVB2	11540	21069	3.52%	0.442%
7	3.921	886	896	927	rBV3	31901	128507	21.47%	2.694%
8	4.362	1015	1033	1059	rBV	113069	284135	47.47%	5.958%
9	5.056	1233	1249	1280	rBV2	244079	598494	100.00%	12.549%
10	5.622	1412	1425	1448	rBV	216599	442642	73.96%	9.281%
11	5.924	1509	1519	1535	rVB7	5374	11863	1.98%	0.249%
12	6.076	1550	1566	1593	rBV	140184	288011	48.12%	6.039%
13	6.992	1841	1851	1868	rBV2	49879	96242	16.08%	2.018%
14	7.320	1939	1953	1975	rBV	271407	479521	80.12%	10.054%
15	7.629	2041	2049	2069	rBV2	27541	50820	8.49%	1.066%
16	8.095	2180	2194	2222	rBV2	153598	331328	55.36%	6.947%
17	8.854	2419	2430	2459	rBV	326563	528973	88.38%	11.091%
18	10.217	2840	2854	2873	rBV	80040	128452	21.46%	2.693%
19	11.249	3163	3175	3195	rBV	268392	422654	70.62%	8.862%
20	11.622	3278	3291	3314	rBV	218526	348483	58.23%	7.307%




Sum of corrected areas: 4769346

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061622\
Data File : VV026328.D
Acq On : 16 Jun 2022 12:59
Operator : SY/MD
Sample : N3275-01DL 5X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BC4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

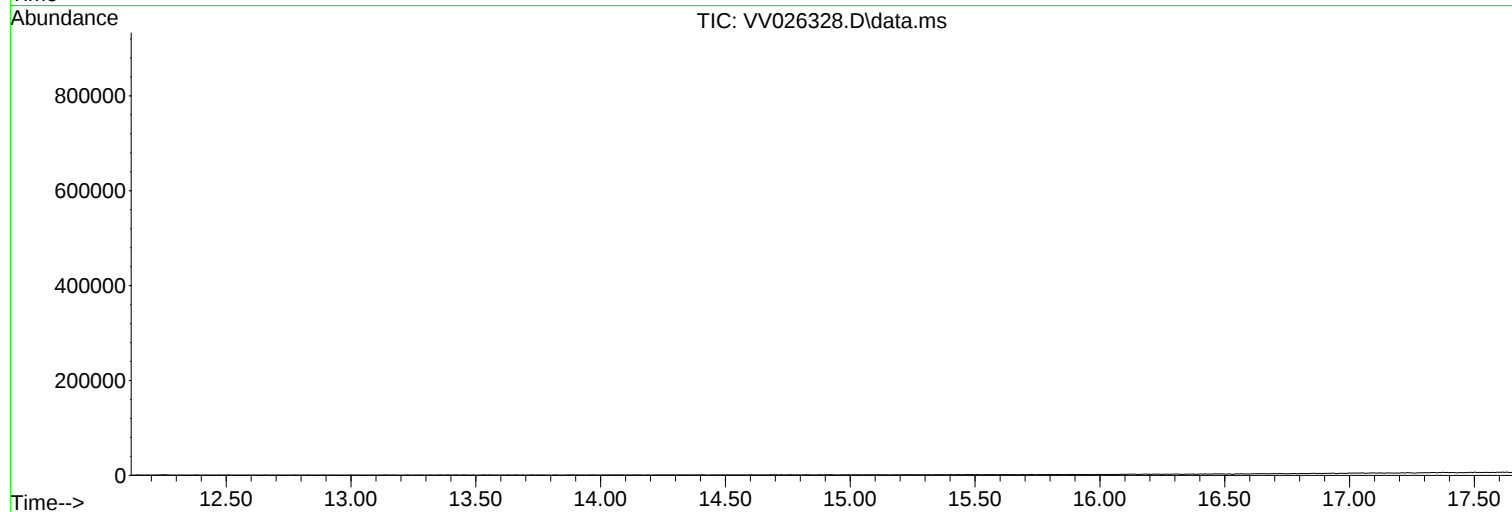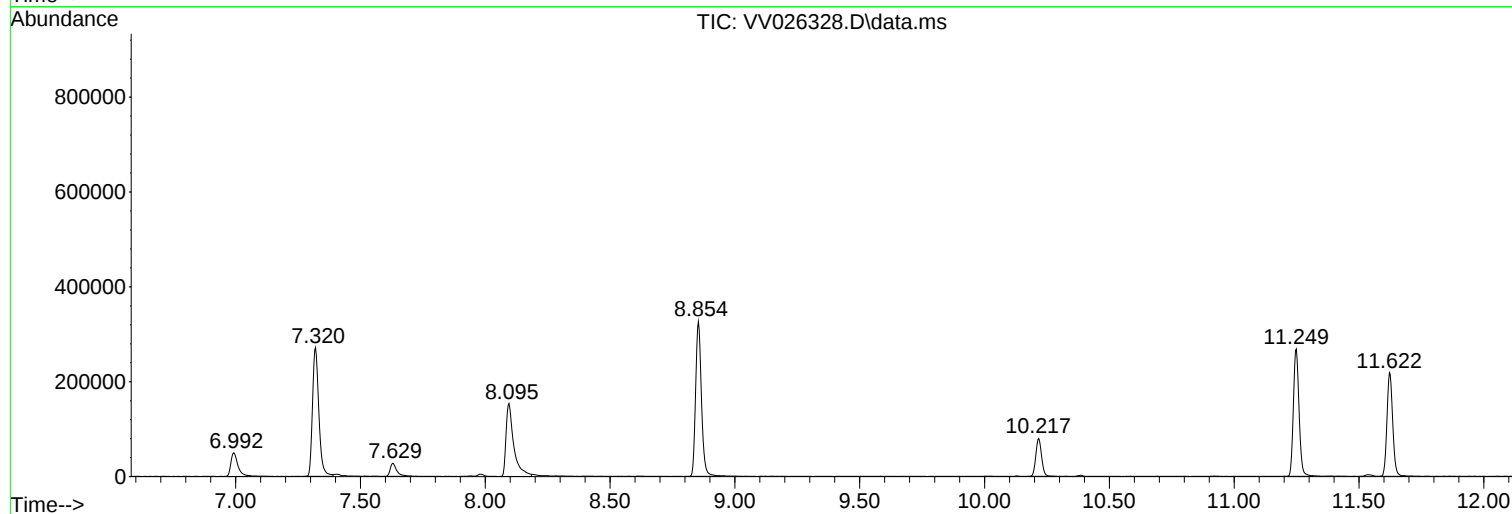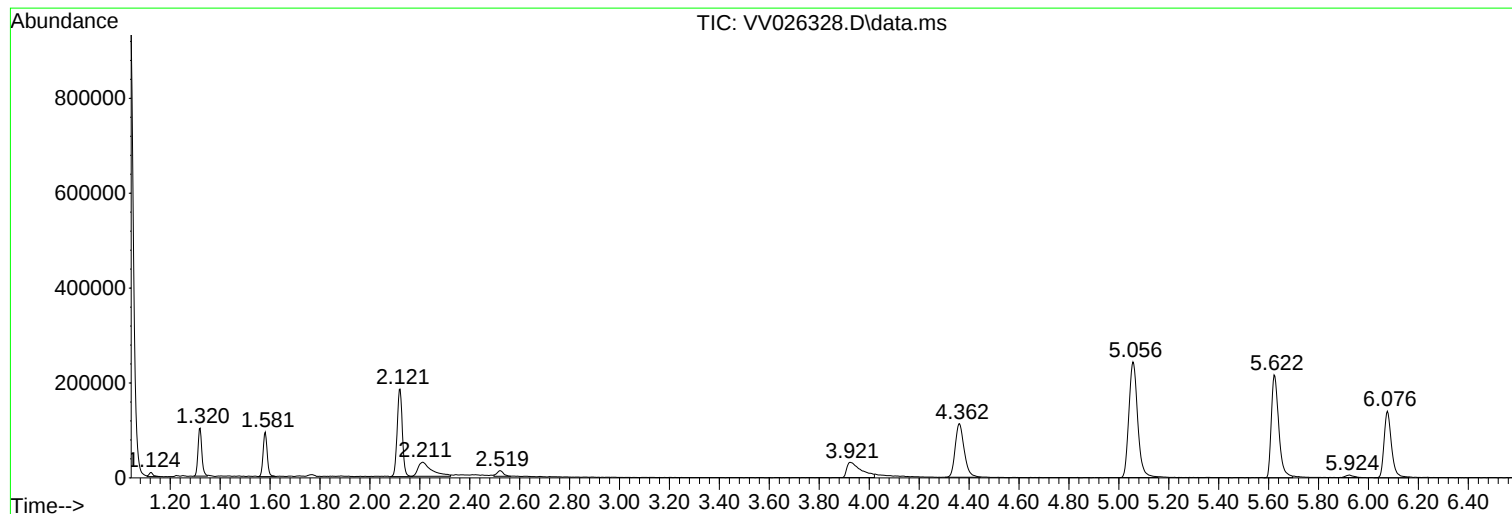

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061622\
Data File : VV026328.D
Acq On : 16 Jun 2022 12:59
Operator : SY/MD
Sample : N3275-01DL 5X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BC4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061622\
Data File : VV026328.D
Acq On : 16 Jun 2022 12:59
Operator : SY/MD
Sample : N3275-01DL 5X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BC4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
