

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061622\
 Data File : VV026331.D
 Acq On : 16 Jun 2022 14:11
 Operator : SY/MD
 Sample : N3275-03
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BD5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV026331.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.124	20	26	34	rVB2	8190	8359	1.26%	0.158%
2	1.224	51	57	67	rBV	16997	18469	2.79%	0.350%
3	1.320	80	87	101	rVB	99421	108072	16.35%	2.048%
4	1.581	159	168	182	rBV	91653	106126	16.06%	2.011%
5	1.767	219	226	234	rVB	6578	8065	1.22%	0.153%
6	2.121	325	336	352	rVB	181662	260824	39.46%	4.943%
7	2.211	353	364	384	rVB2	6043	17572	2.66%	0.333%
8	3.925	885	897	945	rBV2	32360	153587	23.24%	2.911%
9	4.362	1016	1033	1063	rBV2	108703	279185	42.24%	5.291%
10	5.056	1232	1249	1283	rBV2	240230	592845	89.70%	11.236%
11	5.622	1413	1425	1458	rBV	269000	552183	83.55%	10.466%
12	5.921	1507	1518	1545	rBV4	46692	101139	15.30%	1.917%
13	6.076	1554	1566	1596	rBV	136229	285206	43.15%	5.406%
14	6.992	1841	1851	1876	rBV2	52275	99247	15.02%	1.881%
15	7.320	1938	1953	1975	rBV	261604	468441	70.88%	8.878%
16	7.404	1975	1979	1995	rVB7	3461	7008	1.06%	0.133%
17	7.629	2039	2049	2065	rBV2	28160	52650	7.97%	0.998%
18	7.944	2134	2147	2150	rBV2	5475	8563	1.30%	0.162%
19	7.982	2152	2159	2171	rVB4	13009	23210	3.51%	0.440%
20	8.095	2184	2194	2227	rBV2	169133	363355	54.98%	6.887%
21	8.854	2416	2430	2453	rBV	406280	660910	100.00%	12.526%
22	10.008	2782	2789	2805	rBV3	3202	6704	1.01%	0.127%
23	10.217	2842	2854	2875	rBV	82429	130667	19.77%	2.477%
24	10.384	2895	2906	2915	rBV2	11267	18195	2.75%	0.345%
25	11.249	3164	3175	3194	rBV	349820	533265	80.69%	10.107%
26	11.532	3253	3263	3280	rBV2	26316	49403	7.47%	0.936%
27	11.622	3281	3291	3309	rVB	225225	362889	54.91%	6.878%




Sum of corrected areas: 5276139

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061622\
Data File : VV026331.D
Acq On : 16 Jun 2022 14:11
Operator : SY/MD
Sample : N3275-03
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BD5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

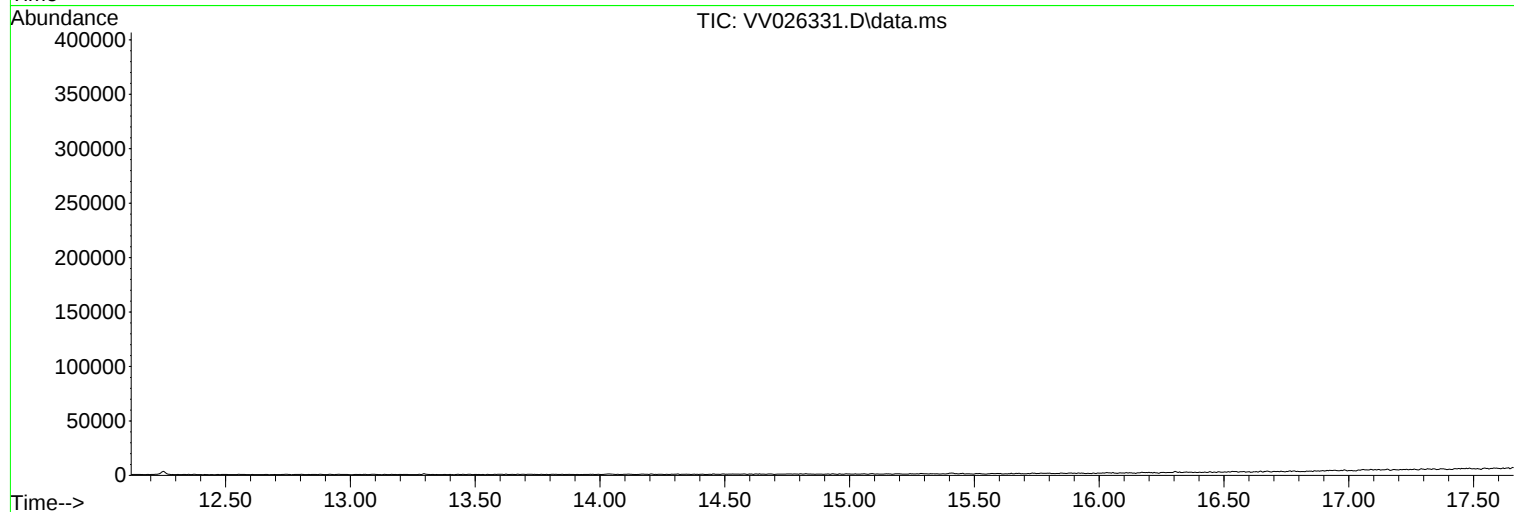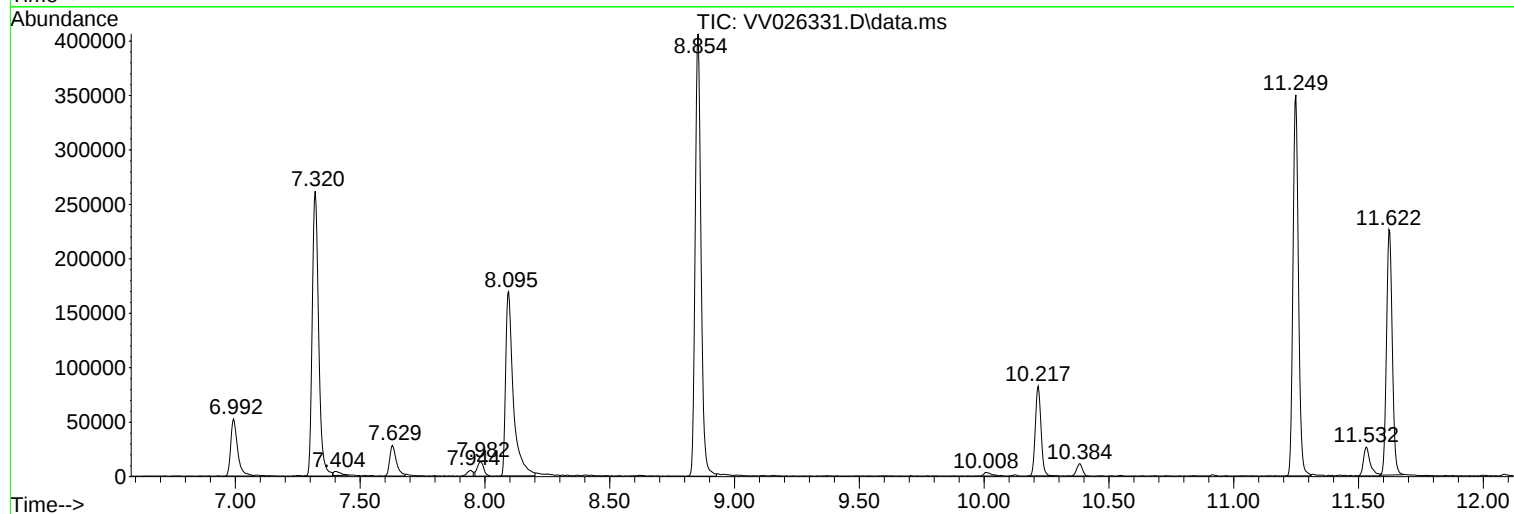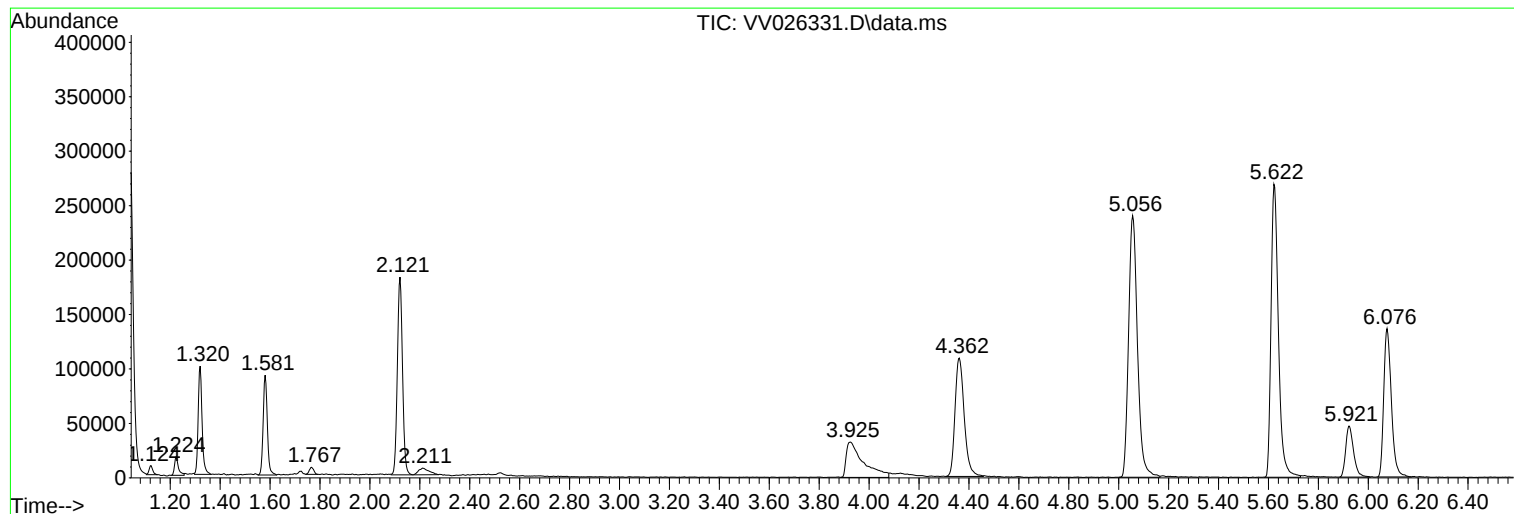

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061622\
Data File : VV026331.D
Acq On : 16 Jun 2022 14:11
Operator : SY/MD
Sample : N3275-03
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BD5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061622\
Data File : VV026331.D
Acq On : 16 Jun 2022 14:11
Operator : SY/MD
Sample : N3275-03
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BD5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc